

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034697.D
 Acq On : 20 Sep 2019 18:29
 Operator : JC/SP
 Sample : K4948-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDR3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	88	95	105	rBV	337305	360960	16.01%	2.043%
2	1.672	175	181	197	rVB	265359	339105	15.04%	1.919%
3	2.260	354	364	376	rVB	479469	726288	32.21%	4.111%
4	2.431	412	417	426	rVB2	14900	22740	1.01%	0.129%
5	2.685	491	496	500	rBV7	2951	2916	0.13%	0.017%
6	2.804	529	533	535	rBV5	1256	1015	0.05%	0.006%
7	2.817	535	537	541	rBV3	2115	1666	0.07%	0.009%
8	2.887	556	559	562	rVB5	1278	920	0.04%	0.005%
9	2.907	562	565	569	rBV6	1049	917	0.04%	0.005%
10	2.929	569	572	575	rBV3	1315	1137	0.05%	0.006%
11	3.038	603	606	609	rVB4	1610	1184	0.05%	0.007%
12	3.058	609	612	615	rBV5	1457	907	0.04%	0.005%
13	3.145	635	639	643	rBV7	1142	1054	0.05%	0.006%
14	3.238	663	668	672	rVV4	1848	2184	0.10%	0.012%
15	3.286	676	683	690	rVV7	2497	4407	0.20%	0.025%
16	3.328	693	696	699	rVB4	1459	986	0.04%	0.006%
17	3.370	704	709	711	rBV4	1088	876	0.04%	0.005%
18	3.424	719	726	730	rBV10	1008	1307	0.06%	0.007%
19	3.537	757	761	764	rBV5	1122	926	0.04%	0.005%
20	3.903	869	875	879	rBV6	1685	1816	0.08%	0.010%
21	3.990	899	902	905	rVB5	1509	1136	0.05%	0.006%
22	4.048	916	920	922	rBV3	2504	1952	0.09%	0.011%
23	4.151	941	952	990	rBV2	229738	660951	29.32%	3.741%
24	4.624	1082	1099	1125	rVV	370802	889312	39.45%	5.034%
25	5.032	1223	1226	1230	rBV5	1288	949	0.04%	0.005%
26	5.173	1267	1270	1273	rVB5	1612	1036	0.05%	0.006%
27	5.318	1291	1315	1340	rBV2	749783	2254528	100.00%	12.762%
28	5.556	1386	1389	1393	rBV5	2075	1515	0.07%	0.009%
29	5.681	1426	1428	1430	rBV3	1431	880	0.04%	0.005%
30	5.865	1472	1485	1502	rBV	641179	1272019	56.42%	7.200%
31	6.308	1608	1623	1650	rBV	526354	1080779	47.94%	6.118%
32	6.517	1686	1688	1692	rVB4	1670	925	0.04%	0.005%
33	6.649	1726	1729	1732	rBV5	1963	1392	0.06%	0.008%
34	6.672	1732	1736	1739	rVB4	1364	1030	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034697.D
 Acq On : 20 Sep 2019 18:29
 Operator : JC/SP
 Sample : K4948-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDR3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	6.820	1780	1782	1787	rVB4	1559	1005	0.04%	0.006%
36	7.144	1877	1883	1885	rBV5	1773	1613	0.07%	0.009%
37	7.205	1889	1902	1930	rBV	308256	582839	25.85%	3.299%
38	7.543	1994	2007	2028	rBV	1010882	1786150	79.23%	10.110%
39	7.829	2082	2096	2120	rBV	203159	388547	17.23%	2.199%
40	8.148	2190	2195	2196	rBV5	2583	1896	0.08%	0.011%
41	8.209	2205	2214	2228	rVB3	27902	46931	2.08%	0.266%
42	8.289	2228	2239	2288	rBV	716290	1408413	62.47%	7.972%
43	8.652	2349	2352	2354	rBV4	1427	891	0.04%	0.005%
44	8.730	2372	2376	2380	rVV6	1391	1250	0.06%	0.007%
45	8.752	2380	2383	2387	rVV3	2139	1715	0.08%	0.010%
46	8.916	2432	2434	2438	rVB4	1766	1063	0.05%	0.006%
47	8.935	2438	2440	2444	rVB4	1903	1223	0.05%	0.007%
48	8.971	2444	2451	2455	rBV8	2551	3320	0.15%	0.019%
49	9.009	2460	2463	2465	rBV4	1186	1056	0.05%	0.006%
50	9.067	2468	2481	2510	rBV	963875	1644714	72.95%	9.310%
51	9.305	2551	2555	2558	rVB6	1886	1307	0.06%	0.007%
52	9.334	2559	2564	2567	rBV7	1358	1111	0.05%	0.006%
53	9.353	2567	2570	2572	rBV4	1766	1092	0.05%	0.006%
54	9.453	2599	2601	2604	rVB3	1425	876	0.04%	0.005%
55	9.636	2656	2658	2663	rBV5	1299	937	0.04%	0.005%
56	9.723	2682	2685	2688	rBV4	1479	1198	0.05%	0.007%
57	9.832	2716	2719	2722	rVB4	1835	1229	0.05%	0.007%
58	9.887	2733	2736	2738	rBV3	1726	1273	0.06%	0.007%
59	9.990	2763	2768	2773	rBV7	1977	1708	0.08%	0.010%
60	10.025	2773	2779	2781	rBV6	1095	1172	0.05%	0.007%
61	10.122	2805	2809	2812	rBV4	1288	1192	0.05%	0.007%
62	10.205	2827	2835	2840	rBV8	2222	2855	0.13%	0.016%
63	10.257	2849	2851	2856	rVB5	1301	964	0.04%	0.005%
64	10.295	2856	2863	2865	rBV7	2140	1827	0.08%	0.010%
65	10.408	2886	2898	2919	rVV	680928	1121123	49.73%	6.346%
66	10.520	2930	2933	2937	rBV5	1189	1078	0.05%	0.006%
67	10.713	2988	2993	2994	rBV3	1350	1175	0.05%	0.007%
68	10.791	3015	3017	3022	rBV3	2125	1105	0.05%	0.006%
69	10.900	3047	3051	3053	rVB5	1263	879	0.04%	0.005%
70	10.955	3064	3068	3071	rBV6	1410	980	0.04%	0.006%
71	10.993	3077	3080	3088	rVB8	1684	1673	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034697.D
 Acq On : 20 Sep 2019 18:29
 Operator : JC/SP
 Sample : K4948-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDR3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	11.064	3097	3102	3107	rVB8	1737	1757	0.08%	0.010%
73	11.090	3107	3110	3114	rVB3	1507	930	0.04%	0.005%
74	11.135	3119	3124	3126	rBV6	2053	1854	0.08%	0.010%
75	11.308	3174	3178	3184	rVB5	1734	1761	0.08%	0.010%
76	11.337	3184	3187	3189	rBV3	1631	854	0.04%	0.005%
77	11.363	3189	3195	3199	rBV9	1272	1635	0.07%	0.009%
78	11.398	3203	3206	3208	rBV3	1778	1390	0.06%	0.008%
79	11.459	3213	3225	3245	rBV	873268	1462505	64.87%	8.278%
80	11.694	3296	3298	3303	rVB5	2221	1380	0.06%	0.008%
81	11.836	3330	3342	3365	rBV	887675	1503512	66.69%	8.510%
82	12.106	3424	3426	3431	rBV5	1818	1767	0.08%	0.010%
83	12.189	3449	3452	3456	rBV5	1331	1123	0.05%	0.006%
84	12.270	3473	3477	3480	rVB6	1890	1440	0.06%	0.008%
85	12.373	3506	3509	3517	rVB6	2605	2217	0.10%	0.013%
86	12.408	3517	3520	3523	rBV5	1832	1177	0.05%	0.007%
87	12.598	3576	3579	3582	rBV5	1981	1419	0.06%	0.008%
88	12.688	3603	3607	3610	rBV5	1884	1613	0.07%	0.009%
89	12.852	3656	3658	3664	rBV5	1443	1203	0.05%	0.007%
90	12.945	3684	3687	3691	rBV5	2529	2039	0.09%	0.012%
91	13.022	3708	3711	3716	rBV5	1433	1192	0.05%	0.007%
92	13.228	3772	3775	3777	rBV4	1597	1019	0.05%	0.006%
93	13.495	3856	3858	3860	rBV3	2058	1029	0.05%	0.006%
94	13.614	3892	3895	3899	rBV5	1995	1906	0.08%	0.011%
95	13.700	3920	3922	3927	rVB4	1486	1016	0.05%	0.006%
96	13.758	3937	3940	3941	rBV2	3008	1587	0.07%	0.009%
97	13.839	3962	3965	3968	rBV5	2119	2034	0.09%	0.012%
98	13.980	4007	4009	4012	rBV4	2602	1573	0.07%	0.009%
99	14.225	4083	4085	4092	rVB8	2329	1539	0.07%	0.009%
100	14.311	4109	4112	4113	rBV3	1816	1026	0.05%	0.006%


Sum of corrected areas: 17666592

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034697.D
Acq On : 20 Sep 2019 18:29
Operator : JC/SP
Sample : K4948-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDR3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

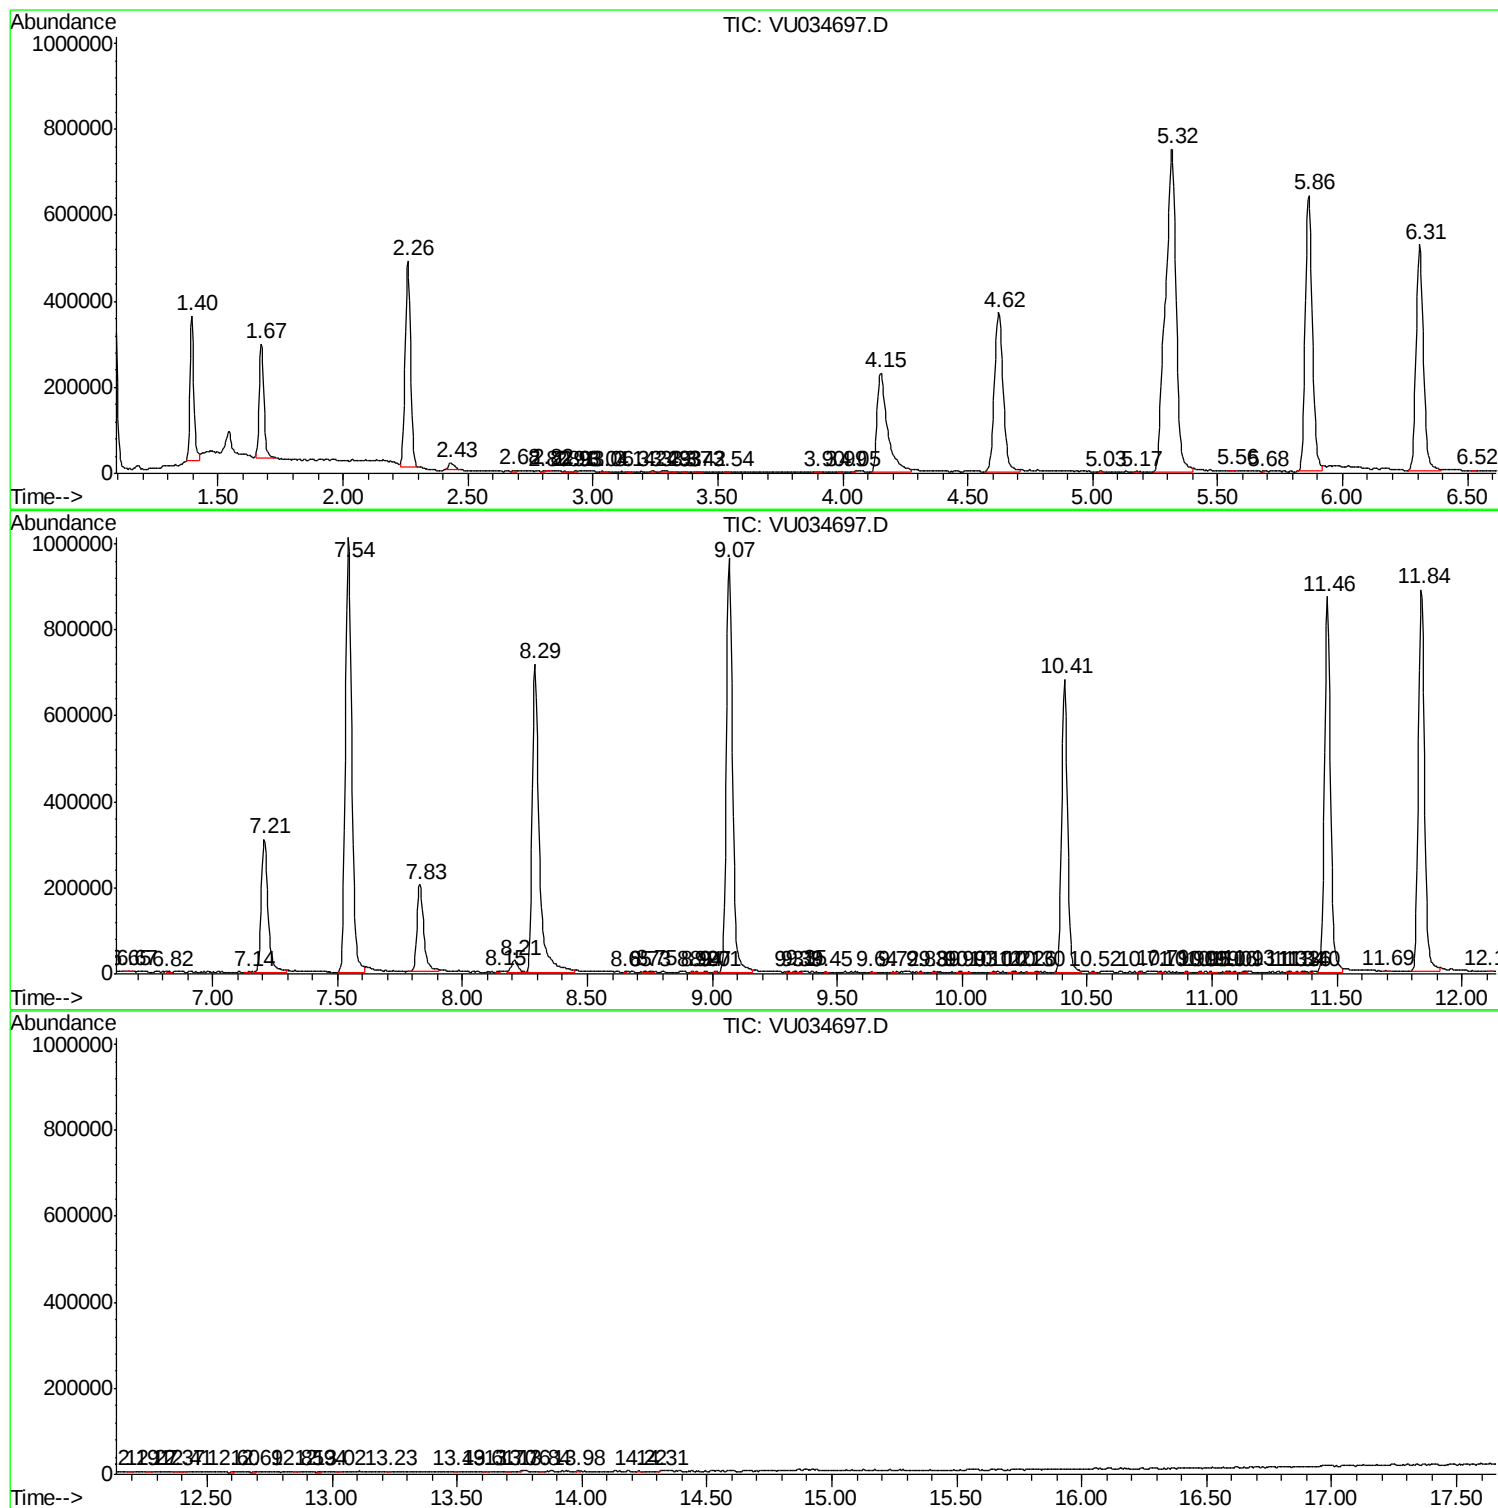

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034697.D
Acq On : 20 Sep 2019 18:29
Operator : JC/SP
Sample : K4948-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDR3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034697.D
Acq On : 20 Sep 2019 18:29
Operator : JC/SP
Sample : K4948-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDR3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc