

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034699.D
 Acq On : 20 Sep 2019 19:15
 Operator : JC/SP
 Sample : K4948-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFCX3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	21	27	35	rBV2	17131	19855	0.88%	0.114%
2	1.392	87	94	103	rBV	324389	352683	15.65%	2.030%
3	1.672	174	181	196	rVB	258542	337351	14.97%	1.941%
4	2.257	354	363	375	rVB	469212	716297	31.79%	4.122%
5	2.431	413	417	428	rVB2	10662	14009	0.62%	0.081%
6	2.543	450	452	455	rVB3	2614	1239	0.05%	0.007%
7	2.817	535	537	539	rBV3	2257	1148	0.05%	0.007%
8	2.852	545	548	551	rBV4	1767	1049	0.05%	0.006%
9	2.977	572	587	603	rBV2	30308	71297	3.16%	0.410%
10	3.087	619	621	624	rVB3	1702	864	0.04%	0.005%
11	3.174	645	648	651	rVB4	2390	1516	0.07%	0.009%
12	3.196	651	655	658	rBV4	1520	1086	0.05%	0.006%
13	3.244	668	670	674	rVB4	1484	1023	0.05%	0.006%
14	3.270	674	678	685	rVB6	1379	1310	0.06%	0.008%
15	3.367	703	708	711	rVB6	2153	1894	0.08%	0.011%
16	3.569	766	771	773	rBV6	944	918	0.04%	0.005%
17	3.707	811	814	818	rVB4	1274	890	0.04%	0.005%
18	3.813	844	847	852	rBV6	1478	923	0.04%	0.005%
19	3.858	856	861	864	rBV5	1826	1741	0.08%	0.010%
20	4.074	925	928	933	rBV6	1398	1097	0.05%	0.006%
21	4.151	935	952	981	rBV	226415	629186	27.92%	3.621%
22	4.418	1032	1035	1039	rBV4	1261	956	0.04%	0.006%
23	4.466	1048	1050	1055	rVB4	2055	1435	0.06%	0.008%
24	4.489	1055	1057	1061	rBV3	1403	1097	0.05%	0.006%
25	4.624	1082	1099	1122	rVV	360372	871463	38.67%	5.015%
26	4.846	1165	1168	1171	rBV5	1617	1146	0.05%	0.007%
27	4.948	1197	1200	1201	rVV3	1789	1037	0.05%	0.006%
28	4.968	1204	1206	1211	rVV5	2758	1734	0.08%	0.010%
29	5.000	1211	1216	1219	rVB6	2267	2119	0.09%	0.012%
30	5.048	1228	1231	1236	rVB7	1707	1714	0.08%	0.010%
31	5.077	1236	1240	1243	rBV3	1761	1703	0.08%	0.010%
32	5.125	1251	1255	1256	rBV2	1630	970	0.04%	0.006%
33	5.135	1256	1258	1261	rVB2	1536	919	0.04%	0.005%
34	5.157	1261	1265	1266	rBV3	1976	1397	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034699.D
 Acq On : 20 Sep 2019 19:15
 Operator : JC/SP
 Sample : K4948-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFCX3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	5.315	1289	1314	1342	rBV2	746747	2253497	100.00%	12.968%
36	5.730	1441	1443	1447	rVB4	1214	973	0.04%	0.006%
37	5.752	1447	1450	1454	rBV5	1627	1109	0.05%	0.006%
38	5.797	1460	1464	1466	rBV4	1295	944	0.04%	0.005%
39	5.865	1470	1485	1508	rBV	627651	1270936	56.40%	7.314%
40	6.309	1608	1623	1644	rBV	525825	1057678	46.93%	6.087%
41	6.569	1700	1704	1706	rVB2	1244	896	0.04%	0.005%
42	6.720	1746	1751	1753	rBV6	1299	1276	0.06%	0.007%
43	6.810	1773	1779	1782	rVB6	1142	1093	0.05%	0.006%
44	6.833	1782	1786	1791	rBV7	2683	2536	0.11%	0.015%
45	6.871	1796	1798	1802	rVB5	2213	1157	0.05%	0.007%
46	6.945	1818	1821	1828	rVB9	897	1009	0.04%	0.006%
47	7.206	1887	1902	1933	rBV	297535	575595	25.54%	3.312%
48	7.543	1993	2007	2026	rBV	987765	1749246	77.62%	10.066%
49	7.829	2085	2096	2119	rBV	205169	377155	16.74%	2.170%
50	8.061	2163	2168	2170	rBV4	1207	1232	0.05%	0.007%
51	8.103	2179	2181	2185	rBV5	1285	886	0.04%	0.005%
52	8.141	2189	2193	2196	rBV5	1278	1377	0.06%	0.008%
53	8.161	2196	2199	2202	rVV4	3444	2388	0.11%	0.014%
54	8.209	2206	2214	2223	rBV10	10420	15117	0.67%	0.087%
55	8.289	2228	2239	2286	rBV	707169	1378500	61.17%	7.933%
56	8.836	2407	2409	2413	rVB4	2192	1573	0.07%	0.009%
57	8.971	2449	2451	2454	rBV4	1835	1106	0.05%	0.006%
58	9.067	2468	2481	2505	rBV	945905	1615577	71.69%	9.297%
59	9.225	2527	2530	2533	rBV5	2656	2189	0.10%	0.013%
60	9.353	2565	2570	2571	rBV4	2235	1755	0.08%	0.010%
61	9.440	2593	2597	2602	rVB8	2024	1862	0.08%	0.011%
62	9.476	2602	2608	2610	rBV6	2498	2786	0.12%	0.016%
63	9.559	2631	2634	2636	rVV3	1476	987	0.04%	0.006%
64	9.649	2656	2662	2666	rBV7	1464	1747	0.08%	0.010%
65	9.755	2691	2695	2701	rBV8	2621	3118	0.14%	0.018%
66	9.839	2717	2721	2723	rBV3	2137	1414	0.06%	0.008%
67	9.890	2733	2737	2739	rVB4	1517	1136	0.05%	0.007%
68	9.926	2746	2748	2752	rVB4	1821	1164	0.05%	0.007%
69	10.006	2769	2773	2776	rVB5	1432	1067	0.05%	0.006%
70	10.038	2780	2783	2787	rVV4	1390	1320	0.06%	0.008%
71	10.080	2792	2796	2798	rBV4	1811	1159	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034699.D
 Acq On : 20 Sep 2019 19:15
 Operator : JC/SP
 Sample : K4948-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFCX3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	10.189	2825	2830	2833	rBV6	1934	1238	0.05%	0.007%
73	10.209	2833	2836	2838	rBV4	1175	905	0.04%	0.005%
74	10.408	2885	2898	2921	rBV	658978	1098230	48.73%	6.320%
75	10.588	2945	2954	2963	rBV	3424	6587	0.29%	0.038%
76	10.662	2972	2977	2979	rBV3	2086	1666	0.07%	0.010%
77	10.858	3036	3038	3041	rVV4	1366	878	0.04%	0.005%
78	10.874	3041	3043	3048	rVB5	1293	1046	0.05%	0.006%
79	11.061	3099	3101	3106	rVB4	1616	960	0.04%	0.006%
80	11.131	3115	3123	3129	rBV9	2936	4659	0.21%	0.027%
81	11.202	3142	3145	3149	rBV4	1540	1223	0.05%	0.007%
82	11.379	3197	3200	3203	rBV4	1497	1143	0.05%	0.007%
83	11.459	3213	3225	3247	rBV	845869	1407952	62.48%	8.102%
84	11.736	3309	3311	3315	rVB5	2553	1507	0.07%	0.009%
85	11.755	3315	3317	3319	rBV3	1598	1036	0.05%	0.006%
86	11.836	3330	3342	3369	rBV	857958	1448793	64.29%	8.337%
87	12.369	3505	3508	3512	rVV5	1691	1327	0.06%	0.008%
88	12.485	3542	3544	3548	rBV5	1417	1123	0.05%	0.006%
89	13.022	3707	3711	3713	rBV3	1550	1030	0.05%	0.006%
90	13.176	3756	3759	3760	rBV3	2198	1222	0.05%	0.007%
91	13.430	3836	3838	3842	rBV4	1357	1355	0.06%	0.008%
92	13.630	3897	3900	3904	rBV5	1615	1343	0.06%	0.008%
93	13.848	3965	3968	3972	rBV5	2792	2510	0.11%	0.014%
94	13.913	3986	3988	3992	rBV6	1385	1101	0.05%	0.006%
95	13.935	3992	3995	3998	rBV4	1753	1628	0.07%	0.009%
96	14.016	4016	4020	4022	rVB4	1420	1010	0.04%	0.006%
97	14.070	4033	4037	4041	rBV8	2402	1813	0.08%	0.010%
98	14.340	4119	4121	4126	rVB5	2360	1649	0.07%	0.009%
99	14.807	4264	4266	4270	rBV4	1898	911	0.04%	0.005%
100	15.044	4338	4340	4344	rBV4	2612	1798	0.08%	0.010%


Sum of corrected areas: 17377269

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034699.D
Acq On : 20 Sep 2019 19:15
Operator : JC/SP
Sample : K4948-15
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFCX3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

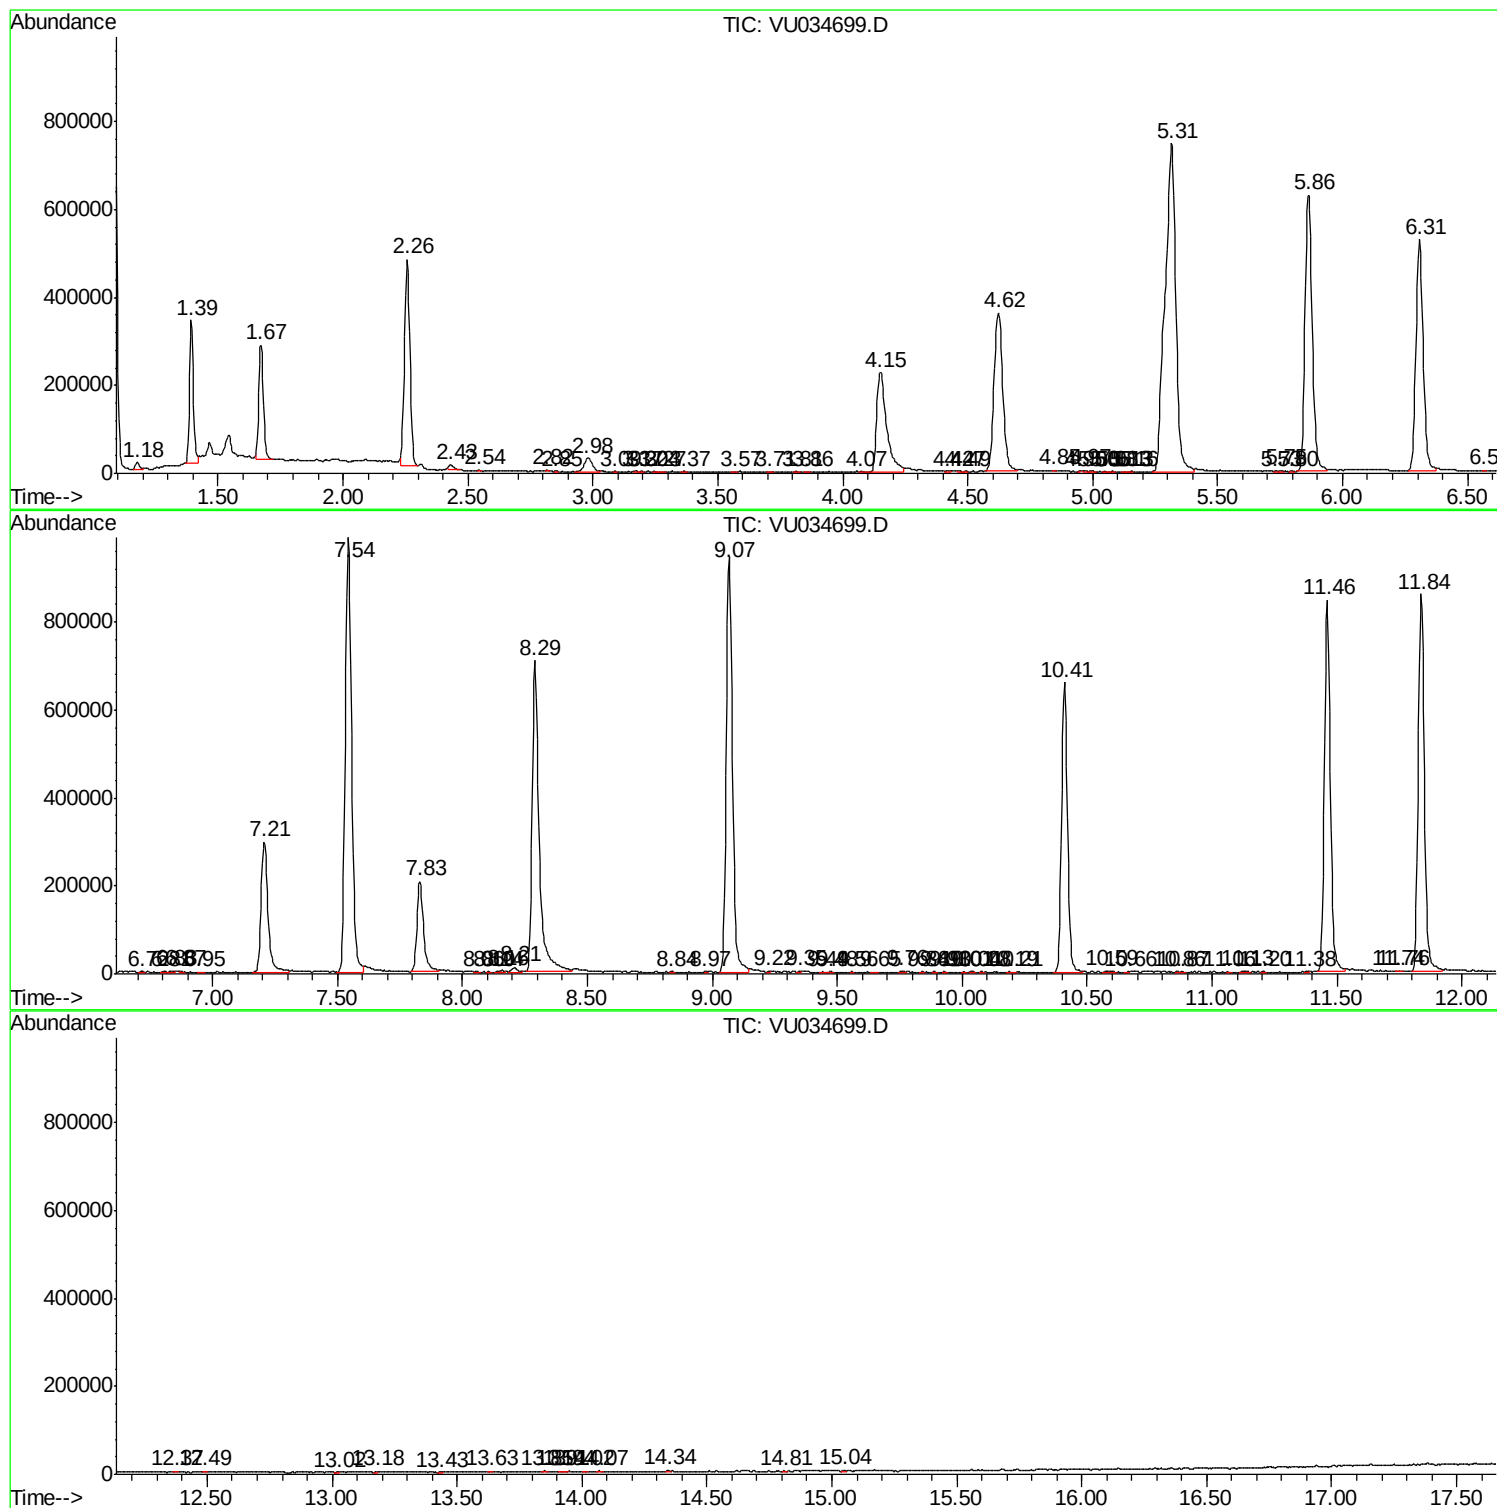

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034699.D
Acq On : 20 Sep 2019 19:15
Operator : JC/SP
Sample : K4948-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFCX3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034699.D
Acq On : 20 Sep 2019 19:15
Operator : JC/SP
Sample : K4948-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFCX3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc