

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034713.D
 Acq On : 21 Sep 2019 01:07
 Operator : JC/SP
 Sample : K4993-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETOJ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	22	27	40	rVB2	56605	55485	2.65%	0.352%
2	1.392	88	94	107	rVB	293930	315798	15.06%	2.001%
3	1.672	174	181	194	rVB	235223	296551	14.14%	1.879%
4	2.257	355	363	377	rVB	424284	653487	31.16%	4.141%
5	3.228	663	665	668	rBV3	839	532	0.03%	0.003%
6	3.347	698	702	706	rBV6	2192	1440	0.07%	0.009%
7	3.363	706	707	709	rBV2	445	115	0.01%	0.001%
8	3.376	709	711	712	rBV3	866	339	0.02%	0.002%
9	3.386	712	714	715	rBV2	795	245	0.01%	0.002%
10	3.498	747	749	752	rBV2	823	450	0.02%	0.003%
11	3.566	767	770	772	rBV2	1893	785	0.04%	0.005%
12	3.585	772	776	778	rVV2	1968	1159	0.06%	0.007%
13	3.608	778	783	788	rVB8	1326	1633	0.08%	0.010%
14	3.637	788	792	795	rBV4	1760	1437	0.07%	0.009%
15	3.672	802	803	804	rBV2	586	163	0.01%	0.001%
16	3.682	804	806	809	rVV3	1351	629	0.03%	0.004%
17	3.698	809	811	813	rVB3	1335	477	0.02%	0.003%
18	3.749	822	827	829	rBV3	1245	891	0.04%	0.006%
19	3.778	834	836	839	rVV3	793	469	0.02%	0.003%
20	3.801	839	843	847	rVB5	1410	1011	0.05%	0.006%
21	3.823	847	850	853	rVB4	940	701	0.03%	0.004%
22	3.842	853	856	858	rBV2	1285	782	0.04%	0.005%
23	3.900	872	874	877	rBV3	1010	732	0.03%	0.005%
24	3.939	884	886	888	rVB4	980	477	0.02%	0.003%
25	3.955	888	891	894	rVB4	1047	585	0.03%	0.004%
26	4.019	910	911	912	rBV4	793	273	0.01%	0.002%
27	4.061	922	924	926	rBV3	1159	595	0.03%	0.004%
28	4.090	931	933	934	rBV2	816	281	0.01%	0.002%
29	4.151	940	952	985	rBV	206056	563689	26.88%	3.572%
30	4.624	1084	1099	1128	rBV2	337180	791917	37.76%	5.018%
31	5.315	1290	1314	1342	rBV2	688407	2097150	100.00%	13.289%
32	5.794	1461	1463	1464	rBV2	1180	480	0.02%	0.003%
33	5.865	1471	1485	1509	rBV	573699	1155904	55.12%	7.324%
34	6.309	1609	1623	1647	rBV	487682	986318	47.03%	6.250%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034713.D
 Acq On : 21 Sep 2019 01:07
 Operator : JC/SP
 Sample : K4993-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETOJ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	6.717	1745	1750	1753	rBV4	1643	1190	0.06%	0.008%
36	6.733	1753	1755	1756	rBV2	951	460	0.02%	0.003%
37	6.759	1761	1763	1766	rVB3	1070	498	0.02%	0.003%
38	6.788	1766	1772	1775	rBV6	1241	1367	0.07%	0.009%
39	6.810	1775	1779	1784	rBV6	1808	1857	0.09%	0.012%
40	6.842	1787	1789	1790	rBV2	1259	512	0.02%	0.003%
41	6.971	1826	1829	1832	rBV3	1207	712	0.03%	0.005%
42	7.003	1837	1839	1840	rBV	606	175	0.01%	0.001%
43	7.013	1840	1842	1844	rBV3	887	331	0.02%	0.002%
44	7.045	1844	1852	1857	rBV8	1800	2529	0.12%	0.016%
45	7.067	1857	1859	1860	rVB3	1301	470	0.02%	0.003%
46	7.077	1860	1862	1864	rBV2	721	370	0.02%	0.002%
47	7.141	1879	1882	1883	rBV3	979	572	0.03%	0.004%
48	7.206	1890	1902	1929	rBV	259290	503953	24.03%	3.193%
49	7.543	1994	2007	2028	rBV	899817	1618028	77.15%	10.253%
50	7.829	2086	2096	2124	rBV	175189	325274	15.51%	2.061%
51	8.125	2185	2188	2190	rBV2	1783	1236	0.06%	0.008%
52	8.289	2226	2239	2274	rBV	627289	1256015	59.89%	7.959%
53	8.781	2389	2392	2395	rBV4	1481	1160	0.06%	0.007%
54	8.820	2399	2404	2406	rBV3	1275	1119	0.05%	0.007%
55	8.923	2434	2436	2439	rBV3	987	642	0.03%	0.004%
56	8.990	2455	2457	2459	rBV3	1261	811	0.04%	0.005%
57	9.067	2467	2481	2499	rBV	872507	1461460	69.69%	9.261%
58	9.344	2564	2567	2568	rBV3	1811	995	0.05%	0.006%
59	9.431	2592	2594	2595	rBV2	1006	398	0.02%	0.003%
60	9.517	2617	2621	2626	rVB6	1891	1551	0.07%	0.010%
61	9.537	2626	2627	2628	rBV	859	331	0.02%	0.002%
62	9.575	2637	2639	2642	rBV3	972	677	0.03%	0.004%
63	9.595	2642	2645	2651	rVV6	1776	1779	0.08%	0.011%
64	9.707	2678	2680	2684	rVB2	1278	959	0.05%	0.006%
65	9.726	2684	2686	2687	rBV2	628	277	0.01%	0.002%
66	9.807	2709	2711	2713	rBV3	1022	453	0.02%	0.003%
67	9.855	2723	2726	2728	rBV4	1325	931	0.04%	0.006%
68	9.961	2755	2759	2761	rBV3	1218	760	0.04%	0.005%
69	10.022	2776	2778	2780	rBV3	826	524	0.02%	0.003%
70	10.083	2793	2797	2801	rBV6	1372	1321	0.06%	0.008%
71	10.209	2834	2836	2837	rBV	986	542	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034713.D
 Acq On : 21 Sep 2019 01:07
 Operator : JC/SP
 Sample : K4993-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETOJ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	10.279	2854	2858	2861	rVB3	2584	1768	0.08%	0.011%
73	10.302	2861	2865	2866	rBV3	1022	753	0.04%	0.005%
74	10.408	2887	2898	2922	rBV	609594	1015653	48.43%	6.436%
75	10.550	2938	2942	2946	rBV6	1579	1257	0.06%	0.008%
76	10.669	2978	2979	2986	rVB5	1542	942	0.04%	0.006%
77	10.694	2986	2987	2989	rBV2	894	285	0.01%	0.002%
78	10.833	3028	3030	3031	rBV2	790	328	0.02%	0.002%
79	10.939	3058	3063	3066	rBV5	1556	1352	0.06%	0.009%
80	10.961	3066	3070	3072	rBV3	1656	985	0.05%	0.006%
81	10.996	3079	3081	3082	rBV2	908	466	0.02%	0.003%
82	11.029	3090	3091	3092	rBV	399	91	0.00%	0.001%
83	11.041	3092	3095	3097	rBV4	811	591	0.03%	0.004%
84	11.167	3132	3134	3137	rBV2	539	320	0.02%	0.002%
85	11.186	3137	3140	3142	rBV4	920	480	0.02%	0.003%
86	11.231	3149	3154	3155	rBV3	822	702	0.03%	0.004%
87	11.344	3186	3189	3191	rBV3	540	447	0.02%	0.003%
88	11.357	3191	3193	3195	rBV2	932	553	0.03%	0.004%
89	11.459	3214	3225	3250	rBV	759993	1283272	61.19%	8.131%
90	11.836	3331	3342	3366	rBV	779704	1339671	63.88%	8.489%
91	12.958	3688	3691	3698	rBV5	2290	1777	0.08%	0.011%
92	13.186	3760	3762	3769	rVB6	1762	1550	0.07%	0.010%
93	13.366	3815	3818	3819	rBV2	1727	932	0.04%	0.006%
94	13.707	3921	3924	3929	rVB6	2765	2202	0.10%	0.014%


Sum of corrected areas: 15781596

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034713.D
Acq On : 21 Sep 2019 01:07
Operator : JC/SP
Sample : K4993-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOJ2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

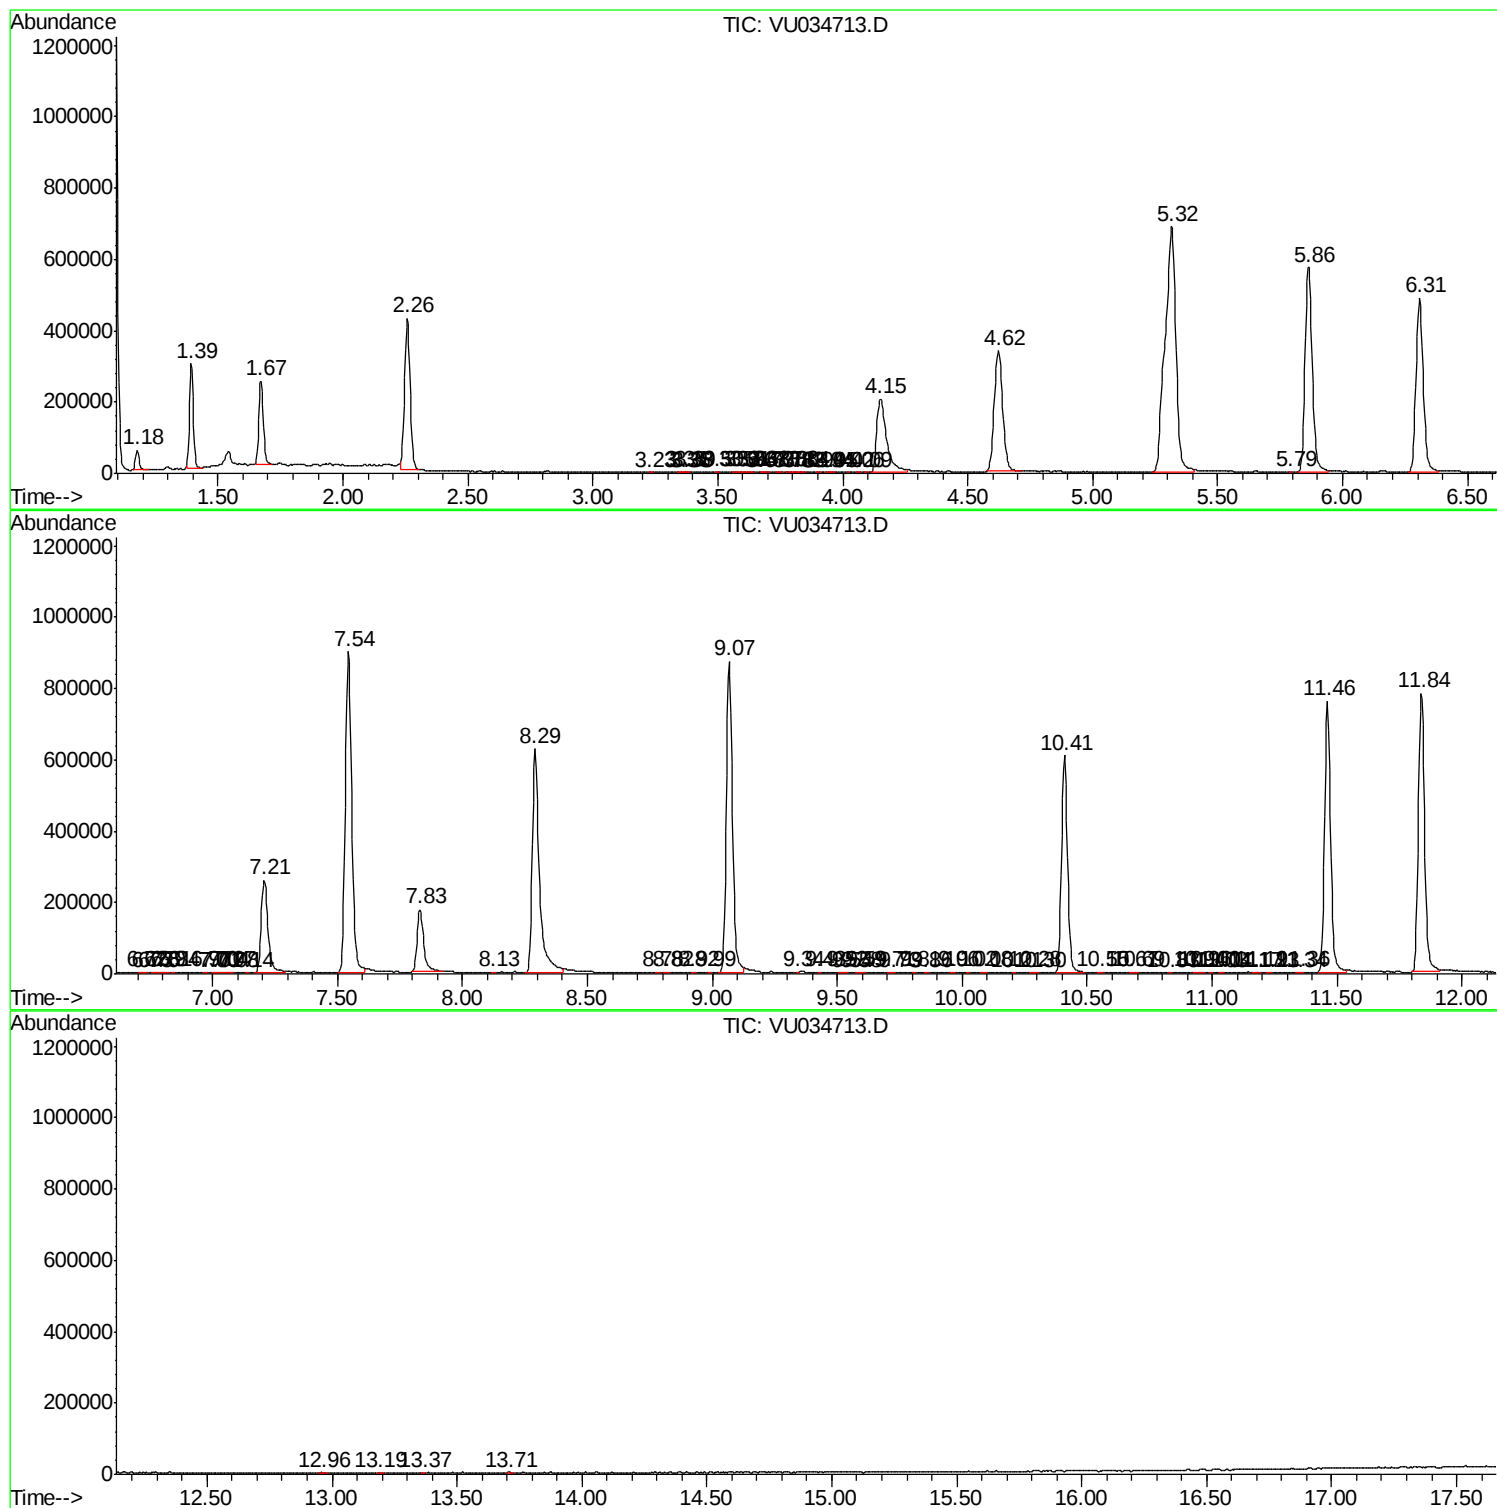

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034713.D
Acq On : 21 Sep 2019 01:07
Operator : JC/SP
Sample : K4993-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOJ2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034713.D
Acq On : 21 Sep 2019 01:07
Operator : JC/SP
Sample : K4993-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOJ2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc