

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034716.D
 Acq On : 21 Sep 2019 02:17
 Operator : JC/SP
 Sample : K5001-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDP7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	22	27	35	rVB2	38185	35568	1.71%	0.227%
2	1.392	88	94	104	rBV	276396	305304	14.67%	1.952%
3	1.672	175	181	195	rVB	236839	296767	14.26%	1.897%
4	2.257	355	363	374	rVB	411287	607778	29.21%	3.885%
5	2.903	560	564	565	rBV3	1279	850	0.04%	0.005%
6	3.167	644	646	648	rBV2	1266	701	0.03%	0.004%
7	3.321	690	694	697	rBV5	1347	1227	0.06%	0.008%
8	3.408	716	721	722	rBV4	1193	1089	0.05%	0.007%
9	3.485	742	745	750	rBV5	1334	1192	0.06%	0.008%
10	3.530	757	759	761	rBV2	644	331	0.02%	0.002%
11	3.543	761	763	765	rVB3	817	343	0.02%	0.002%
12	3.566	765	770	771	rBV2	1480	1004	0.05%	0.006%
13	3.598	778	780	781	rBV	526	190	0.01%	0.001%
14	3.698	808	811	814	rBV5	1462	1125	0.05%	0.007%
15	3.720	814	818	820	rBV2	1190	727	0.03%	0.005%
16	3.765	830	832	834	rVB3	843	342	0.02%	0.002%
17	3.781	834	837	840	rVB3	1230	685	0.03%	0.004%
18	3.797	840	842	845	rVB3	1316	717	0.03%	0.005%
19	3.820	845	849	854	rBV5	1201	1120	0.05%	0.007%
20	3.845	854	857	858	rBV3	2071	1126	0.05%	0.007%
21	3.910	875	877	879	rBV3	1265	688	0.03%	0.004%
22	4.151	940	952	962	rBV	196338	503236	24.18%	3.217%
23	4.620	1084	1098	1119	rBV2	331785	785696	37.76%	5.023%
24	5.218	1282	1284	1285	rBV	622	183	0.01%	0.001%
25	5.315	1288	1314	1346	rBV2	682823	2080898	100.00%	13.302%
26	5.804	1464	1466	1470	rVB5	1916	1234	0.06%	0.008%
27	5.865	1470	1485	1513	rBV	591461	1184721	56.93%	7.573%
28	6.167	1569	1579	1594	rBV6	23964	47998	2.31%	0.307%
29	6.308	1608	1623	1646	rBV	484899	993506	47.74%	6.351%
30	6.685	1736	1740	1742	rVB5	1456	1093	0.05%	0.007%
31	6.707	1742	1747	1752	rBV6	1513	1831	0.09%	0.012%
32	6.765	1763	1765	1769	rBV4	975	766	0.04%	0.005%
33	6.852	1789	1792	1795	rBV4	1827	1347	0.06%	0.009%
34	6.900	1805	1807	1810	rVB3	1344	570	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034716.D
 Acq On : 21 Sep 2019 02:17
 Operator : JC/SP
 Sample : K5001-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDP7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	6.916	1810	1812	1813	rBV	1523	588	0.03%	0.004%
36	6.993	1834	1836	1837	rBV	1053	467	0.02%	0.003%
37	7.035	1847	1849	1851	rVB2	844	312	0.01%	0.002%
38	7.061	1855	1857	1861	rVB2	1863	992	0.05%	0.006%
39	7.080	1861	1863	1864	rBV2	848	330	0.02%	0.002%
40	7.103	1868	1870	1874	rVB3	1204	541	0.03%	0.003%
41	7.125	1874	1877	1879	rBV3	1511	918	0.04%	0.006%
42	7.138	1879	1881	1884	rVB3	962	391	0.02%	0.002%
43	7.205	1887	1902	1924	rBV	254358	493793	23.73%	3.157%
44	7.402	1961	1963	1964	rBV2	1667	620	0.03%	0.004%
45	7.543	1994	2007	2023	rBV	899863	1583863	76.11%	10.125%
46	7.829	2085	2096	2119	rBV	172191	325050	15.62%	2.078%
47	8.289	2229	2239	2270	rBV	604711	1204241	57.87%	7.698%
48	8.836	2407	2409	2414	rVB5	1496	1061	0.05%	0.007%
49	8.881	2421	2423	2424	rBV2	603	214	0.01%	0.001%
50	8.932	2437	2439	2441	rBV3	1022	406	0.02%	0.003%
51	9.067	2469	2481	2508	rBV	854642	1483543	71.29%	9.484%
52	9.453	2598	2601	2602	rBV3	1340	718	0.03%	0.005%
53	9.514	2618	2620	2622	rBV3	1050	620	0.03%	0.004%
54	9.614	2648	2651	2654	rBV5	704	547	0.03%	0.003%
55	9.633	2654	2657	2659	rBV2	943	586	0.03%	0.004%
56	9.662	2664	2666	2669	rBV3	1031	599	0.03%	0.004%
57	9.868	2726	2730	2733	rVB5	1873	1659	0.08%	0.011%
58	9.890	2734	2737	2739	rBV4	1202	625	0.03%	0.004%
59	9.922	2745	2747	2749	rBV2	1337	844	0.04%	0.005%
60	9.938	2749	2752	2754	rVV4	1760	1256	0.06%	0.008%
61	9.955	2754	2757	2761	rVV4	1613	1245	0.06%	0.008%
62	9.980	2761	2765	2768	rVV5	1371	1063	0.05%	0.007%
63	10.019	2774	2777	2781	rBV4	3491	2991	0.14%	0.019%
64	10.119	2805	2808	2810	rBV3	1080	548	0.03%	0.004%
65	10.202	2832	2834	2838	rBV4	2072	1355	0.07%	0.009%
66	10.221	2838	2840	2842	rVV3	1197	464	0.02%	0.003%
67	10.270	2853	2855	2857	rVB3	1450	524	0.03%	0.003%
68	10.408	2886	2898	2918	rBV	623543	1020137	49.02%	6.521%
69	10.858	3036	3038	3047	rVB8	1289	1222	0.06%	0.008%
70	10.967	3069	3072	3074	rBV4	1820	1028	0.05%	0.007%
71	11.028	3086	3091	3092	rBV4	1210	962	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034716.D
Acq On : 21 Sep 2019 02:17
Operator : JC/SP
Sample : K5001-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDP7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Title : VOC Analysis

72	11.061	3097	3101	3106	rVV7	2122	2276	0.11%	0.015%
73	11.189	3139	3141	3143	rBV2	1270	604	0.03%	0.004%
74	11.353	3190	3192	3193	rBV2	581	318	0.02%	0.002%
75	11.459	3214	3225	3253	rBV	763968	1300219	62.48%	8.312%
76	11.836	3330	3342	3361	rBV	792708	1337557	64.28%	8.550%
77	13.192	3761	3764	3765	rBV4	1382	843	0.04%	0.005%
78	13.977	4004	4008	4014	rBV7	2376	3011	0.14%	0.019%


Sum of corrected areas: 15643104

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034716.D
Acq On : 21 Sep 2019 02:17
Operator : JC/SP
Sample : K5001-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDP7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

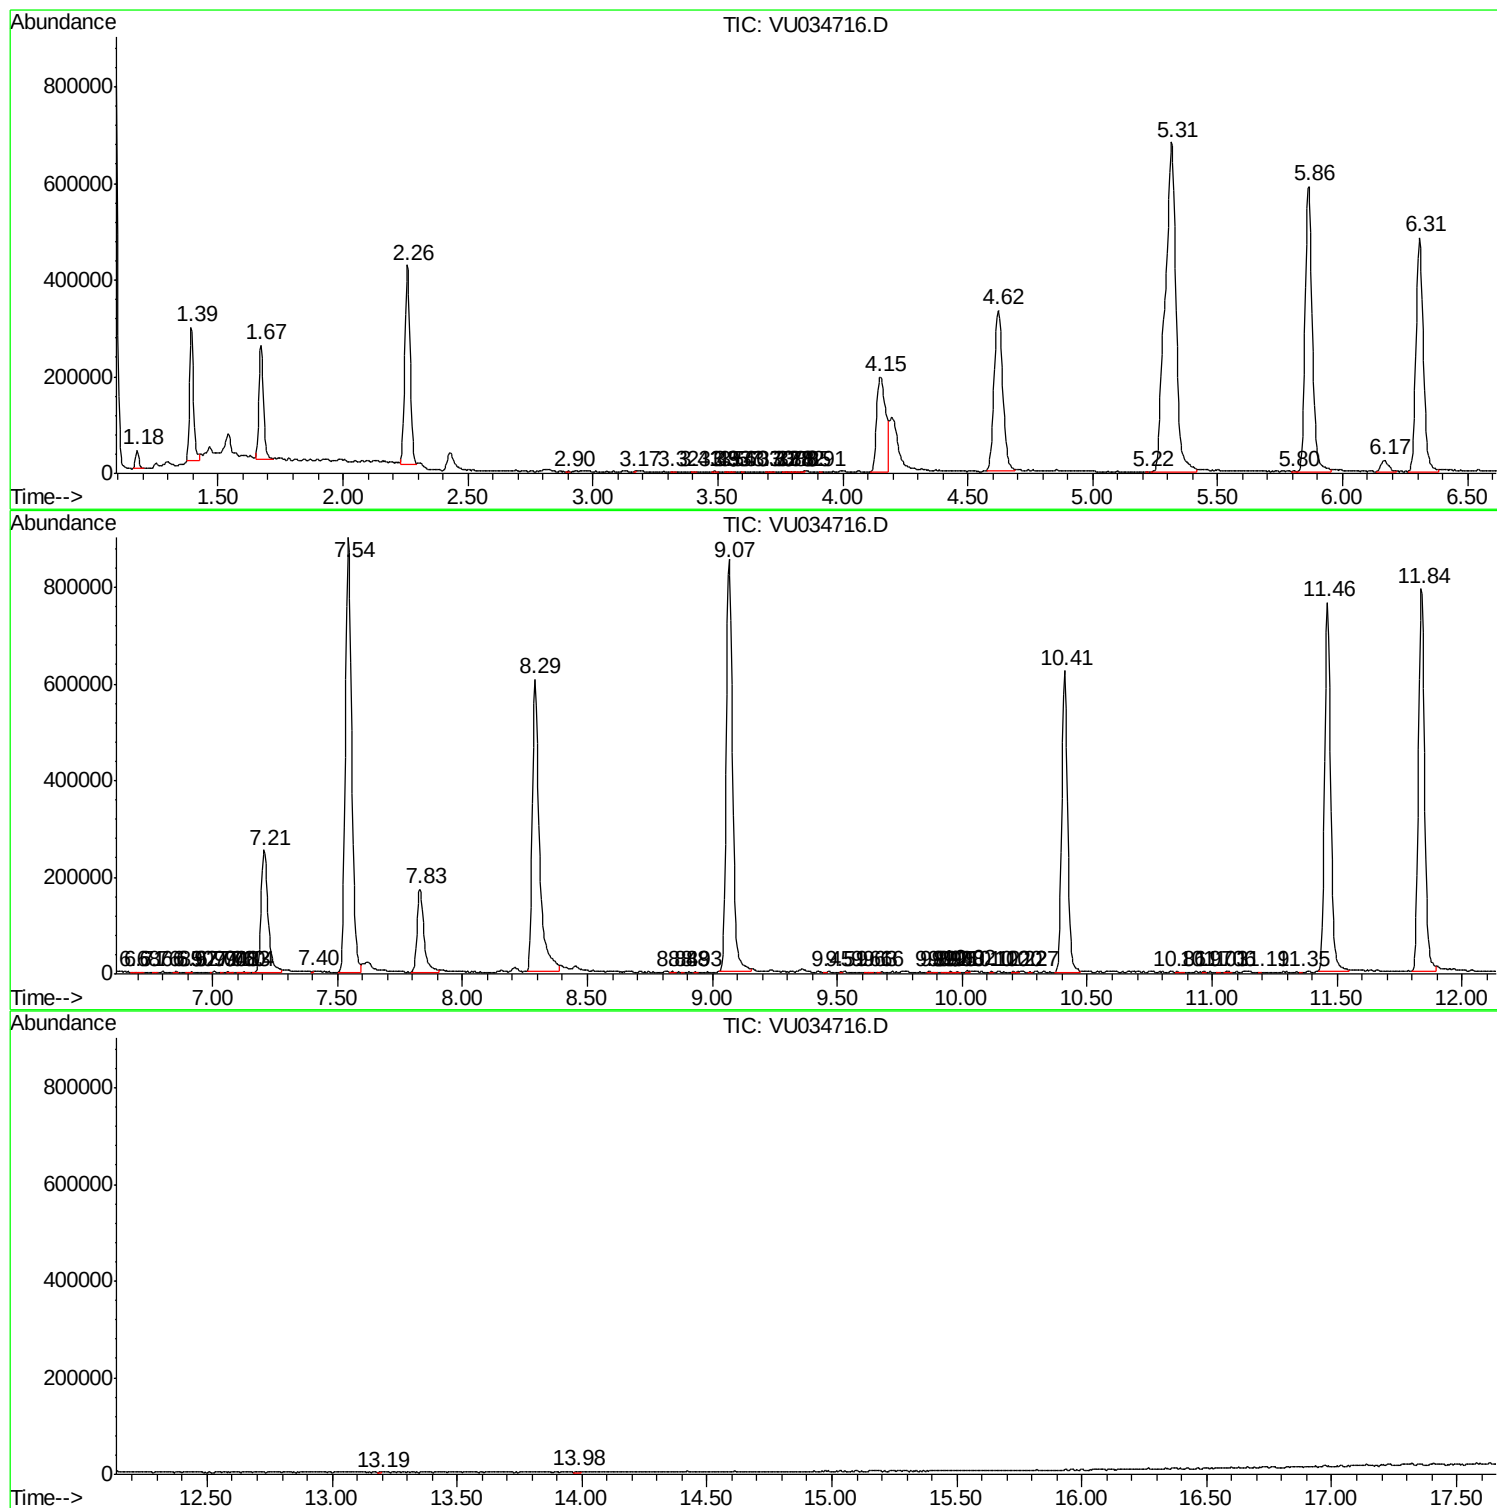

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034716.D
Acq On : 21 Sep 2019 02:17
Operator : JC/SP
Sample : K5001-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDP7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU092019\
Data File : VU034716.D
Acq On : 21 Sep 2019 02:17
Operator : JC/SP
Sample : K5001-04
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
BEDP7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
