

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034717.D
 Acq On : 21 Sep 2019 02:41
 Operator : JC/SP
 Sample : K5001-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDQ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	88	94	106	rBV	265993	276460	13.61%	1.778%
2	1.672	175	181	195	rVB	228822	285731	14.06%	1.838%
3	2.257	355	363	378	rVB	404981	609995	30.02%	3.923%
4	3.026	599	602	603	rBV3	1152	545	0.03%	0.004%
5	3.154	636	642	644	rBV5	1359	1432	0.07%	0.009%
6	3.392	714	716	720	rBV3	896	568	0.03%	0.004%
7	3.460	734	737	739	rVB3	1153	563	0.03%	0.004%
8	3.534	758	760	761	rBV	1111	505	0.02%	0.003%
9	3.592	775	778	781	rBV4	1148	957	0.05%	0.006%
10	3.611	781	784	788	rVB4	1877	1127	0.06%	0.007%
11	3.643	788	794	796	rBV6	1009	1014	0.05%	0.007%
12	3.662	797	800	801	rVB2	1239	555	0.03%	0.004%
13	3.691	801	809	812	rBV9	899	1211	0.06%	0.008%
14	3.714	813	816	818	rVB5	676	349	0.02%	0.002%
15	3.727	818	820	822	rVB3	679	323	0.02%	0.002%
16	3.740	822	824	827	rBV4	1500	941	0.05%	0.006%
17	3.772	832	834	835	rBV2	398	192	0.01%	0.001%
18	3.817	847	848	851	rVB2	1488	559	0.03%	0.004%
19	3.833	851	853	854	rBV2	391	194	0.01%	0.001%
20	3.842	854	856	860	rBV2	1442	1321	0.07%	0.008%
21	3.929	881	883	886	rVB4	841	383	0.02%	0.002%
22	3.949	886	889	890	rBV3	1176	664	0.03%	0.004%
23	3.981	895	899	902	rBV3	1021	885	0.04%	0.006%
24	4.016	908	910	912	rBV2	861	300	0.01%	0.002%
25	4.048	916	920	921	rBV3	1669	1244	0.06%	0.008%
26	4.151	940	952	994	rBV2	198850	568493	27.98%	3.656%
27	4.624	1082	1099	1119	rBV2	322453	786687	38.72%	5.060%
28	5.096	1244	1246	1248	rBV2	767	482	0.02%	0.003%
29	5.167	1266	1268	1273	rVB3	1213	763	0.04%	0.005%
30	5.193	1273	1276	1278	rVB3	1236	591	0.03%	0.004%
31	5.315	1286	1314	1339	rBV2	675371	2031730	100.00%	13.067%
32	5.865	1470	1485	1514	rBV	606703	1228978	60.49%	7.904%
33	6.222	1594	1596	1599	rBV3	1151	651	0.03%	0.004%
34	6.309	1609	1623	1643	rBV	470189	958856	47.19%	6.167%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034717.D
 Acq On : 21 Sep 2019 02:41
 Operator : JC/SP
 Sample : K5001-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDQ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	6.694	1740	1743	1744	rBV2	564	303	0.01%	0.002%
36	6.736	1751	1756	1757	rBV5	974	683	0.03%	0.004%
37	6.820	1779	1782	1787	rVB6	2182	1965	0.10%	0.013%
38	6.842	1787	1789	1791	rBV3	1151	652	0.03%	0.004%
39	6.897	1803	1806	1810	rVB4	1081	653	0.03%	0.004%
40	6.974	1827	1830	1831	rBV3	743	483	0.02%	0.003%
41	7.000	1837	1838	1839	rVB3	497	96	0.00%	0.001%
42	7.019	1841	1844	1846	rBV	1097	749	0.04%	0.005%
43	7.157	1885	1887	1890	rBV	1034	585	0.03%	0.004%
44	7.206	1890	1902	1924	rBV	248675	474531	23.36%	3.052%
45	7.501	1990	1994	1995	rBV3	2409	1431	0.07%	0.009%
46	7.543	1995	2007	2028	rVV	892247	1571803	77.36%	10.109%
47	7.829	2083	2096	2119	rBV	165525	323595	15.93%	2.081%
48	8.067	2166	2170	2176	rVB7	1937	2197	0.11%	0.014%
49	8.109	2176	2183	2184	rBV5	1571	1450	0.07%	0.009%
50	8.215	2212	2216	2221	rVB5	2441	2277	0.11%	0.015%
51	8.247	2225	2226	2228	rBV	1151	542	0.03%	0.003%
52	8.289	2228	2239	2276	rBV	608099	1215157	59.81%	7.815%
53	8.775	2386	2390	2393	rBV4	2039	1908	0.09%	0.012%
54	8.981	2452	2454	2456	rBV3	1276	743	0.04%	0.005%
55	9.013	2460	2464	2468	rBV6	1276	1467	0.07%	0.009%
56	9.067	2469	2481	2503	rBV	896899	1532797	75.44%	9.858%
57	9.344	2566	2567	2570	rBV3	1500	874	0.04%	0.006%
58	9.543	2627	2629	2631	rBV2	1340	849	0.04%	0.005%
59	9.585	2638	2642	2644	rBV2	1619	1254	0.06%	0.008%
60	9.630	2654	2656	2658	rVB3	1768	786	0.04%	0.005%
61	9.704	2676	2679	2684	rBV4	739	831	0.04%	0.005%
62	9.836	2714	2720	2724	rVB7	1876	1984	0.10%	0.013%
63	9.858	2725	2727	2729	rVB3	1327	509	0.03%	0.003%
64	9.874	2731	2732	2733	rVV	814	167	0.01%	0.001%
65	10.045	2782	2785	2787	rBV3	974	632	0.03%	0.004%
66	10.106	2803	2804	2806	rBV2	816	336	0.02%	0.002%
67	10.119	2806	2808	2809	rBV	762	348	0.02%	0.002%
68	10.328	2870	2873	2875	rBV3	1666	1003	0.05%	0.006%
69	10.408	2886	2898	2920	rBV	607795	1004993	49.46%	6.464%
70	10.723	2993	2996	2999	rBV3	1263	1046	0.05%	0.007%
71	10.878	3039	3044	3046	rBV4	1710	1504	0.07%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034717.D
 Acq On : 21 Sep 2019 02:41
 Operator : JC/SP
 Sample : K5001-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDQ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	10.913	3054	3055	3057	rVB2	862	273	0.01%	0.002%
73	11.003	3080	3083	3087	rBV3	1239	981	0.05%	0.006%
74	11.099	3111	3113	3115	rBV3	1317	544	0.03%	0.003%
75	11.128	3120	3122	3125	rBV3	1647	776	0.04%	0.005%
76	11.164	3131	3133	3134	rBV2	890	312	0.02%	0.002%
77	11.334	3182	3186	3187	rBV3	1947	1298	0.06%	0.008%
78	11.460	3213	3225	3243	rBV	797101	1329690	65.45%	8.552%
79	11.836	3331	3342	3360	rBV	761773	1287511	63.37%	8.281%
80	12.170	3444	3446	3451	rVB5	2743	1827	0.09%	0.012%
81	12.877	3664	3666	3668	rBV3	1244	681	0.03%	0.004%
82	13.344	3808	3811	3816	rBV6	1898	2013	0.10%	0.013%
83	13.884	3976	3979	3981	rBV3	2010	1444	0.07%	0.009%
84	14.221	4082	4084	4086	rBV3	1610	882	0.04%	0.006%
85	14.537	4180	4182	4188	rVB7	2108	1378	0.07%	0.009%


Sum of corrected areas: 15548042

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034717.D
Acq On : 21 Sep 2019 02:41
Operator : JC/SP
Sample : K5001-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDQ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

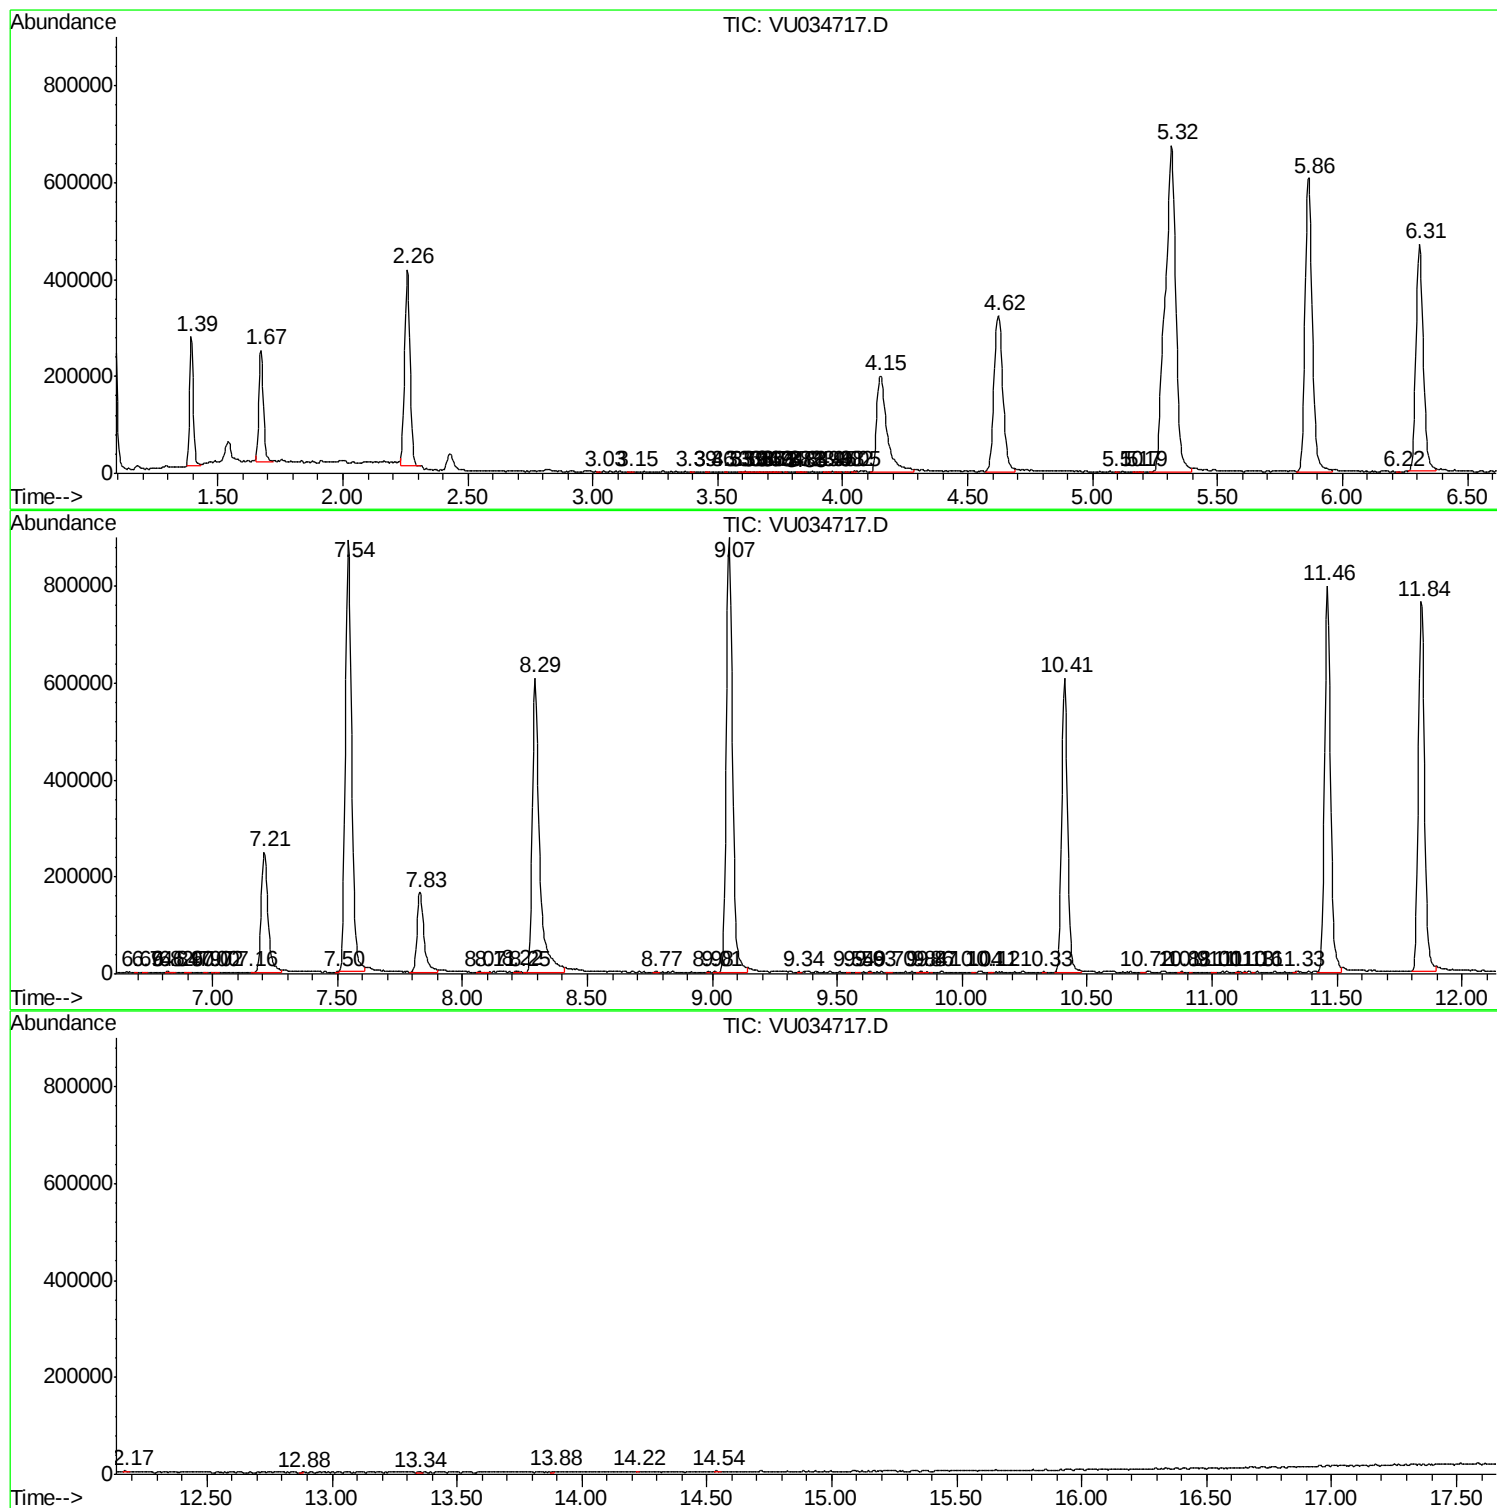

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034717.D
Acq On : 21 Sep 2019 02:41
Operator : JC/SP
Sample : K5001-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDQ3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034717.D
Acq On : 21 Sep 2019 02:41
Operator : JC/SP
Sample : K5001-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDQ3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc