

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034721.D
 Acq On : 21 Sep 2019 04:14
 Operator : JC/SP
 Sample : K5001-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFCY6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	34	rVB	21544	19858	1.00%	0.133%
2	1.392	89	94	108	rBV	250475	268507	13.57%	1.798%
3	1.672	176	181	195	rVB	223881	277406	14.02%	1.857%
4	2.257	355	363	376	rVB	387920	592275	29.93%	3.966%
5	2.794	528	530	532	rBV2	1571	936	0.05%	0.006%
6	2.871	551	554	556	rBV4	1522	914	0.05%	0.006%
7	3.093	618	623	624	rBV4	1570	1315	0.07%	0.009%
8	3.167	643	646	648	rBV3	1228	768	0.04%	0.005%
9	3.292	683	685	687	rBV2	1000	630	0.03%	0.004%
10	3.334	695	698	700	rBV2	772	503	0.03%	0.003%
11	3.392	712	716	720	rBV6	1058	930	0.05%	0.006%
12	3.431	726	728	731	rVB4	1648	858	0.04%	0.006%
13	3.453	731	735	736	rBV2	811	566	0.03%	0.004%
14	3.479	739	743	747	rVB6	1627	1524	0.08%	0.010%
15	3.508	747	752	755	rBV5	1202	1206	0.06%	0.008%
16	3.582	772	775	777	rVB2	1571	803	0.04%	0.005%
17	3.604	777	782	784	rBV5	782	767	0.04%	0.005%
18	3.636	788	792	797	rBV5	1925	1996	0.10%	0.013%
19	3.701	809	812	816	rVV3	1086	973	0.05%	0.007%
20	3.794	837	841	845	rBV5	914	1051	0.05%	0.007%
21	3.826	849	851	853	rVB2	915	396	0.02%	0.003%
22	3.842	853	856	857	rBV3	1050	537	0.03%	0.004%
23	3.884	865	869	870	rBV2	758	506	0.03%	0.003%
24	3.900	870	874	877	rBV5	1585	1022	0.05%	0.007%
25	3.952	886	890	894	rBV6	1309	1283	0.06%	0.009%
26	4.074	925	928	931	rBV3	1262	860	0.04%	0.006%
27	4.151	941	952	981	rBV	189805	523271	26.45%	3.503%
28	4.620	1082	1098	1125	rBV	318188	767645	38.80%	5.140%
29	4.926	1190	1193	1195	rBV3	2306	1143	0.06%	0.008%
30	5.090	1242	1244	1247	rBV3	882	581	0.03%	0.004%
31	5.106	1247	1249	1254	rVV4	1283	1169	0.06%	0.008%
32	5.164	1264	1267	1269	rBV2	1433	954	0.05%	0.006%
33	5.209	1278	1281	1283	rBV3	1478	689	0.03%	0.005%
34	5.315	1289	1314	1342	rBV2	659922	1978634	100.00%	13.248%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034721.D
 Acq On : 21 Sep 2019 04:14
 Operator : JC/SP
 Sample : K5001-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFCY6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	5.707	1434	1436	1438	rBV3	1415	463	0.02%	0.003%
36	5.813	1467	1469	1471	rVB2	1302	421	0.02%	0.003%
37	5.865	1471	1485	1512	rBV	558157	1116128	56.41%	7.473%
38	6.257	1601	1607	1609	rBV5	1991	1991	0.10%	0.013%
39	6.308	1610	1623	1646	rVV	451875	930167	47.01%	6.228%
40	6.746	1757	1759	1765	rBV5	1639	1350	0.07%	0.009%
41	6.794	1772	1774	1775	rBV3	821	284	0.01%	0.002%
42	6.890	1801	1804	1807	rBV5	1073	882	0.04%	0.006%
43	6.955	1821	1824	1826	rBV2	1331	819	0.04%	0.005%
44	6.968	1826	1828	1832	rVB3	733	582	0.03%	0.004%
45	7.000	1837	1838	1840	rBV2	566	252	0.01%	0.002%
46	7.013	1840	1842	1844	rBV3	831	436	0.02%	0.003%
47	7.038	1849	1850	1852	rVB2	810	238	0.01%	0.002%
48	7.058	1852	1856	1858	rBV4	1370	886	0.04%	0.006%
49	7.125	1874	1877	1879	rBV3	1107	490	0.02%	0.003%
50	7.141	1880	1882	1884	rVB3	896	287	0.01%	0.002%
51	7.205	1890	1902	1926	rBV	241340	463994	23.45%	3.107%
52	7.543	1993	2007	2030	rBV	854534	1535634	77.61%	10.282%
53	7.829	2086	2096	2123	rBV	162809	311430	15.74%	2.085%
54	8.196	2208	2210	2213	rBV4	1737	1206	0.06%	0.008%
55	8.289	2227	2239	2280	rBV	579803	1204046	60.85%	8.062%
56	8.691	2361	2364	2368	rBV4	1417	1266	0.06%	0.008%
57	8.903	2427	2430	2436	rBV4	1506	1884	0.10%	0.013%
58	8.983	2453	2455	2457	rVB3	1013	367	0.02%	0.002%
59	9.067	2469	2481	2504	rBV	826098	1414177	71.47%	9.468%
60	9.463	2601	2604	2606	rBV2	2022	1141	0.06%	0.008%
61	9.475	2606	2608	2610	rBV3	844	401	0.02%	0.003%
62	9.588	2641	2643	2644	rBV2	1098	432	0.02%	0.003%
63	9.623	2652	2654	2657	rVB5	1515	720	0.04%	0.005%
64	9.643	2657	2660	2662	rBV2	1117	658	0.03%	0.004%
65	9.707	2676	2680	2682	rBV4	1242	1191	0.06%	0.008%
66	9.810	2707	2712	2714	rBV5	1261	964	0.05%	0.006%
67	9.858	2725	2727	2731	rVB3	2248	1541	0.08%	0.010%
68	9.877	2731	2733	2735	rBV3	1510	866	0.04%	0.006%
69	9.916	2743	2745	2749	rVB4	1243	808	0.04%	0.005%
70	9.938	2749	2752	2753	rBV2	1034	543	0.03%	0.004%
71	9.964	2757	2760	2762	rBV3	1234	746	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034721.D
 Acq On : 21 Sep 2019 04:14
 Operator : JC/SP
 Sample : K5001-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFCY6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	9.993	2768	2769	2771	rVB2	996	285	0.01%	0.002%
73	10.009	2771	2774	2776	rBV3	1125	672	0.03%	0.004%
74	10.077	2793	2795	2797	rBV3	1427	813	0.04%	0.005%
75	10.135	2811	2813	2815	rBV2	1061	524	0.03%	0.004%
76	10.192	2828	2831	2833	rBV5	1593	930	0.05%	0.006%
77	10.295	2862	2863	2865	rBV2	910	322	0.02%	0.002%
78	10.408	2887	2898	2919	rBV	592592	970884	49.07%	6.500%
79	10.668	2977	2979	2983	rVB4	1438	857	0.04%	0.006%
80	10.697	2983	2988	2992	rBV8	1965	2001	0.10%	0.013%
81	10.729	2995	2998	2999	rVV2	1764	909	0.05%	0.006%
82	10.749	3002	3004	3009	rVV3	1256	766	0.04%	0.005%
83	10.787	3014	3016	3019	rVV3	1044	674	0.03%	0.005%
84	10.832	3027	3030	3031	rBV3	854	414	0.02%	0.003%
85	10.868	3039	3041	3043	rBV2	1064	330	0.02%	0.002%
86	10.945	3063	3065	3067	rBV3	1041	625	0.03%	0.004%
87	10.993	3078	3080	3084	rBV4	1702	1609	0.08%	0.011%
88	11.064	3100	3102	3106	rBV5	1680	1203	0.06%	0.008%
89	11.163	3131	3133	3138	rBV6	1153	974	0.05%	0.007%
90	11.241	3150	3157	3158	rBV6	987	1001	0.05%	0.007%
91	11.260	3161	3163	3166	rBV2	707	480	0.02%	0.003%
92	11.340	3186	3188	3191	rVB2	1393	722	0.04%	0.005%
93	11.356	3191	3193	3194	rBV	1322	628	0.03%	0.004%
94	11.392	3201	3204	3205	rBV3	1233	674	0.03%	0.005%
95	11.414	3209	3211	3212	rBV3	703	268	0.01%	0.002%
96	11.459	3214	3225	3246	rBV	718579	1223991	61.86%	8.195%
97	11.835	3331	3342	3371	rBV	734124	1267591	64.06%	8.487%
98	13.655	3905	3908	3910	rBV4	1700	1118	0.06%	0.007%
99	13.810	3954	3956	3962	rBV5	1730	1383	0.07%	0.009%
100	13.848	3967	3968	3971	rBV	1308	871	0.04%	0.006%


Sum of corrected areas: 14935686

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034721.D
Acq On : 21 Sep 2019 04:14
Operator : JC/SP
Sample : K5001-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFCY6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

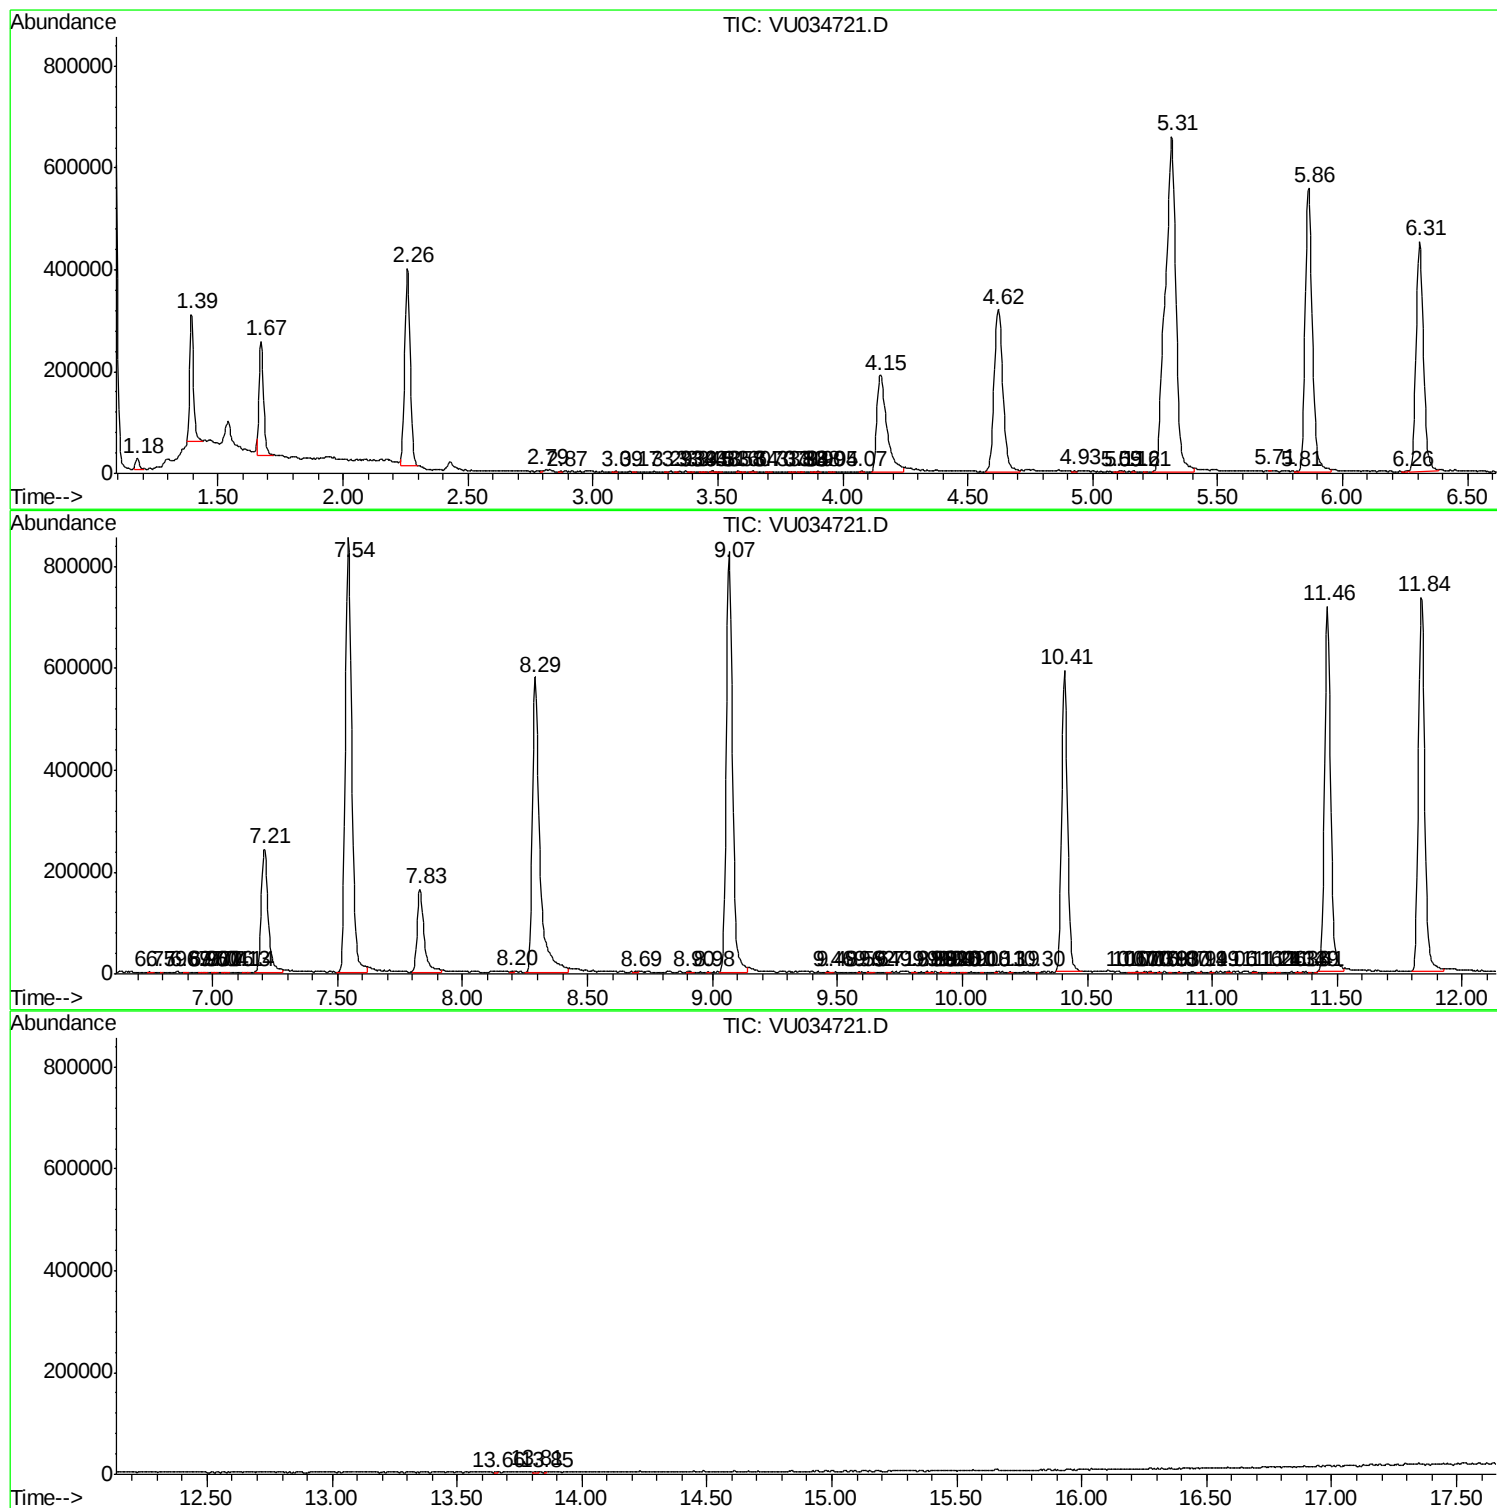

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034721.D
Acq On : 21 Sep 2019 04:14
Operator : JC/SP
Sample : K5001-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFCY6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034721.D
Acq On : 21 Sep 2019 04:14
Operator : JC/SP
Sample : K5001-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFCY6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc