

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034722.D
 Acq On : 21 Sep 2019 04:37
 Operator : JC/SP
 Sample : K5001-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFCZ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	21	27	39	rBV	45704	45429	2.23%	0.295%
2	1.254	46	51	55	rBV2	7856	9447	0.46%	0.061%
3	1.392	88	94	107	rBV	269490	295128	14.52%	1.917%
4	1.672	174	181	197	rVB	230372	292655	14.39%	1.901%
5	2.257	354	363	374	rVB	393045	596112	29.32%	3.872%
6	2.428	409	416	434	rVB2	14493	31336	1.54%	0.204%
7	2.495	434	437	440	rBV5	1414	1090	0.05%	0.007%
8	2.575	460	462	467	rVB4	1518	1032	0.05%	0.007%
9	2.604	467	471	474	rVB6	1576	1245	0.06%	0.008%
10	2.910	563	566	568	rBV3	2003	1208	0.06%	0.008%
11	2.948	575	578	582	rVB5	1819	1111	0.05%	0.007%
12	2.974	582	586	587	rBV2	2463	1763	0.09%	0.011%
13	3.071	613	616	618	rBV4	1470	949	0.05%	0.006%
14	3.122	626	632	638	rBV9	2344	3664	0.18%	0.024%
15	3.244	663	670	674	rBV7	1477	1385	0.07%	0.009%
16	3.321	693	694	699	rVB3	1692	1137	0.06%	0.007%
17	3.370	704	709	712	rVB6	1211	958	0.05%	0.006%
18	3.389	712	715	719	rBV5	1158	1095	0.05%	0.007%
19	3.563	766	769	772	rVB3	1547	965	0.05%	0.006%
20	3.749	825	827	831	rVB4	1778	1118	0.05%	0.007%
21	3.784	835	838	844	rVB4	1716	1485	0.07%	0.010%
22	3.813	844	847	850	rBV3	1752	1193	0.06%	0.008%
23	3.958	887	892	894	rBV3	2267	1909	0.09%	0.012%
24	4.151	940	952	963	rBV	191963	494718	24.33%	3.214%
25	4.444	1040	1043	1047	rBV6	1781	1405	0.07%	0.009%
26	4.624	1081	1099	1123	rBV	322925	782388	38.48%	5.083%
27	5.074	1233	1239	1243	rVB7	1871	2406	0.12%	0.016%
28	5.103	1243	1248	1251	rVB6	1355	1077	0.05%	0.007%
29	5.186	1270	1274	1277	rBV4	1102	975	0.05%	0.006%
30	5.315	1291	1314	1344	rBV2	669313	2033103	100.00%	13.207%
31	5.492	1367	1369	1372	rBV3	2546	1468	0.07%	0.010%
32	5.733	1436	1444	1446	rBV7	1851	2232	0.11%	0.014%
33	5.865	1471	1485	1506	rBV	563660	1138663	56.01%	7.397%
34	6.074	1547	1550	1554	rVB5	2028	1207	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034722.D
 Acq On : 21 Sep 2019 04:37
 Operator : JC/SP
 Sample : K5001-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFCZ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	6.170	1568	1580	1593	rBV5	18038	40698	2.00%	0.264%
36	6.308	1607	1623	1646	rBV2	470548	964511	47.44%	6.266%
37	6.694	1740	1743	1746	rBV2	1486	1003	0.05%	0.007%
38	6.726	1750	1753	1760	rVB5	1217	1195	0.06%	0.008%
39	6.823	1777	1783	1788	rBV10	1278	1402	0.07%	0.009%
40	6.874	1794	1799	1801	rBV6	1375	976	0.05%	0.006%
41	7.064	1856	1858	1862	rVB4	1546	985	0.05%	0.006%
42	7.205	1889	1902	1925	rBV	253130	477781	23.50%	3.104%
43	7.488	1986	1990	1992	rBV3	1875	1802	0.09%	0.012%
44	7.543	1994	2007	2024	rBV	875179	1543127	75.90%	10.024%
45	7.829	2086	2096	2119	rVV	161516	304912	15.00%	1.981%
46	8.019	2153	2155	2158	rVB2	1918	1037	0.05%	0.007%
47	8.074	2169	2172	2174	rBV4	1709	1120	0.06%	0.007%
48	8.141	2188	2193	2194	rBV3	1332	1148	0.06%	0.007%
49	8.209	2206	2214	2224	rBV8	9370	16615	0.82%	0.108%
50	8.292	2228	2240	2281	rBV	570310	1194204	58.74%	7.758%
51	8.604	2333	2337	2340	rBV4	2225	2050	0.10%	0.013%
52	8.643	2347	2349	2354	rVB5	1857	1022	0.05%	0.007%
53	8.672	2354	2358	2360	rBV4	1716	1411	0.07%	0.009%
54	8.765	2383	2387	2389	rBV4	1482	1244	0.06%	0.008%
55	8.932	2434	2439	2440	rBV5	1386	956	0.05%	0.006%
56	9.000	2457	2460	2464	rVB4	1565	951	0.05%	0.006%
57	9.067	2469	2481	2508	rBV	841405	1453806	71.51%	9.444%
58	9.234	2527	2533	2539	rBV7	3995	4894	0.24%	0.032%
59	9.331	2559	2563	2564	rBV4	1582	1080	0.05%	0.007%
60	9.360	2565	2572	2587	rVB6	7388	14057	0.69%	0.091%
61	9.591	2642	2644	2647	rVB3	1743	1087	0.05%	0.007%
62	9.765	2692	2698	2699	rBV5	2296	2165	0.11%	0.014%
63	9.861	2726	2728	2732	rVB5	1498	1102	0.05%	0.007%
64	9.897	2734	2739	2743	rBV8	1110	1210	0.06%	0.008%
65	9.961	2756	2759	2762	rVB3	1841	1127	0.06%	0.007%
66	10.109	2801	2805	2807	rBV4	1434	947	0.05%	0.006%
67	10.408	2884	2898	2920	rBV	605084	997300	49.05%	6.479%
68	10.524	2930	2934	2936	rBV4	2319	1693	0.08%	0.011%
69	10.662	2973	2977	2982	rBV7	2062	2580	0.13%	0.017%
70	10.720	2992	2995	2997	rBV3	1570	1054	0.05%	0.007%
71	10.829	3024	3029	3032	rBV5	1862	1528	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034722.D
 Acq On : 21 Sep 2019 04:37
 Operator : JC/SP
 Sample : K5001-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFCZ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	11.064	3098	3102	3105	rBV5	1879	1261	0.06%	0.008%
73	11.122	3117	3120	3121	rBV3	2168	1335	0.07%	0.009%
74	11.157	3130	3131	3136	rVB4	2019	1200	0.06%	0.008%
75	11.237	3153	3156	3161	rVV6	1439	1241	0.06%	0.008%
76	11.392	3198	3204	3208	rVB8	2484	2135	0.11%	0.014%
77	11.463	3213	3226	3248	rBV	737191	1258422	61.90%	8.175%
78	11.839	3329	3343	3363	rBV	757401	1300353	63.96%	8.447%
79	12.228	3459	3464	3467	rBV7	1869	1959	0.10%	0.013%
80	12.376	3507	3510	3514	rBV4	1611	1045	0.05%	0.007%
81	12.466	3536	3538	3545	rVB6	1124	1020	0.05%	0.007%
82	12.819	3644	3648	3650	rBV2	1394	1009	0.05%	0.007%
83	13.067	3721	3725	3727	rBV3	1571	1311	0.06%	0.009%
84	13.109	3735	3738	3739	rBV3	1698	939	0.05%	0.006%
85	13.286	3790	3793	3798	rBV7	1566	1470	0.07%	0.010%
86	13.311	3798	3801	3805	rVV4	1276	995	0.05%	0.006%
87	13.443	3838	3842	3845	rBV5	1848	1600	0.08%	0.010%
88	13.462	3846	3848	3850	rVV3	2016	920	0.05%	0.006%
89	13.520	3864	3866	3868	rBV3	1667	1023	0.05%	0.007%
90	13.681	3913	3916	3921	rVB7	1986	1839	0.09%	0.012%
91	14.003	4012	4016	4021	rBV7	2056	1851	0.09%	0.012%
92	14.064	4032	4035	4037	rBV4	2017	1318	0.06%	0.009%
93	14.151	4058	4062	4065	rBV3	1313	1204	0.06%	0.008%
94	14.244	4088	4091	4093	rBV3	2196	1061	0.05%	0.007%
95	14.347	4121	4123	4128	rVB5	1736	1535	0.08%	0.010%
96	14.372	4128	4131	4133	rBV2	1500	921	0.05%	0.006%
97	14.427	4145	4148	4152	rBV4	1860	1726	0.08%	0.011%
98	14.681	4225	4227	4230	rBV3	1671	1137	0.06%	0.007%
99	15.009	4326	4329	4334	rBV7	1852	1775	0.09%	0.012%
100	15.649	4526	4528	4530	rBV3	2090	1186	0.06%	0.008%


Sum of corrected areas: 15393627

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034722.D
Acq On : 21 Sep 2019 04:37
Operator : JC/SP
Sample : K5001-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BFCZ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

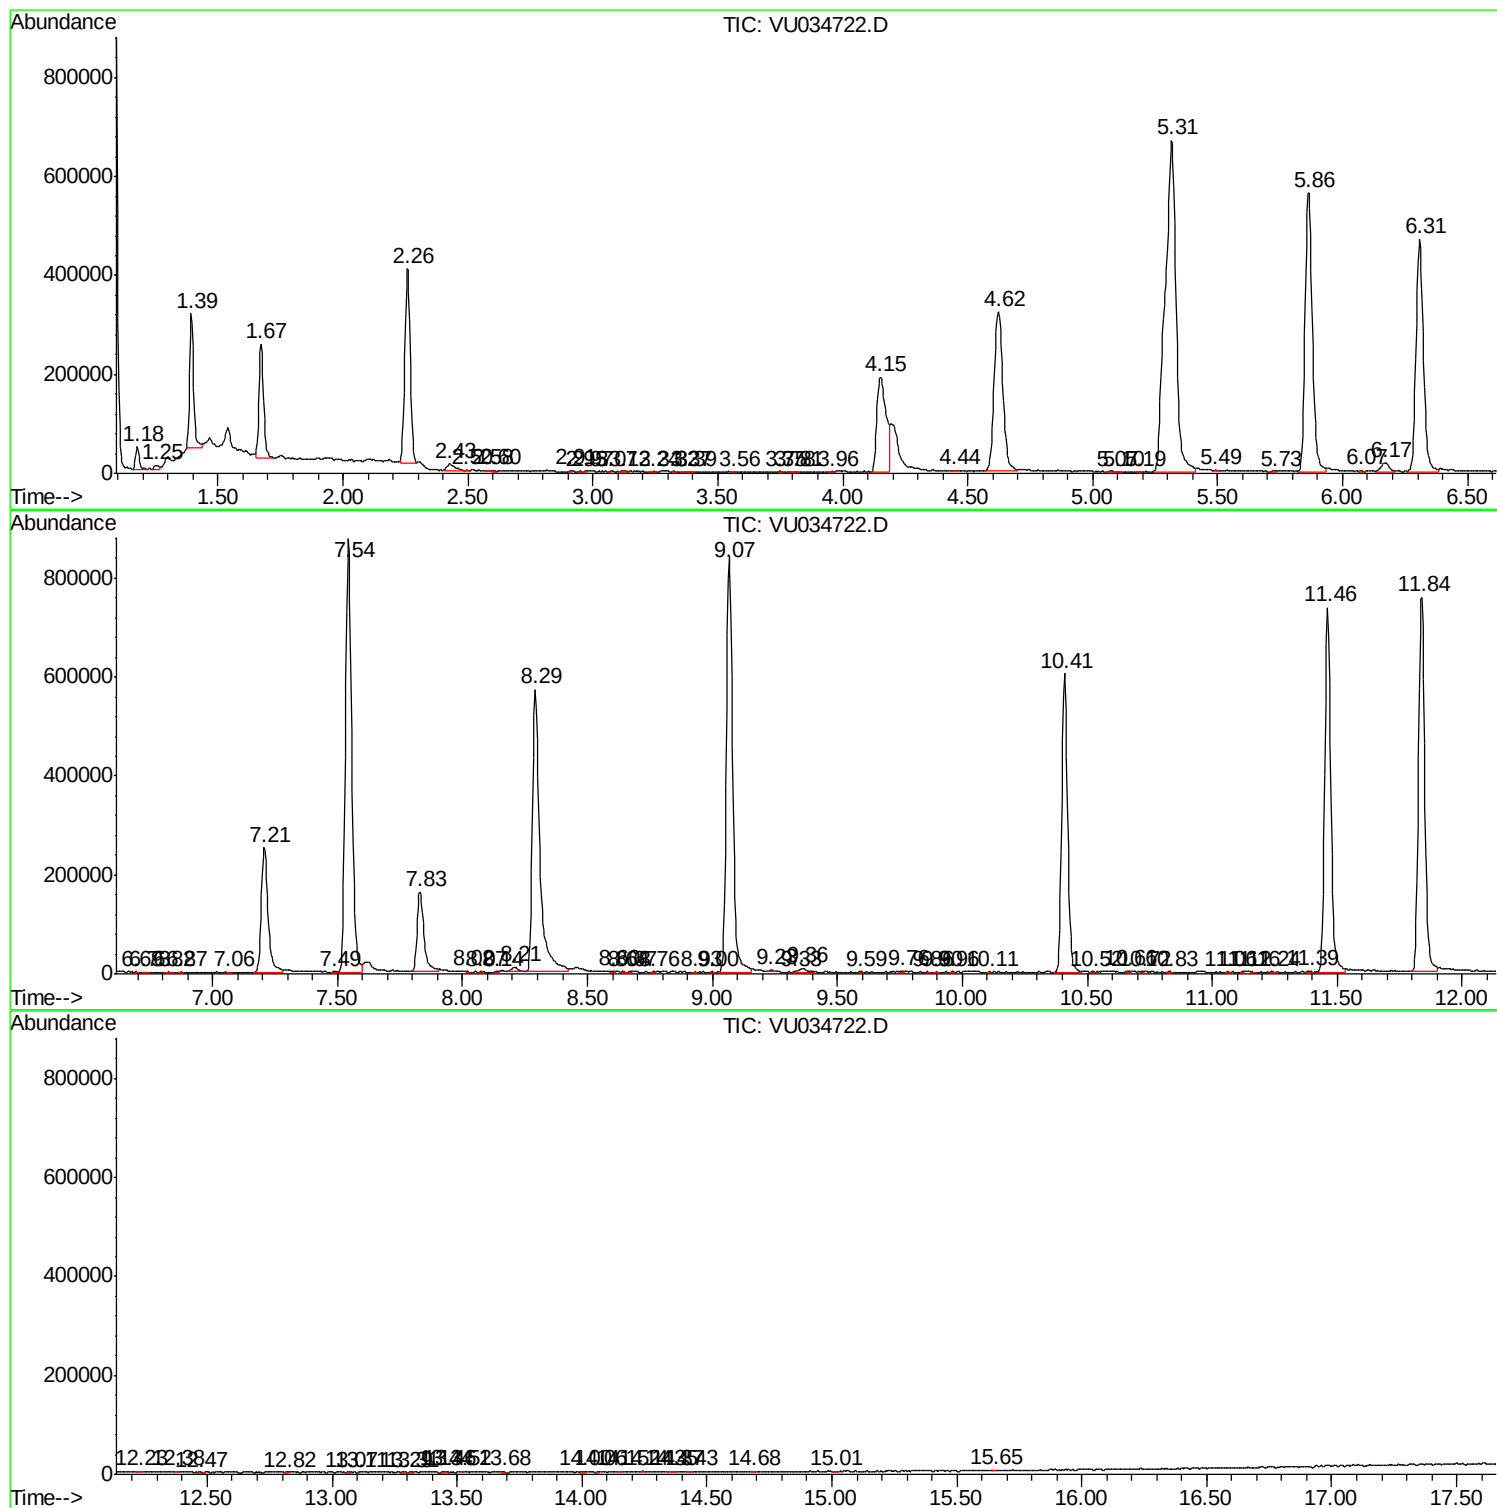

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034722.D
Acq On : 21 Sep 2019 04:37
Operator : JC/SP
Sample : K5001-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFCZ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034722.D
Acq On : 21 Sep 2019 04:37
Operator : JC/SP
Sample : K5001-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFCZ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc