


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092019\
 Data File : VU034678.D
 Acq On : 20 Sep 2019 09:04
 Operator : JC/SP
 Sample : BFB35
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB35

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 21 05:27:34 2019

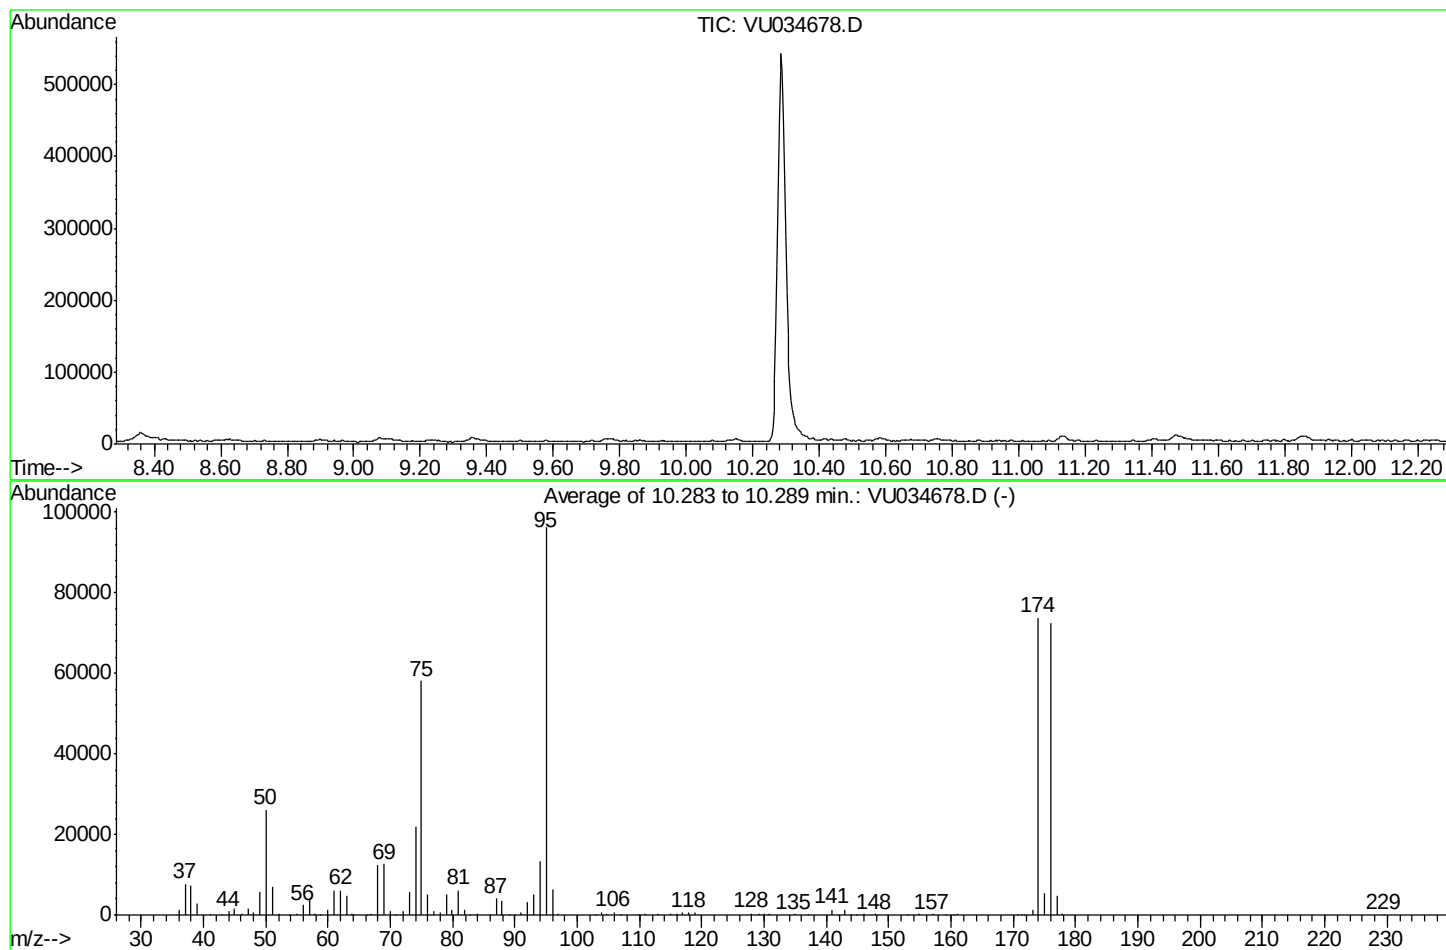

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	27.1	26082	PASS
75	95	30	80	60.4	58101	PASS
95	95	100	100	100.0	96248	PASS
96	95	5	9	6.8	6516	PASS
173	174	0.00	2	1.7	1234	PASS
174	95	50	120	76.7	73808	PASS
175	174	5	9	7.1	5266	PASS
176	174	95	101	98.1	72437	PASS
177	176	5	9	6.4	4658	PASS

m/z	Abundance
36.00	1323.0
37.00	7804.0
38.00	7255.0
39.00	3117.0
40.00	616.0
40.90	218.0
42.90	439.0
44.00	1829.0
44.90	1438.0
46.20	187.0
47.10	1574.0
47.90	897.0
49.00	5656.0
50.00	26504.0
51.00	7570.0
52.00	331.0
54.80	431.0
56.00	2554.0
57.00	4029.0
57.90	137.0
60.00	1266.0
61.00	5921.0
62.00	6308.0
63.00	4721.0
63.90	455.0
66.90	352.0
68.00	12475.0
69.00	12564.0
70.00	870.0
72.00	992.0
73.00	6022.0
74.00	21656.0
75.00	57824.0
76.00	4792.0
77.10	912.0
78.00	651.0
78.90	5108.0
79.90	1549.0
80.90	5840.0
81.90	1339.0
82.80	127.0
84.00	205.0
87.00	4195.0
87.90	3479.0
90.00	100.0
90.90	541.0
92.00	3324.0
93.00	5167.0
94.00	12925.0
95.00	96296.0
96.00	6619.0
97.00	367.0
102.80	172.0
103.80	636.0
104.70	144.0
105.90	748.0
110.80	180.0
112.80	170.0
115.10	148.0
115.90	472.0
116.90	553.0
117.90	708.0
119.00	494.0
127.90	452.0
129.10	311.0
130.00	500.0
130.70	219.0
134.90	290.0
140.90	1564.0
142.00	131.0
142.90	1375.0
144.80	112.0
145.90	169.0
147.80	241.0
154.80	153.0
157.10	250.0
160.30	102.0
161.00	242.0
170.70	104.0
171.30	137.0
173.00	1021.0
174.00	71112.0
175.00	5407.0
176.00	68104.0
177.00	4408.0
177.90	157.0
206.90	154.0
208.30	120.0
229.50	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
36.00	1481.0
37.00	8063.0
38.00	7464.0
39.00	3049.0
40.00	521.0
41.00	242.0
42.90	485.0
44.00	2036.0
44.90	1520.0
46.20	156.0
47.10	1604.0
47.90	785.0
49.00	5708.0
50.00	26888.0
51.00	7442.0
52.00	360.0
54.90	452.0
56.00	2575.0
57.00	4225.0
57.90	172.0
60.00	1247.0
61.00	6103.0
62.00	6375.0
63.00	4878.0
63.90	462.0
66.30	104.0
67.00	345.0
68.00	12937.0
69.00	13070.0
70.00	847.0
71.90	875.0
73.00	5903.0
74.00	22712.0
75.00	59840.0
76.00	5258.0
77.00	985.0
78.00	748.0
78.90	5263.0
79.90	1470.0
80.90	6453.0
81.90	1272.0
82.80	128.0
84.00	196.0
87.00	4099.0
87.90	3716.0
90.00	100.0
90.90	576.0
92.00	3139.0
93.00	5317.0
94.00	13717.0
95.00	98704.0
96.00	6771.0
97.00	463.0
102.70	137.0
103.90	691.0
104.80	199.0
105.90	762.0
107.00	104.0
110.80	248.0
112.80	163.0
115.00	172.0
116.00	481.0
116.90	556.0
117.90	660.0
118.90	588.0
128.00	460.0
129.10	317.0
130.00	501.0
130.70	243.0
134.90	194.0
137.00	117.0
140.90	1482.0
141.90	149.0
142.90	1474.0
144.80	142.0
145.90	208.0
147.80	167.0
153.00	107.0
154.80	195.0
157.00	183.0
161.00	220.0
171.70	194.0
173.00	1206.0
174.00	76472.0
175.00	5312.0
176.00	75184.0
177.00	4793.0
177.90	181.0
208.30	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
36.00	1478.0
37.00	7378.0
38.00	6950.0
39.00	2678.0
40.00	485.0
41.10	273.0
41.90	120.0
42.90	525.0
44.00	2367.0
44.90	1392.0
46.10	174.0
47.10	1421.0
48.00	739.0
49.00	5741.0
50.00	24856.0
51.00	6950.0
52.00	375.0
53.80	115.0
55.00	465.0
56.00	2471.0
57.00	3842.0
57.90	228.0
58.60	132.0
60.00	1136.0
61.00	6012.0
62.00	5894.0
63.00	4719.0
64.10	422.0
67.10	359.0
68.00	12032.0
69.00	12461.0
70.00	772.0
70.80	102.0
71.90	734.0
73.00	5314.0
74.00	21416.0
75.00	56640.0
76.00	5303.0
77.10	731.0
78.00	686.0
79.00	5019.0
79.90	1256.0
80.90	6127.0
81.90	1131.0
82.80	130.0
84.10	123.0
86.00	105.0
87.00	3727.0
87.90	3559.0
89.00	123.0
90.90	657.0
92.00	2776.0
93.00	5084.0
94.00	13155.0
95.00	93744.0
96.00	6158.0
96.90	419.0
102.80	116.0
103.90	640.0
104.80	261.0
105.90	771.0
106.90	213.0
109.90	150.0
110.80	248.0
112.90	213.0
114.90	199.0
116.00	506.0
116.90	570.0
117.90	467.0
118.80	667.0
128.00	448.0
129.10	264.0
130.00	353.0
130.80	209.0
134.80	185.0
137.00	165.0
140.90	1285.0
141.80	167.0
143.00	1294.0
144.00	140.0
144.80	124.0
145.90	191.0
147.70	128.0
154.90	248.0
156.90	223.0
159.10	122.0
161.00	154.0
171.70	212.0
173.10	1477.0
174.00	73840.0
175.00	5079.0
176.00	74024.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

177.004775.0

177.90197.0

Instrument :
MSVOA_U

ClientSampleId :
BFB35

Scan 2847 (10.244 min): VU034678.D
BFB35

m/z	Abundance
38.50	117.0
39.90	552.0
41.00	233.0
41.90	205.0
42.90	312.0
44.00	1196.0
45.20	164.0
51.00	167.0
52.70	154.0
66.80	152.0
81.70	123.0
207.00	117.0
208.10	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35