

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
 Data File : VU044704.D
 Acq On : 20 Sep 2021 13:15
 Operator : SY/MD
 Sample : M3790-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CM1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	75	81	91	rVB	20681	22550	3.85%	0.900%
2	1.919	172	180	192	rBV	28338	36894	6.30%	1.472%
3	2.572	372	383	396	rBV2	32304	52039	8.88%	2.076%
4	2.652	398	408	416	rBV2	3659	7693	1.31%	0.307%
5	3.054	523	533	545	rVB4	6746	12518	2.14%	0.500%
6	4.645	1013	1028	1070	rBV	48328	216933	37.02%	8.656%
7	5.073	1144	1161	1189	rVB	59850	134377	22.93%	5.362%
8	5.732	1345	1366	1391	rBV2	94874	268988	45.91%	10.733%
9	6.256	1514	1529	1550	rBV	96468	182432	31.14%	7.280%
10	6.697	1652	1666	1685	rBV	77074	149090	25.45%	5.949%
11	7.571	1926	1938	1958	rBV	21996	38061	6.50%	1.519%
12	7.903	2029	2041	2055	rBV	74705	126645	21.61%	5.053%
13	7.976	2055	2064	2074	rVB2	8805	14653	2.50%	0.585%
14	8.185	2119	2129	2145	rBV2	13403	23281	3.97%	0.929%
15	8.648	2259	2273	2310	rBV	213458	585917	100.00%	23.380%
16	8.796	2313	2319	2330	rVB6	4630	7870	1.34%	0.314%
17	9.423	2502	2514	2534	rBV	125117	212874	36.33%	8.494%
18	10.118	2720	2730	2740	rBV4	5834	9748	1.66%	0.389%
19	10.761	2918	2930	2945	rBV	72124	118773	20.27%	4.739%
20	11.819	3247	3259	3274	rBV	95680	156167	26.65%	6.231%
21	12.198	3366	3377	3395	rBV	80778	128591	21.95%	5.131%




Sum of corrected areas: 2506094

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044704.D
Acq On : 20 Sep 2021 13:15
Operator : SY/MD
Sample : M3790-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

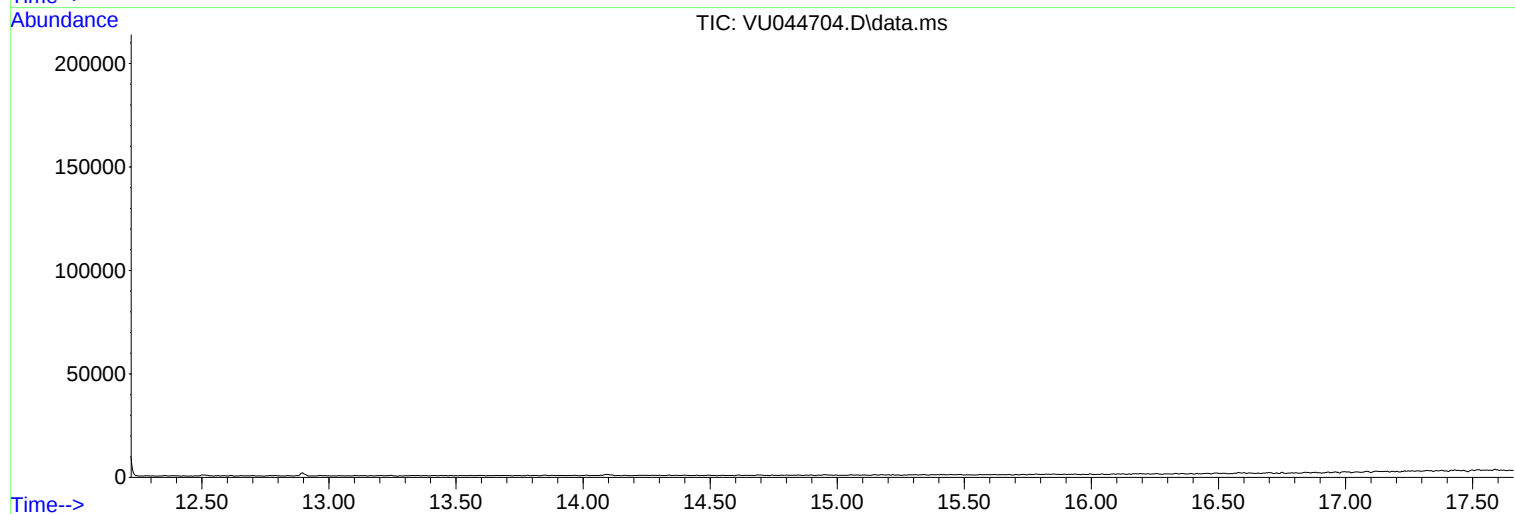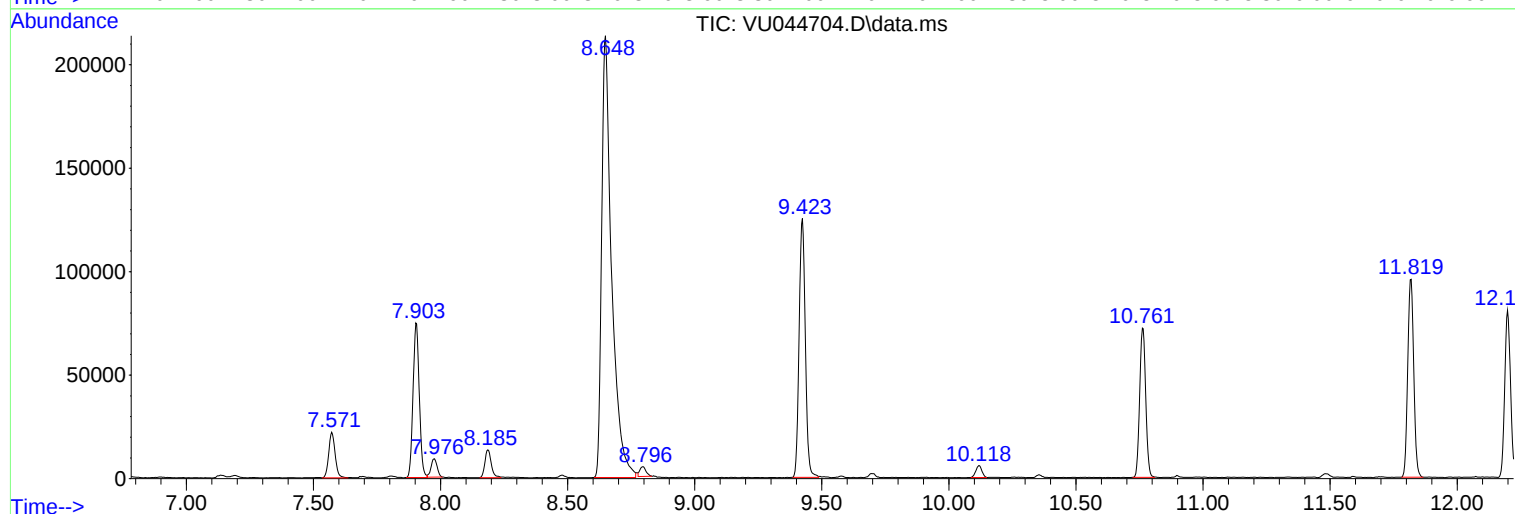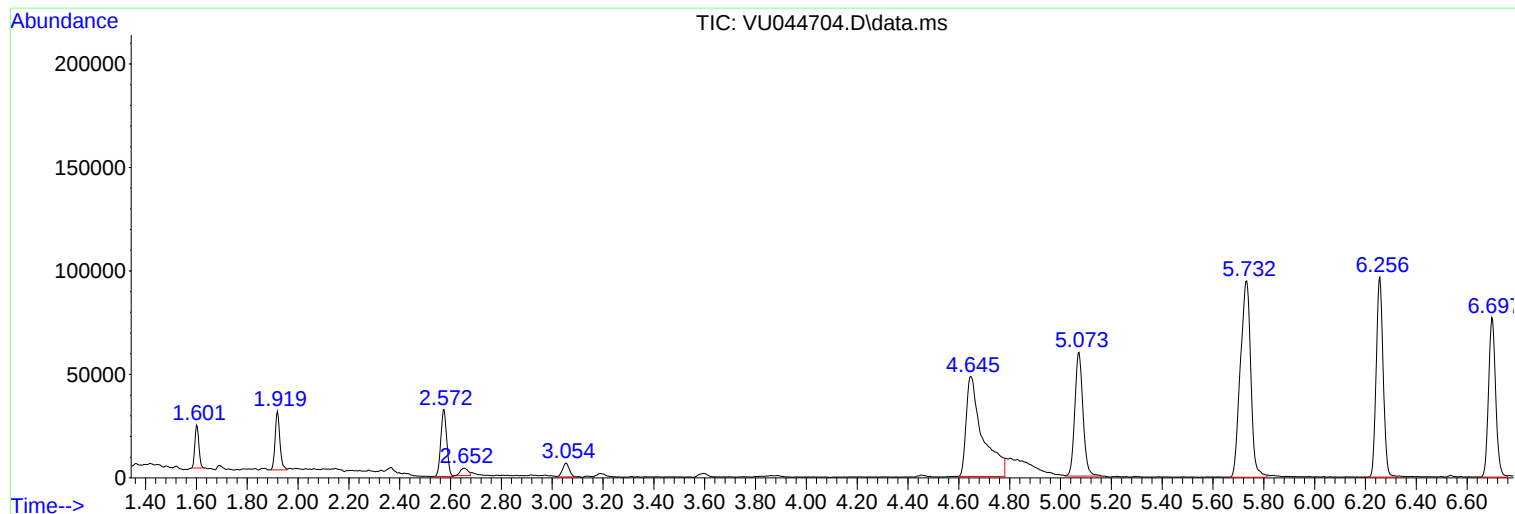

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044704.D
Acq On : 20 Sep 2021 13:15
Operator : SY/MD
Sample : M3790-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044704.D
Acq On : 20 Sep 2021 13:15
Operator : SY/MD
Sample : M3790-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
