

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
 Data File : VU044707.D
 Acq On : 20 Sep 2021 14:28
 Operator : SY/MD
 Sample : M3739-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	95	rVB	50450	58044	10.88%	1.324%
2	1.919	171	180	190	rBV	41639	55376	10.38%	1.263%
3	2.571	370	383	399	rBV	78216	128094	24.00%	2.922%
4	4.645	1012	1028	1054	rBV	39925	145127	27.20%	3.310%
5	5.073	1145	1161	1183	rBV	84091	197622	37.03%	4.508%
6	5.732	1345	1366	1388	rBV2	146178	385314	72.21%	8.789%
7	6.256	1514	1529	1550	rBV	167422	317772	59.55%	7.249%
8	6.697	1652	1666	1681	rBV	97310	190774	35.75%	4.352%
9	7.571	1926	1938	1960	rBV	44263	79893	14.97%	1.822%
10	7.722	1977	1985	1996	rVB5	3724	6796	1.27%	0.155%
11	7.902	2029	2041	2052	rBV	163036	280330	52.53%	6.394%
12	7.973	2052	2063	2093	rVB	202357	350522	65.69%	7.996%
13	8.185	2117	2129	2150	rBV2	27096	47222	8.85%	1.077%
14	8.645	2258	2272	2312	rBV	204492	533624	100.00%	12.172%
15	9.423	2501	2514	2532	rBV	247040	413413	77.47%	9.430%
16	9.574	2548	2561	2580	rBV	42333	68831	12.90%	1.570%
17	9.697	2587	2599	2617	rBV	146171	244453	45.81%	5.576%
18	10.105	2714	2726	2746	rBV	74415	122235	22.91%	2.788%
19	10.761	2918	2930	2947	rVB	78330	126483	23.70%	2.885%
20	11.815	3246	3258	3273	rBV	232957	369217	69.19%	8.422%
21	12.198	3364	3377	3393	rBV	162732	262783	49.24%	5.994%




Sum of corrected areas: 4383925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044707.D
Acq On : 20 Sep 2021 14:28
Operator : SY/MD
Sample : M3739-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

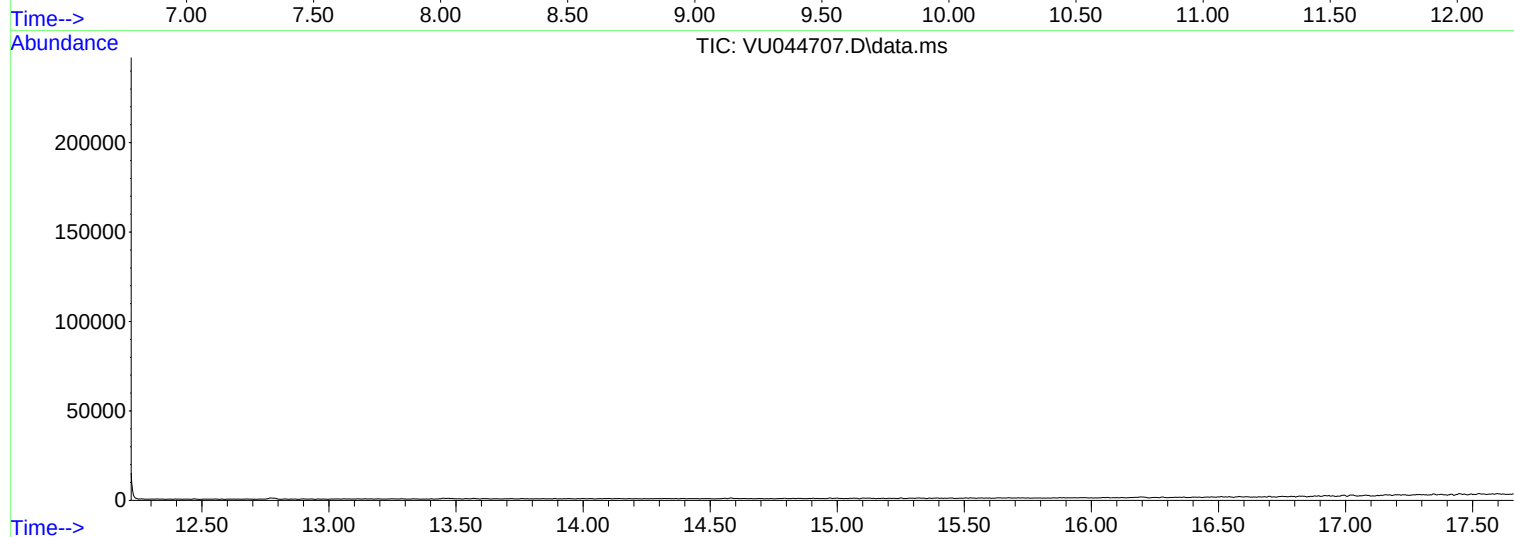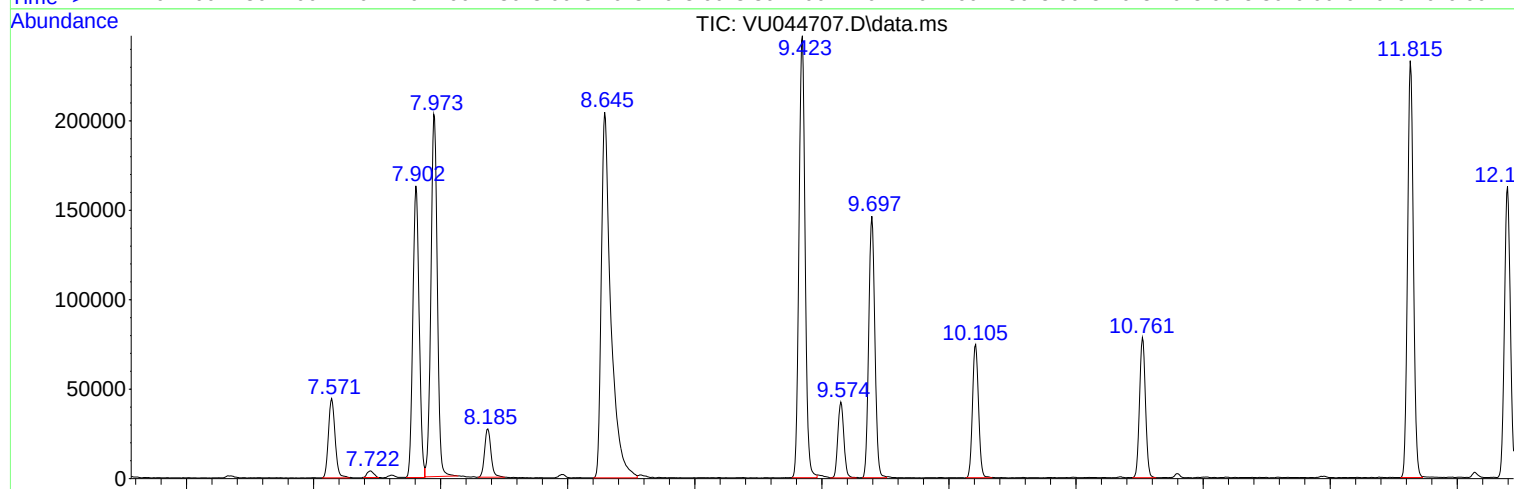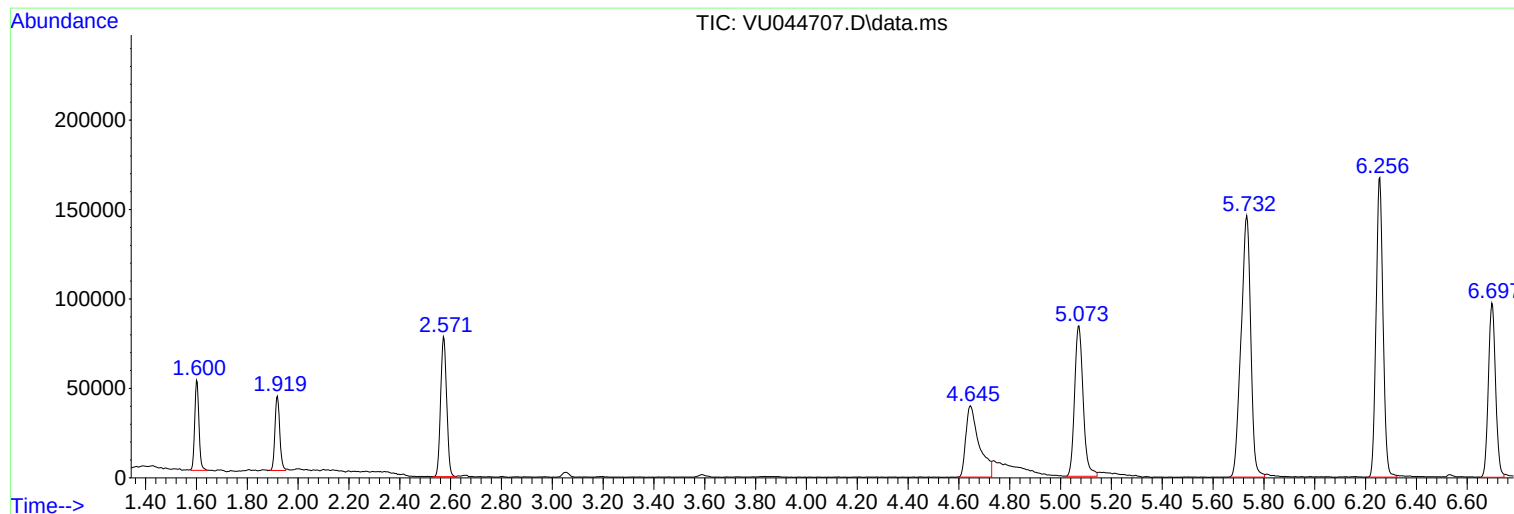

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044707.D
Acq On : 20 Sep 2021 14:28
Operator : SY/MD
Sample : M3739-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044707.D
Acq On : 20 Sep 2021 14:28
Operator : SY/MD
Sample : M3739-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
