

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
 Data File : VU044708.D
 Acq On : 20 Sep 2021 14:51
 Operator : SY/MD
 Sample : M3790-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CM1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	95	rVB	49153	55436	11.10%	1.612%
2	1.919	172	180	198	rBV	40296	52537	10.52%	1.528%
3	2.572	371	383	397	rBV	76710	125465	25.13%	3.648%
4	2.649	399	407	425	rVV2	2992	7265	1.45%	0.211%
5	4.645	1012	1028	1045	rBV2	36567	116798	23.39%	3.396%
6	5.070	1145	1160	1180	rBV	72757	160691	32.18%	4.673%
7	5.732	1344	1366	1393	rBV2	142692	373932	74.89%	10.873%
8	6.256	1514	1529	1550	rBV	158415	302824	60.65%	8.806%
9	6.697	1653	1666	1689	rBV	93165	183785	36.81%	5.344%
10	7.571	1924	1938	1958	rBV	42460	76157	15.25%	2.215%
11	7.903	2028	2041	2054	rBV	153392	269025	53.88%	7.823%
12	7.976	2054	2064	2075	rVB2	15418	26416	5.29%	0.768%
13	8.185	2118	2129	2142	rBV	26206	45186	9.05%	1.314%
14	8.645	2258	2272	2310	rBV	186634	499337	100.00%	14.520%
15	8.793	2312	2318	2332	rVB5	4421	7788	1.56%	0.226%
16	9.420	2500	2513	2535	rBV	233647	389854	78.07%	11.336%
17	9.697	2589	2599	2610	rBV3	7048	10943	2.19%	0.318%
18	10.118	2717	2730	2742	rBV4	14675	25631	5.13%	0.745%
19	10.761	2918	2930	2945	rBV	73821	119791	23.99%	3.483%
20	11.816	3246	3258	3276	rBV	218015	342327	68.56%	9.954%
21	12.195	3364	3376	3393	rVB	148568	247771	49.62%	7.205%




Sum of corrected areas: 3438959

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044708.D
Acq On : 20 Sep 2021 14:51
Operator : SY/MD
Sample : M3790-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

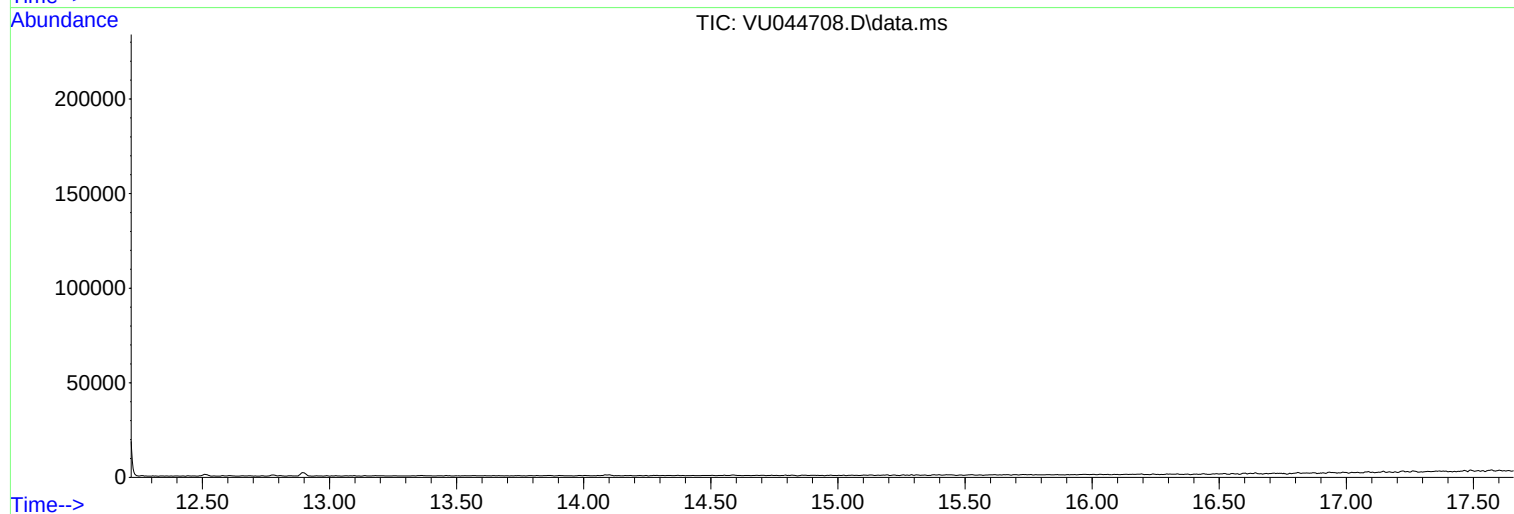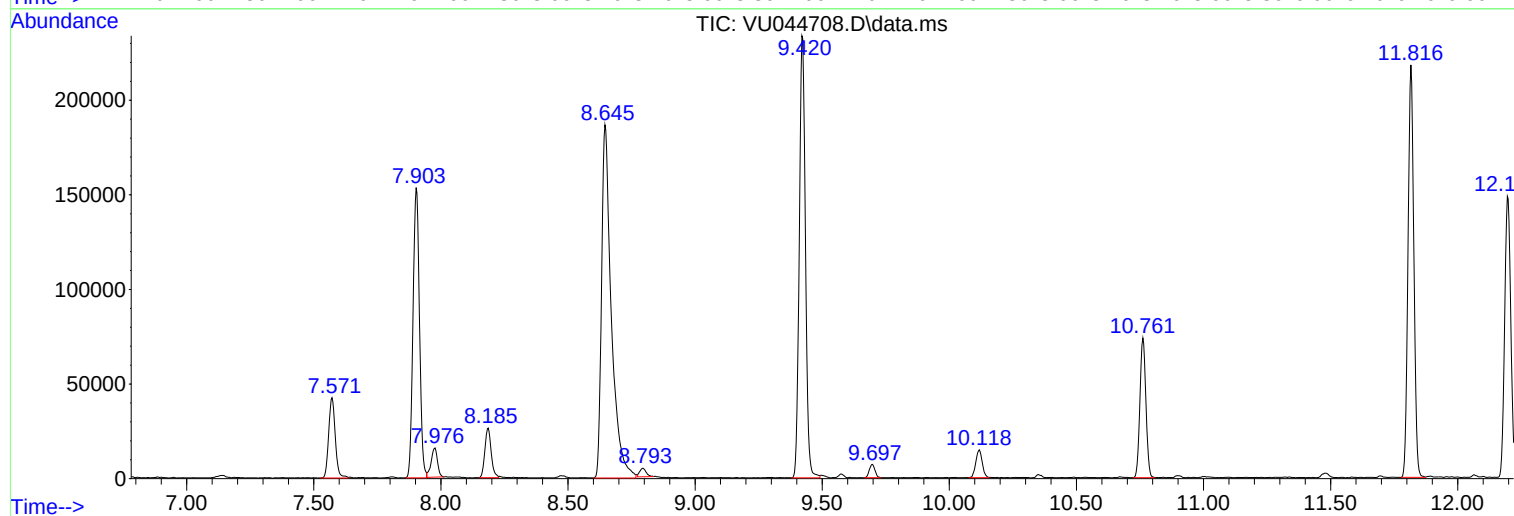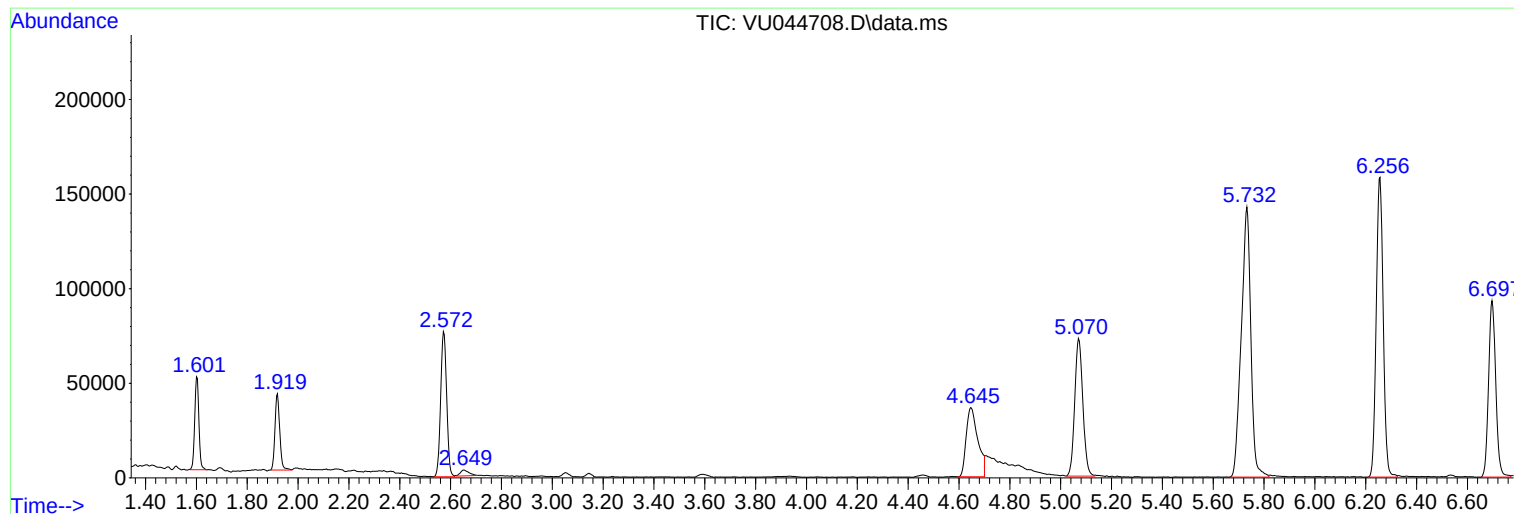

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044708.D
Acq On : 20 Sep 2021 14:51
Operator : SY/MD
Sample : M3790-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044708.D
Acq On : 20 Sep 2021 14:51
Operator : SY/MD
Sample : M3790-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
