

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
 Data File : VU044723.D
 Acq On : 20 Sep 2021 20:54
 Operator : SY/MD
 Sample : M3789-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	91	rBV	27442	29741	5.17%	0.891%
2	1.919	172	180	192	rBB	31846	41428	7.20%	1.241%
3	2.572	368	383	399	rBV2	54040	87182	15.16%	2.612%
4	4.690	1018	1042	1110	rBV2	37529	263190	45.76%	7.886%
5	5.070	1144	1160	1185	rBV	67482	156415	27.20%	4.687%
6	5.732	1346	1366	1393	rBV2	125534	335935	58.41%	10.066%
7	6.256	1514	1529	1551	rBV	150072	284623	49.49%	8.529%
8	6.697	1653	1666	1684	rBV	89233	174959	30.42%	5.243%
9	7.571	1926	1938	1953	rBV2	24805	42833	7.45%	1.283%
10	7.903	2027	2041	2054	rBV	127195	219375	38.14%	6.573%
11	7.973	2054	2063	2077	rVB	14207	23561	4.10%	0.706%
12	8.185	2118	2129	2145	rVB2	15467	25922	4.51%	0.777%
13	8.648	2259	2273	2309	rBV	246901	575145	100.00%	17.234%
14	8.793	2310	2318	2332	rVB5	4811	9108	1.58%	0.273%
15	9.420	2501	2513	2539	rBV	222472	374434	65.10%	11.220%
16	9.697	2590	2599	2610	rBB3	5448	8409	1.46%	0.252%
17	10.118	2715	2730	2742	rBV3	13393	22898	3.98%	0.686%
18	10.761	2915	2930	2945	rVB	79525	127765	22.21%	3.828%
19	11.816	3247	3258	3277	rBV	199654	315494	54.85%	9.454%
20	12.198	3365	3377	3395	rBV	136593	218868	38.05%	6.558%




Sum of corrected areas: 3337285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044723.D
Acq On : 20 Sep 2021 20:54
Operator : SY/MD
Sample : M3789-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

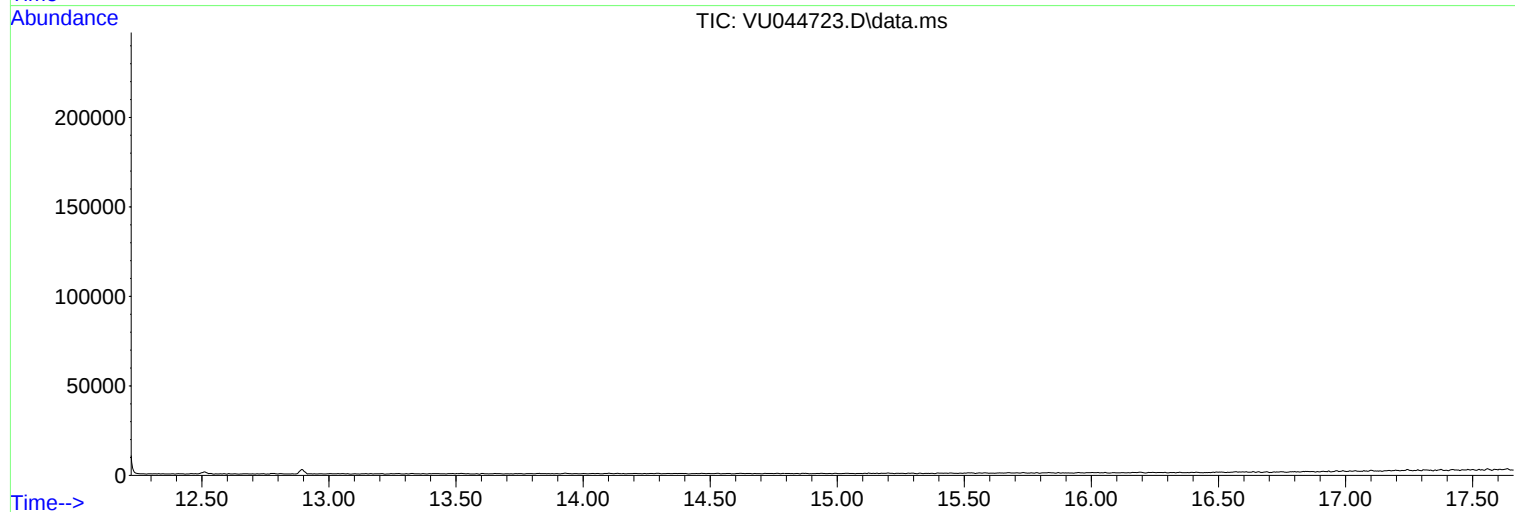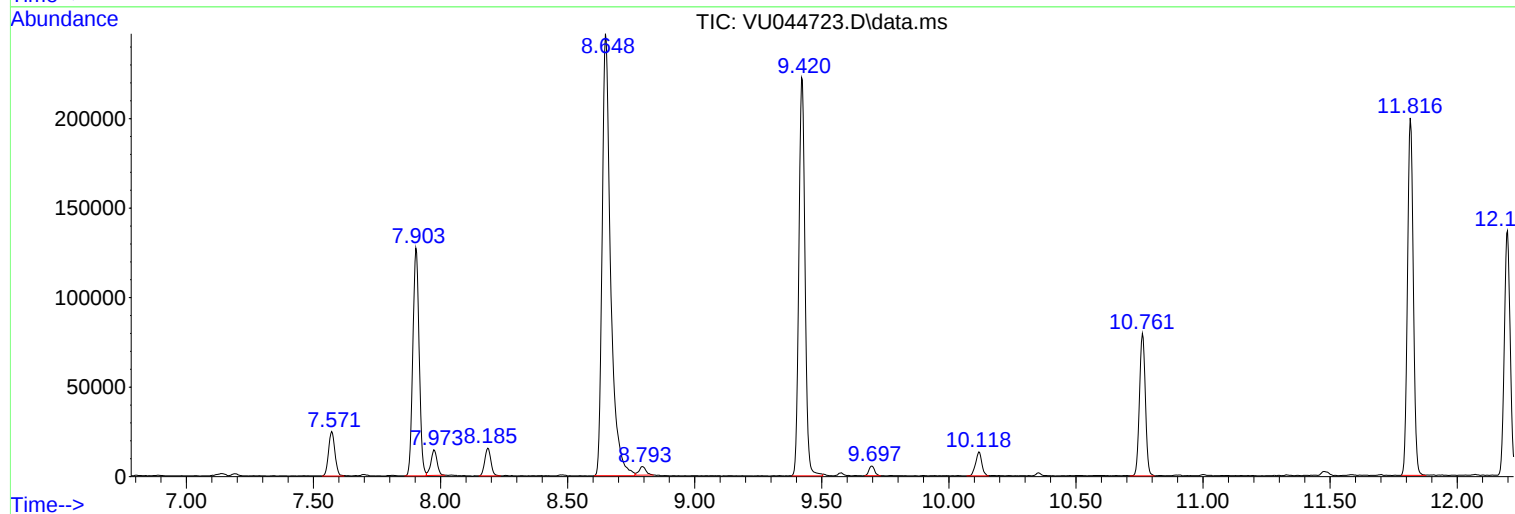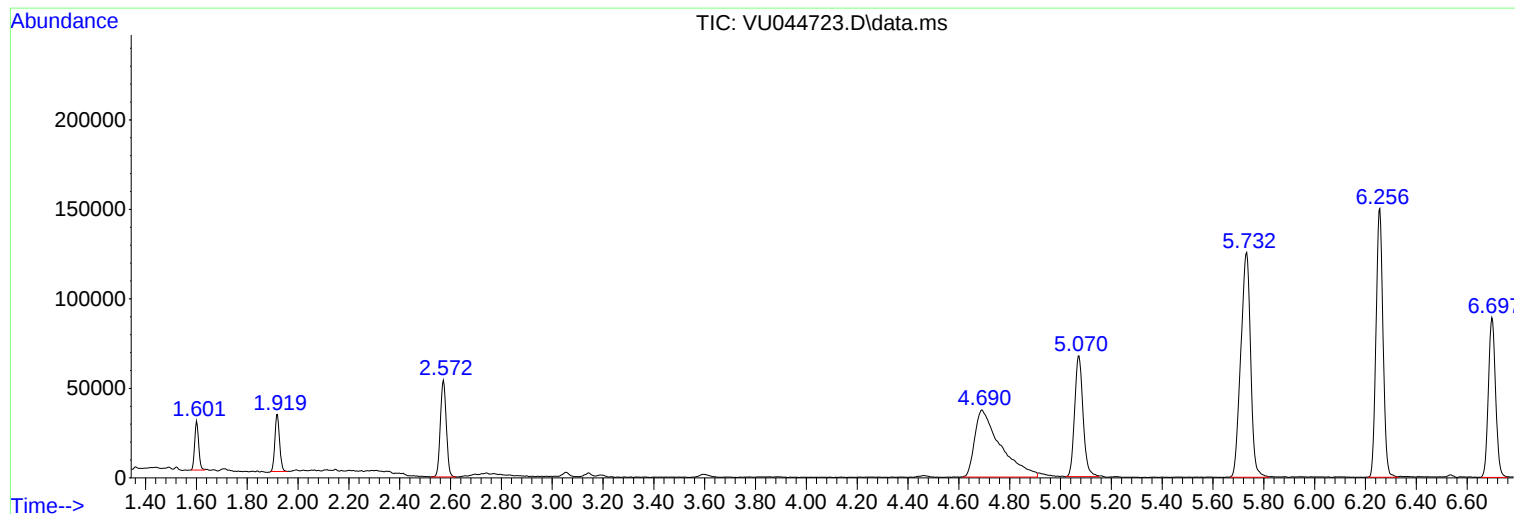

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044723.D
Acq On : 20 Sep 2021 20:54
Operator : SY/MD
Sample : M3789-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
Data File : VU044723.D
Acq On : 20 Sep 2021 20:54
Operator : SY/MD
Sample : M3789-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
