


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092021\
 Data File : VU044701.D
 Acq On : 20 Sep 2021 09:40
 Operator : SY/MD
 Sample : BFB021
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB021

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Sep 22 01:40:07 2021

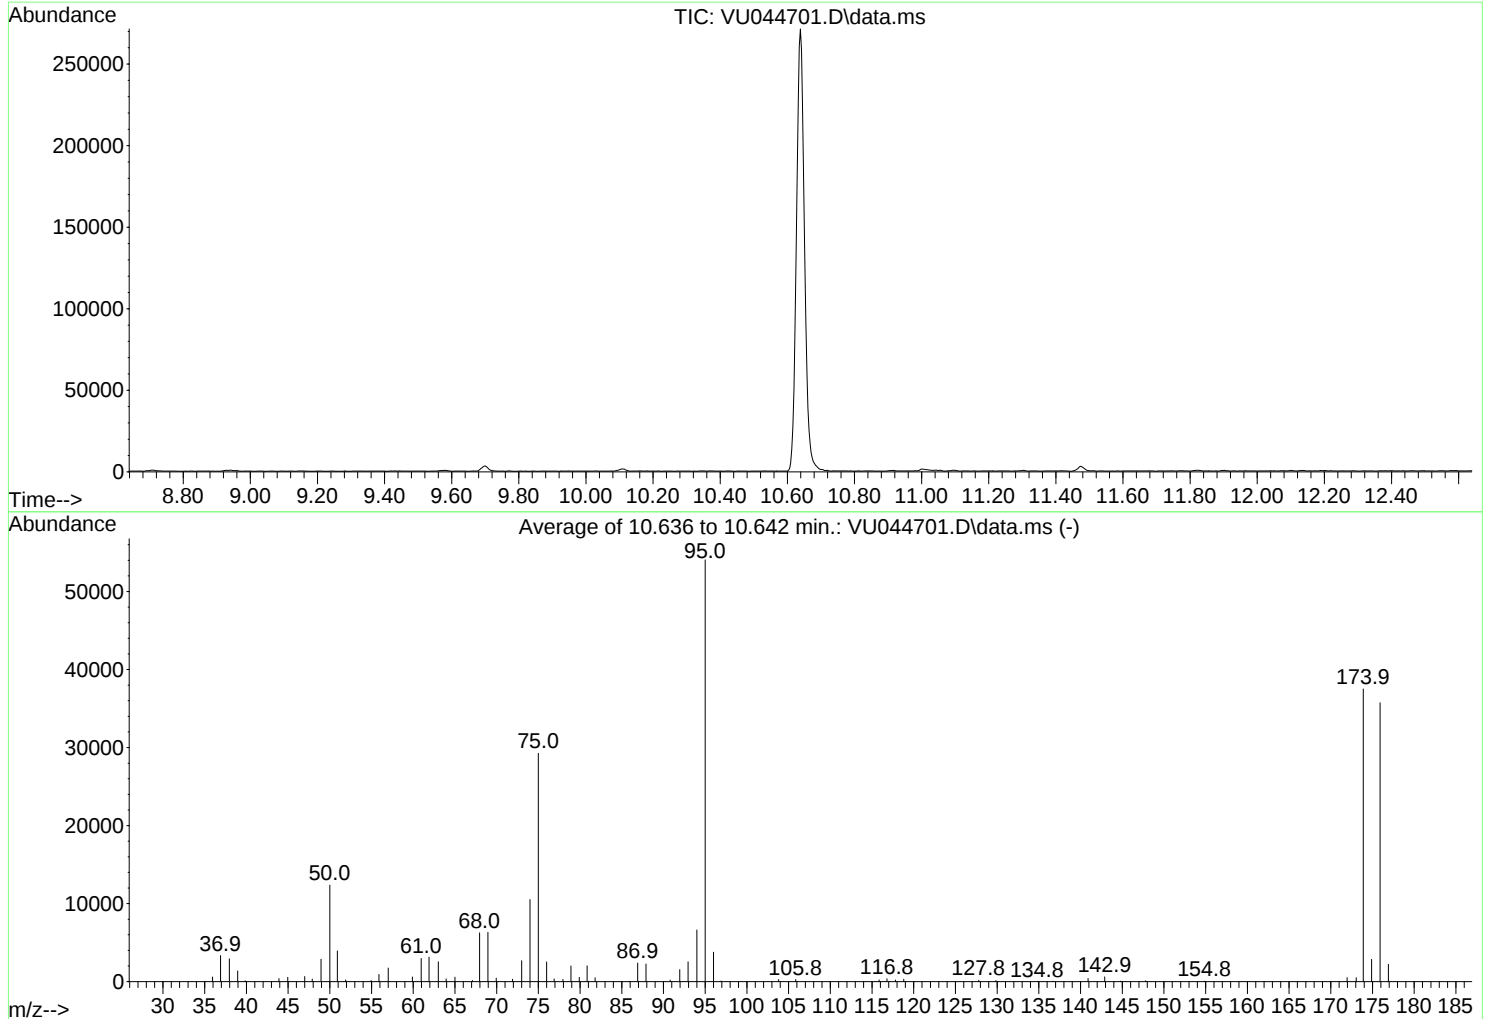

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	12375	PASS
75	95	30	80	54.1	29267	PASS
95	95	100	100	100.0	54056	PASS
96	95	5	9	7.0	3781	PASS
173	174	0.00	2	1.4	522	PASS
174	95	50	120	69.4	37509	PASS
175	174	5	9	7.6	2858	PASS
176	174	95	101	95.3	35744	PASS
177	176	5	9	6.2	2220	PASS

Scan 2878 (10.594 min): VU044701.D\data.ms
BFB021

m/z	Abundance
39.80	117.0
43.90	339.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.90	614.0
36.90	3462.0
38.00	3024.0
38.90	1418.0
39.90	236.0
43.90	727.0
45.00	559.0
47.00	649.0
47.90	355.0
49.00	2945.0
50.00	12403.0
50.90	4096.0
51.90	239.0
55.00	160.0
55.90	936.0
57.00	1717.0
59.90	617.0
61.00	3006.0
61.90	3138.0
63.00	2625.0
64.00	400.0
65.00	513.0
67.10	149.0
68.00	6254.0
69.00	6123.0
69.90	507.0
71.90	298.0
73.00	2823.0
74.00	10322.0
75.00	28960.0
76.00	2603.0
76.90	395.0
77.90	266.0
78.90	1957.0
79.90	592.0
80.80	2000.0
81.80	524.0
85.90	100.0
86.90	2384.0
87.90	2299.0
90.80	186.0
92.00	1485.0
93.00	2604.0
94.00	6584.0
95.00	53520.0
96.00	3693.0
96.90	147.0
103.80	270.0
105.80	228.0
115.90	243.0
116.80	387.0
117.80	198.0
118.80	333.0
127.80	174.0
129.90	138.0
136.70	106.0
140.90	383.0
142.90	619.0
144.80	102.0
147.80	101.0
154.80	105.0
172.00	458.0
173.10	454.0
173.90	36640.0
174.90	2878.0
175.90	34336.0
176.90	2230.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
35.90	611.0
36.90	3453.0
38.00	3018.0
38.90	1420.0
39.90	217.0
43.90	721.0
44.90	576.0
47.00	695.0
47.90	330.0
49.00	2919.0
50.00	12730.0
50.90	4088.0
51.90	245.0
54.90	133.0
55.90	956.0
57.00	1800.0
59.90	620.0
61.00	3016.0
61.90	3289.0
63.00	2629.0
64.00	337.0
65.00	587.0
67.10	148.0
68.00	6445.0
69.00	6518.0
70.00	447.0
71.90	332.0
73.00	2774.0
74.00	10860.0
75.00	30176.0
76.00	2598.0
76.90	378.0
77.90	306.0
78.90	2095.0
79.90	574.0
80.80	2111.0
81.80	501.0
86.90	2412.0
87.90	2337.0
90.80	204.0
91.90	1567.0
92.90	2609.0
94.00	6844.0
95.00	55688.0
96.00	3943.0
96.90	118.0
103.80	268.0
105.90	276.0
115.90	243.0
116.80	379.0
117.80	198.0
118.80	333.0
127.80	179.0
129.90	150.0
136.70	103.0
140.90	419.0
142.90	632.0
147.80	129.0
171.90	509.0
173.00	573.0
173.90	38616.0
174.90	2957.0
175.90	36840.0
176.90	2304.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
36.00	537.0
36.90	3133.0
37.90	2755.0
39.00	1312.0
39.90	207.0
43.90	709.0
44.90	559.0
47.00	647.0
47.90	311.0
48.90	2731.0
50.00	11992.0
50.90	3624.0
51.90	218.0
54.90	113.0
55.90	908.0
57.00	1734.0
59.90	546.0
60.90	2922.0
61.90	3016.0
63.00	2381.0
63.90	301.0
65.00	609.0
67.10	142.0
67.90	6097.0
68.90	6341.0
70.00	379.0
71.90	322.0
73.00	2465.0
74.00	10369.0
75.00	28664.0
76.00	2371.0
76.90	285.0
78.00	278.0
78.90	1965.0
79.90	530.0
80.90	1971.0
81.80	439.0
86.90	2364.0
87.90	2129.0
90.80	203.0
91.90	1540.0
92.90	2432.0
94.00	6452.0
95.00	52960.0
96.00	3707.0
103.80	236.0
105.90	280.0
115.80	219.0
116.80	360.0
117.80	202.0
118.80	281.0
127.80	189.0
129.80	153.0
134.80	104.0
140.90	448.0
142.90	574.0
144.80	107.0
147.80	148.0
154.90	103.0
171.90	548.0
173.00	539.0
173.90	37272.0
174.90	2739.0
175.90	36056.0
176.90	2125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021