

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092023\
 Data File : VU055421.D
 Acq On : 20 Sep 2023 13:32
 Operator : MD/SY
 Sample : 04398-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4Q0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	108	rBV2	259781	317460	3.45%	1.167%
2	1.911	185	193	209	rBV	144165	186961	2.03%	0.687%
3	2.570	384	398	417	rBV3	419766	833315	9.05%	3.064%
4	3.865	786	801	817	rBV	42768	106299	1.15%	0.391%
5	4.660	1022	1048	1092	rBV	3467506	8226598	89.30%	30.249%
6	5.058	1156	1172	1193	rBV	234571	548436	5.95%	2.017%
7	5.724	1355	1379	1396	rBV2	466966	1223640	13.28%	4.499%
8	6.245	1528	1541	1568	rBV	300633	586622	6.37%	2.157%
9	6.537	1616	1632	1667	rBV	4876052	9212634	100.00%	33.874%
10	6.689	1667	1679	1709	rVB	289504	599087	6.50%	2.203%
11	7.563	1938	1951	1974	rBV	140770	255863	2.78%	0.941%
12	7.894	2041	2054	2072	rBV	572592	1014182	11.01%	3.729%
13	8.177	2125	2142	2163	rBV	83880	149464	1.62%	0.550%
14	8.550	2247	2258	2273	rBV	89934	151457	1.64%	0.557%
15	8.634	2273	2284	2321	rBV4	406926	1031356	11.20%	3.792%
16	9.415	2513	2527	2550	rBV	450180	782262	8.49%	2.876%
17	10.753	2929	2943	2961	rBV	198199	326682	3.55%	1.201%
18	11.810	3260	3272	3294	rBV	467904	778163	8.45%	2.861%
19	12.190	3376	3390	3412	rBV	512581	865977	9.40%	3.184%




Sum of corrected areas: 27196458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092023\
Data File : VU055421.D
Acq On : 20 Sep 2023 13:32
Operator : MD/SY
Sample : 04398-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4Q0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

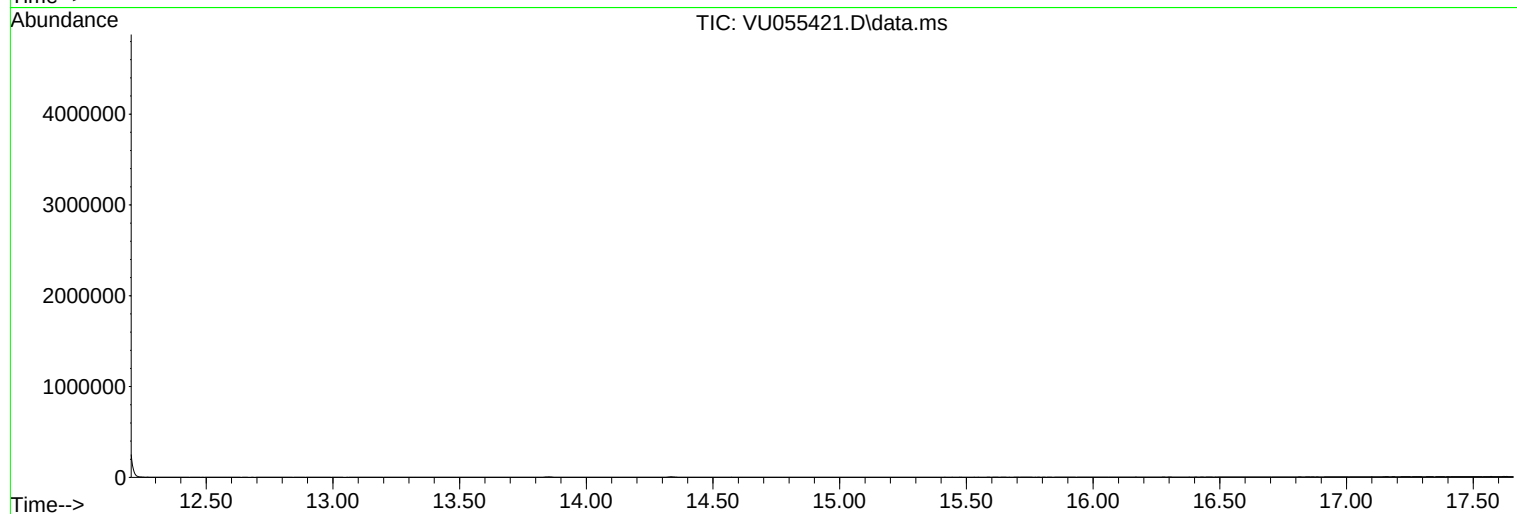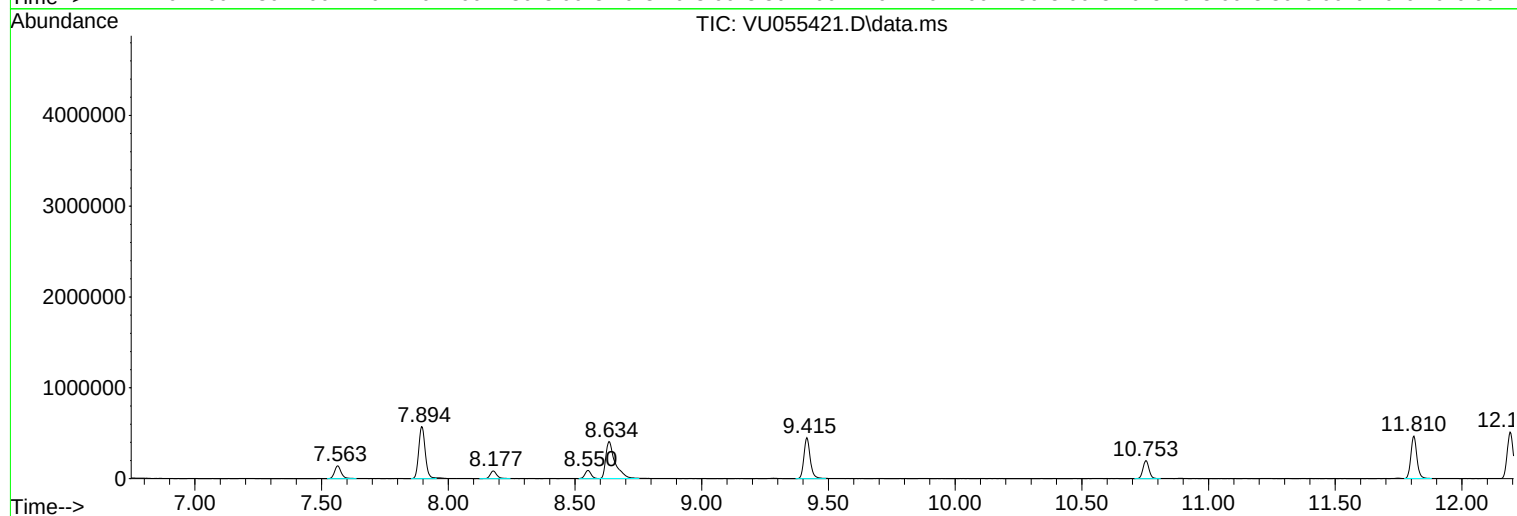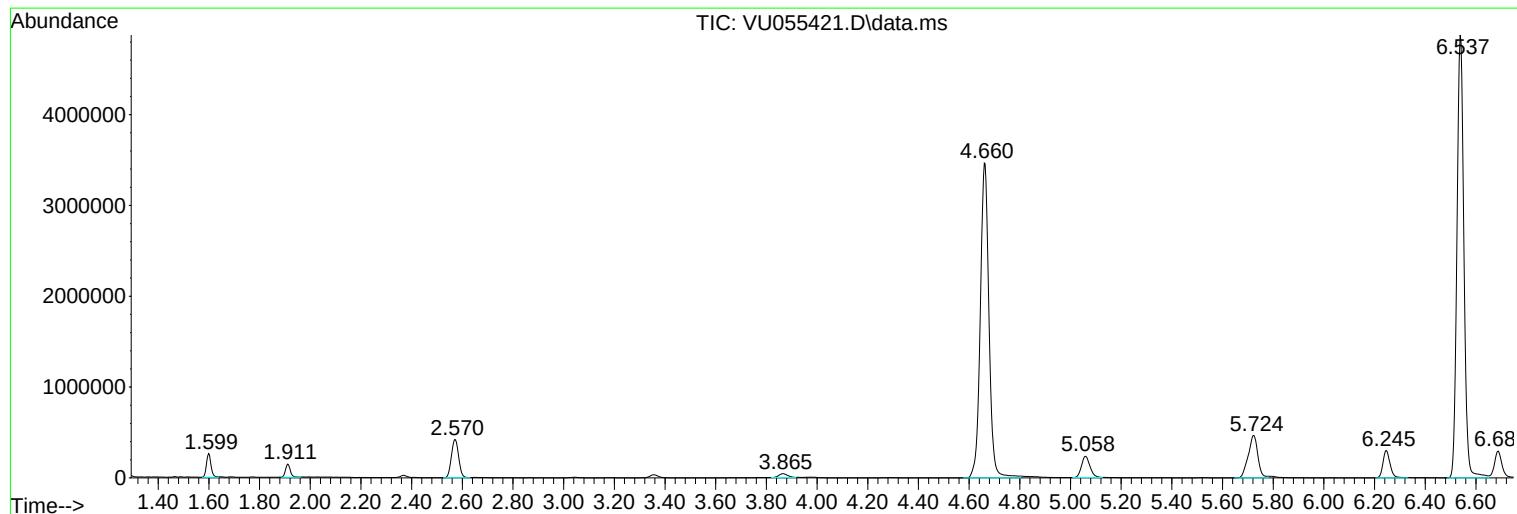

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092023\
Data File : VU055421.D
Acq On : 20 Sep 2023 13:32
Operator : MD/SY
Sample : 04398-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4Q0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092023\
Data File : VU055421.D
Acq On : 20 Sep 2023 13:32
Operator : MD/SY
Sample : 04398-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4Q0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc