

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092023\
 Data File : VU055431.D
 Acq On : 20 Sep 2023 17:42
 Operator : MD/SY
 Sample : 04398-03DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4P3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	111	rVB	174403	207361	16.66%	1.932%
2	1.911	183	193	207	rBV	150110	199362	16.02%	1.858%
3	2.563	383	396	414	rBV2	265584	452647	36.37%	4.218%
4	3.039	528	544	559	rBV2	23574	43243	3.47%	0.403%
5	3.181	575	588	602	rBV2	11600	26742	2.15%	0.249%
6	4.660	1021	1048	1081	rBV3	256810	918503	73.79%	8.560%
7	5.058	1155	1172	1193	rBV	245336	554257	44.53%	5.165%
8	5.721	1355	1378	1399	rBV2	475046	1244730	100.00%	11.600%
9	6.245	1528	1541	1563	rBV	312137	601796	48.35%	5.608%
10	6.541	1619	1633	1655	rBV3	309187	601708	48.34%	5.608%
11	6.689	1665	1679	1700	rBV	292903	574153	46.13%	5.351%
12	7.563	1935	1951	1982	rBV	137764	259351	20.84%	2.417%
13	7.897	2042	2055	2086	rBV	570489	1029345	82.70%	9.593%
14	8.177	2129	2142	2167	rBV2	84560	152307	12.24%	1.419%
15	8.634	2272	2284	2317	rBV5	426056	1069014	85.88%	9.962%
16	9.415	2515	2527	2551	rBV	463497	801862	64.42%	7.473%
17	10.753	2931	2943	2963	rBV	210569	338152	27.17%	3.151%
18	11.811	3260	3272	3304	rBV	484983	785989	63.15%	7.325%
19	12.190	3376	3390	3415	rBV	526528	869863	69.88%	8.107%




Sum of corrected areas: 10730385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092023\
Data File : VU055431.D
Acq On : 20 Sep 2023 17:42
Operator : MD/SY
Sample : 04398-03DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4P3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

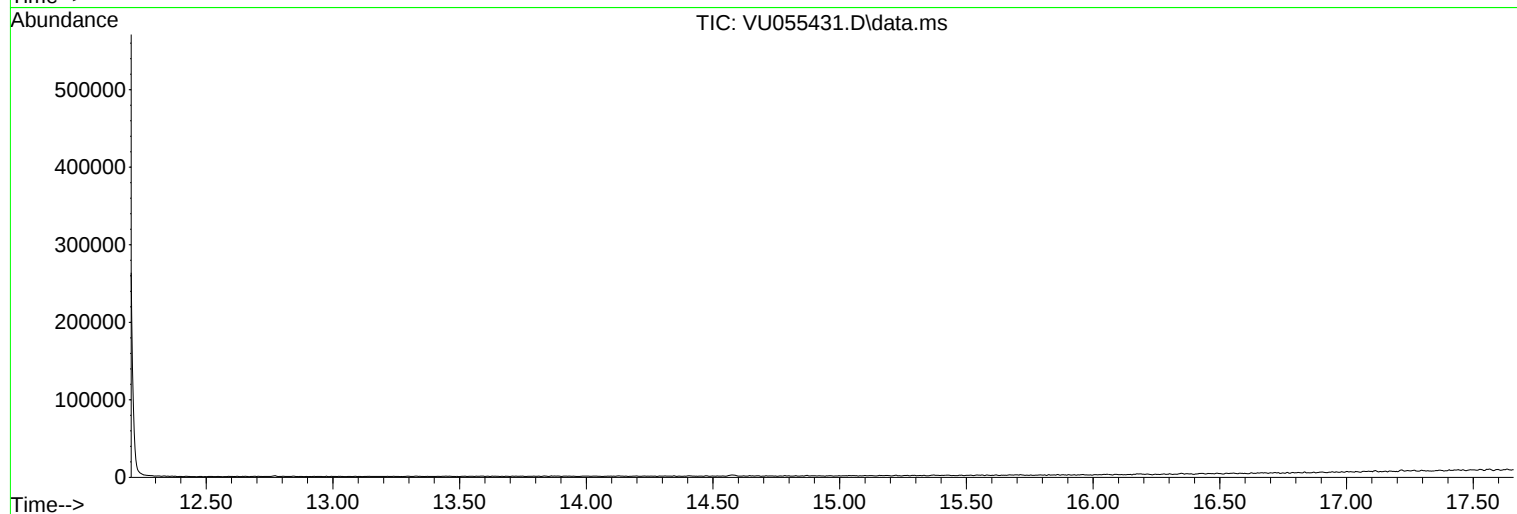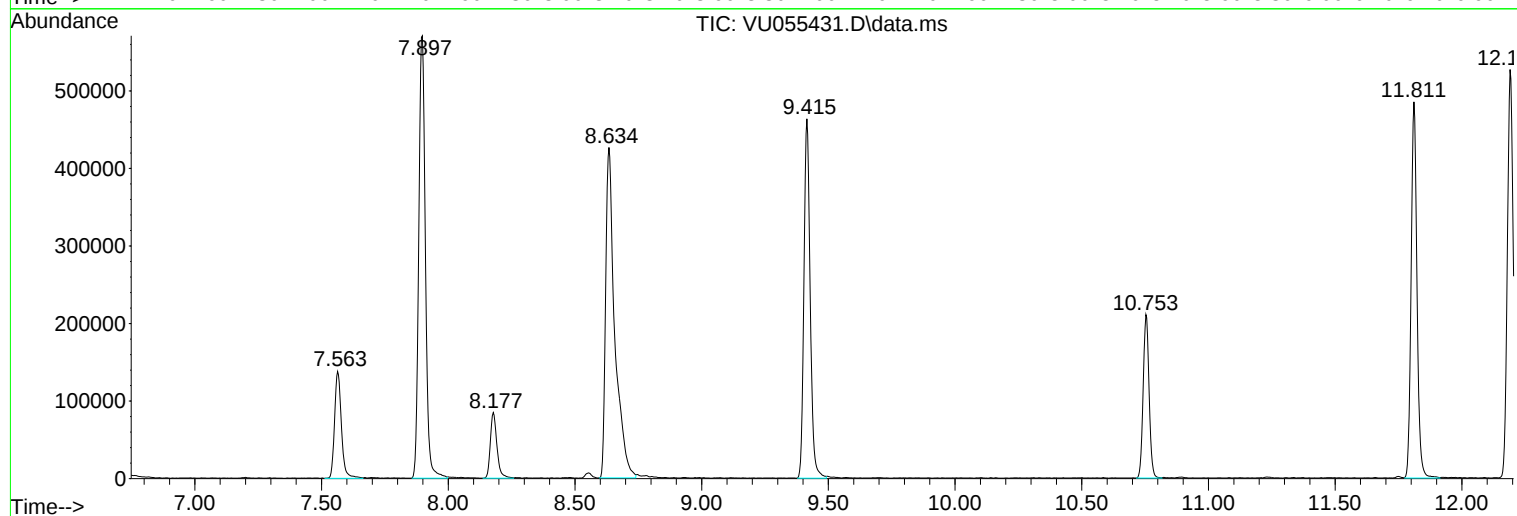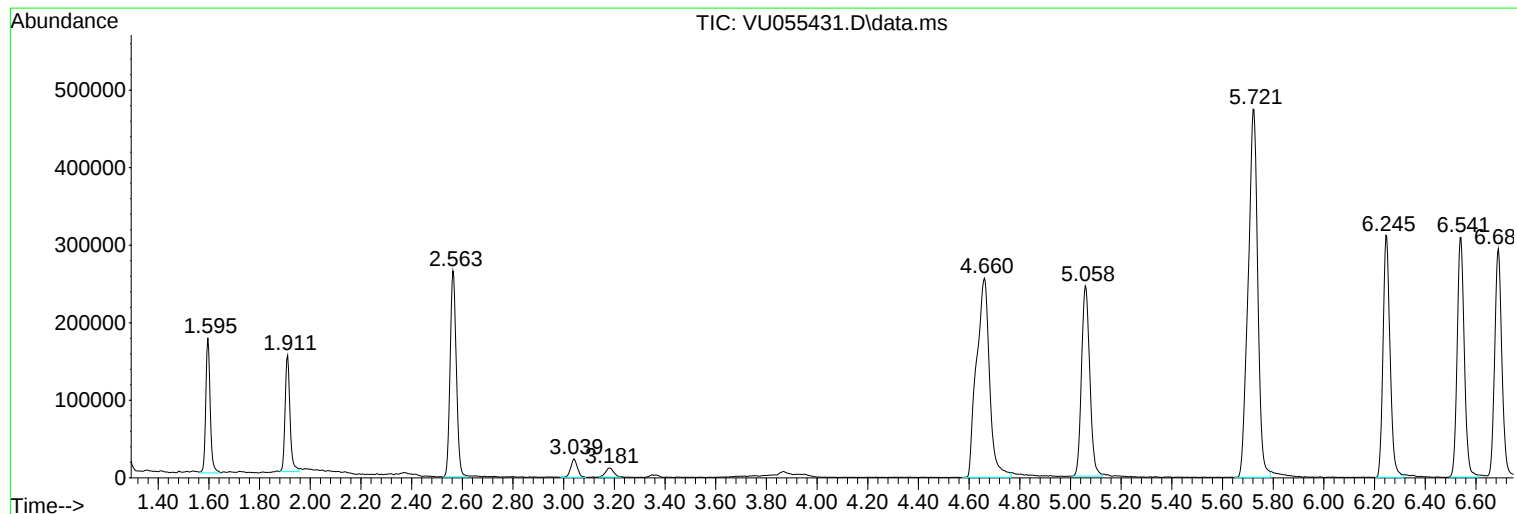

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092023\
Data File : VU055431.D
Acq On : 20 Sep 2023 17:42
Operator : MD/SY
Sample : 04398-03DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4P3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092023\
Data File : VU055431.D
Acq On : 20 Sep 2023 17:42
Operator : MD/SY
Sample : 04398-03DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4P3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc