

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092118\
 Data File : VU026958.D
 Acq On : 21 Sep 2018 01:11
 Operator : MD/SY
 Sample : J5012-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Q4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	62	69	83	rBV	114328	117206	14.75%	2.598%
2	1.669	147	154	173	rVB	93253	121534	15.29%	2.694%
3	2.267	330	340	354	rBV	175349	263520	33.15%	5.841%
4	2.701	469	475	483	rVB3	1045	1567	0.20%	0.035%
5	2.785	499	501	503	rBV	137	79	0.01%	0.002%
6	2.836	506	517	537	rVB2	3768	7857	0.99%	0.174%
7	2.913	537	541	543	rBV2	281	237	0.03%	0.005%
8	3.119	602	605	610	rBV	260	175	0.02%	0.004%
9	3.145	610	613	616	rBV	213	136	0.02%	0.003%
10	3.199	626	630	633	rBV2	195	141	0.02%	0.003%
11	3.293	657	659	665	rVB	167	108	0.01%	0.002%
12	3.328	665	670	674	rBV	143	155	0.02%	0.003%
13	3.370	681	683	684	rBV	171	55	0.01%	0.001%
14	3.457	708	710	712	rVB	136	54	0.01%	0.001%
15	3.498	720	723	725	rBV	113	66	0.01%	0.001%
16	3.511	725	727	734	rVB	120	84	0.01%	0.002%
17	3.643	766	768	771	rBV	156	96	0.01%	0.002%
18	3.675	776	778	780	rVB	134	53	0.01%	0.001%
19	3.765	805	806	811	rVB	164	88	0.01%	0.002%
20	3.791	811	814	815	rBV	131	54	0.01%	0.001%
21	3.826	823	825	827	rVB	180	75	0.01%	0.002%
22	3.855	832	834	836	rBV	150	79	0.01%	0.002%
23	3.875	836	840	843	rVB	236	128	0.02%	0.003%
24	3.897	844	847	849	rBV	141	77	0.01%	0.002%
25	3.984	871	874	877	rBV	117	99	0.01%	0.002%
26	4.064	897	899	903	rBV	69	50	0.01%	0.001%
27	4.116	913	915	916	rBV	142	57	0.01%	0.001%
28	4.177	920	934	964	rBV	78739	208105	26.18%	4.613%
29	4.466	1022	1024	1027	rVB	249	120	0.02%	0.003%
30	4.486	1028	1030	1032	rVB	158	69	0.01%	0.002%
31	4.521	1040	1041	1048	rVB2	271	203	0.03%	0.004%
32	4.646	1062	1080	1102	rBV2	137146	319296	40.17%	7.078%
33	5.000	1187	1190	1194	rVB	113	70	0.01%	0.002%
34	5.023	1194	1197	1202	rVB	186	105	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092118\
 Data File : VU026958.D
 Acq On : 21 Sep 2018 01:11
 Operator : MD/SY
 Sample : J5012-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Q4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

35	5.045	1202	1204	1206	rBV	88	55	0.01%	0.001%
36	5.087	1214	1217	1220	rBV	97	75	0.01%	0.002%
37	5.170	1237	1243	1244	rBV	75	68	0.01%	0.002%
38	5.341	1271	1296	1324	rBV2	264058	794822	100.00%	17.618%
39	5.518	1348	1351	1353	rBV	124	58	0.01%	0.001%
40	5.531	1353	1355	1357	rVB	148	57	0.01%	0.001%
41	5.547	1357	1360	1361	rBV	91	54	0.01%	0.001%
42	5.579	1367	1370	1371	rBV	112	64	0.01%	0.001%
43	5.746	1420	1422	1426	rVB	162	63	0.01%	0.001%
44	5.781	1430	1433	1435	rBV	193	111	0.01%	0.002%
45	5.887	1454	1466	1483	rBV	38226	73225	9.21%	1.623%
46	6.003	1500	1502	1504	rBV	139	67	0.01%	0.001%
47	6.032	1509	1511	1514	rVB	113	54	0.01%	0.001%
48	6.061	1514	1520	1523	rBV	94	118	0.01%	0.003%
49	6.177	1552	1556	1562	rVB2	630	624	0.08%	0.014%
50	6.331	1589	1604	1630	rVB	190064	371553	46.75%	8.236%
51	6.434	1632	1636	1638	rBV2	270	180	0.02%	0.004%
52	6.453	1639	1642	1648	rBV2	245	262	0.03%	0.006%
53	6.505	1654	1658	1661	rBV	106	78	0.01%	0.002%
54	6.521	1661	1663	1665	rVB	166	86	0.01%	0.002%
55	6.582	1679	1682	1684	rBV	74	51	0.01%	0.001%
56	6.633	1695	1698	1701	rBV	69	60	0.01%	0.001%
57	6.662	1705	1707	1711	rVB	206	82	0.01%	0.002%
58	6.727	1724	1727	1733	rVB	102	89	0.01%	0.002%
59	6.784	1742	1745	1754	rVB	259	267	0.03%	0.006%
60	6.823	1754	1757	1759	rBV	221	114	0.01%	0.003%
61	6.858	1764	1768	1777	rVB	531	602	0.08%	0.013%
62	6.968	1800	1802	1807	rVB	209	144	0.02%	0.003%
63	7.006	1811	1814	1817	rBV	107	78	0.01%	0.002%
64	7.145	1854	1857	1862	rBV	86	66	0.01%	0.001%
65	7.183	1866	1869	1871	rBV2	136	79	0.01%	0.002%
66	7.228	1871	1883	1900	rBV	87370	153940	19.37%	3.412%
67	7.331	1913	1915	1918	rBV	75	49	0.01%	0.001%
68	7.344	1918	1919	1921	rVV	124	51	0.01%	0.001%
69	7.354	1921	1922	1925	rVB	195	102	0.01%	0.002%
70	7.379	1925	1930	1932	rBV	57	48	0.01%	0.001%
71	7.411	1937	1940	1943	rVV2	162	111	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092118\
 Data File : VU026958.D
 Acq On : 21 Sep 2018 01:11
 Operator : MD/SY
 Sample : J5012-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Q4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

72	7.444	1948	1950	1954	rVB	138	84	0.01%	0.002%
73	7.566	1975	1988	2017	rBV	308347	535310	67.35%	11.866%
74	7.723	2034	2037	2040	rBV	341	277	0.03%	0.006%
75	7.849	2066	2076	2092	rBV	63836	106776	13.43%	2.367%
76	7.929	2099	2101	2106	rVB	323	275	0.03%	0.006%
77	7.977	2114	2116	2119	rVB	294	110	0.01%	0.002%
78	7.993	2119	2121	2123	rBV	169	100	0.01%	0.002%
79	8.013	2125	2127	2129	rBV	167	83	0.01%	0.002%
80	8.083	2147	2149	2151	rBV	176	82	0.01%	0.002%
81	8.177	2173	2178	2179	rBV	1368	1101	0.14%	0.024%
82	8.312	2208	2220	2254	rBV	244260	417806	52.57%	9.261%
83	8.540	2289	2291	2301	rVB2	359	375	0.05%	0.008%
84	8.591	2306	2307	2309	rVB2	207	60	0.01%	0.001%
85	8.611	2309	2313	2317	rBV	212	208	0.03%	0.005%
86	8.672	2328	2332	2334	rBV	206	147	0.02%	0.003%
87	8.707	2340	2343	2345	rBV	156	105	0.01%	0.002%
88	8.749	2355	2356	2360	rVB2	153	100	0.01%	0.002%
89	8.942	2413	2416	2421	rVB2	210	229	0.03%	0.005%
90	8.968	2421	2424	2429	rBV	115	103	0.01%	0.002%
91	9.093	2452	2463	2484	rBV	51805	94125	11.84%	2.086%
92	9.254	2510	2513	2514	rBV	83	50	0.01%	0.001%
93	9.263	2514	2516	2519	rVB	179	90	0.01%	0.002%
94	10.318	2842	2844	2847	rVB	211	99	0.01%	0.002%
95	10.434	2868	2880	2901	rBV	268149	424963	53.47%	9.420%
96	10.939	3035	3037	3043	rBV	258	161	0.02%	0.004%
97	11.485	3197	3207	3227	rVB	37190	64712	8.14%	1.434%
98	11.861	3312	3324	3349	rBV	263639	424059	53.35%	9.400%
99	12.186	3423	3425	3426	rBV	252	124	0.02%	0.003%
100	13.064	3696	3698	3700	rBV2	355	235	0.03%	0.005%


Sum of corrected areas: 4511354

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092118\
Data File : VU026958.D
Acq On : 21 Sep 2018 01:11
Operator : MD/SY
Sample : J5012-15 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Q4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

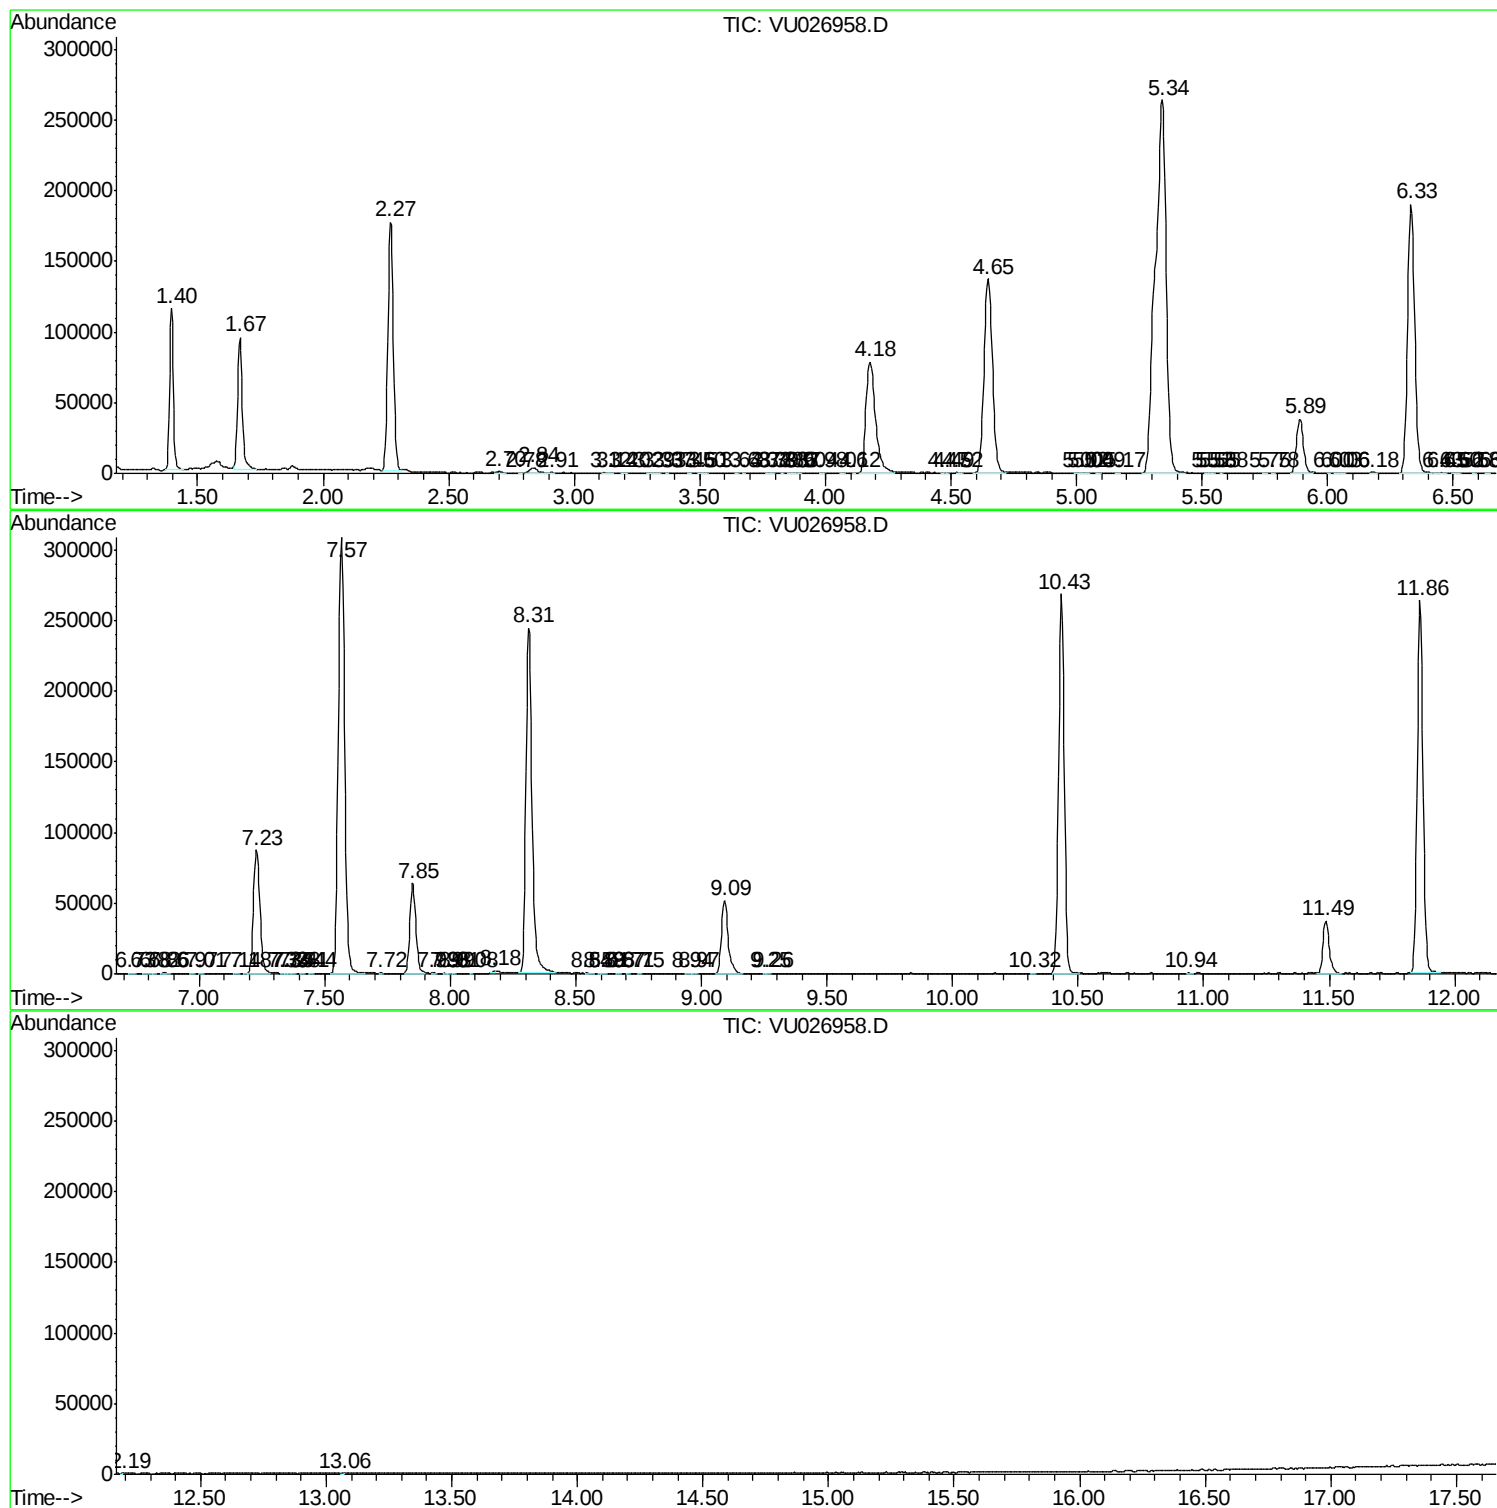

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092118\
Data File : VU026958.D
Acq On : 21 Sep 2018 01:11
Operator : MD/SY
Sample : J5012-15 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Q4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092118\
Data File : VU026958.D
Acq On : 21 Sep 2018 01:11
Operator : MD/SY
Sample : J5012-15 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Q4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc