

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092118\
 Data File : VU026961.D
 Acq On : 21 Sep 2018 02:23
 Operator : MD/SY
 Sample : J5012-18 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Q7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	62	69	86	rVB	134060	136970	15.20%	2.079%
2	1.662	145	152	165	rBV	104607	130600	14.50%	1.983%
3	2.267	330	340	353	rBV	212724	318211	35.32%	4.831%
4	2.546	424	427	429	rBV	318	200	0.02%	0.003%
5	2.662	460	463	465	rBV2	232	150	0.02%	0.002%
6	2.836	507	517	532	rVB2	4373	9391	1.04%	0.143%
7	2.935	546	548	552	rBV	195	130	0.01%	0.002%
8	3.009	569	571	580	rBV	175	146	0.02%	0.002%
9	3.067	587	589	593	rVB	137	49	0.01%	0.001%
10	3.151	610	615	619	rVB2	178	195	0.02%	0.003%
11	3.215	633	635	636	rBV2	141	43	0.00%	0.001%
12	3.328	667	670	671	rBV	136	74	0.01%	0.001%
13	3.389	687	689	692	rBV	124	104	0.01%	0.002%
14	3.501	722	724	725	rBV	116	28	0.00%	0.000%
15	3.607	755	757	761	rVB	172	111	0.01%	0.002%
16	3.630	761	764	765	rBV	158	70	0.01%	0.001%
17	3.691	781	783	788	rVB	176	92	0.01%	0.001%
18	3.730	792	795	796	rBV	103	53	0.01%	0.001%
19	3.787	812	813	814	rBV	107	24	0.00%	0.000%
20	3.810	817	820	823	rVB	150	67	0.01%	0.001%
21	3.858	833	835	838	rBV	154	65	0.01%	0.001%
22	3.910	849	851	852	rBV	140	45	0.00%	0.001%
23	3.942	859	861	864	rVB	113	26	0.00%	0.000%
24	3.955	864	865	867	rBV	119	32	0.00%	0.000%
25	4.115	913	915	917	rBV	143	62	0.01%	0.001%
26	4.176	920	934	966	rBV	81870	219214	24.33%	3.328%
27	4.508	1034	1037	1040	rBV	82	69	0.01%	0.001%
28	4.524	1041	1042	1043	rBV	110	24	0.00%	0.000%
29	4.559	1052	1053	1054	rBV	117	26	0.00%	0.000%
30	4.646	1064	1080	1102	rBV	152265	354883	39.39%	5.388%
31	4.877	1148	1152	1165	rVB4	656	1421	0.16%	0.022%
32	4.977	1182	1183	1184	rBV4	203	64	0.01%	0.001%
33	5.009	1191	1193	1194	rBV4	146	65	0.01%	0.001%
34	5.112	1223	1225	1227	rBV	75	44	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092118\
 Data File : VU026961.D
 Acq On : 21 Sep 2018 02:23
 Operator : MD/SY
 Sample : J5012-18 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Q7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

35	5.183	1245	1247	1249	rBV	80	45	0.00%	0.001%
36	5.340	1272	1296	1324	rBV2	306191	900993	100.00%	13.678%
37	5.511	1346	1349	1352	rVB	209	110	0.01%	0.002%
38	5.585	1370	1372	1373	rBV	89	34	0.00%	0.001%
39	5.755	1423	1425	1429	rVB	176	93	0.01%	0.001%
40	5.829	1446	1448	1450	rBV	62	28	0.00%	0.000%
41	5.887	1450	1466	1494	rBV	268326	526034	58.38%	7.986%
42	6.102	1531	1533	1535	rVB	120	59	0.01%	0.001%
43	6.180	1550	1557	1561	rBV3	627	802	0.09%	0.012%
44	6.260	1579	1582	1585	rVB	212	114	0.01%	0.002%
45	6.279	1585	1588	1590	rBV	78	47	0.01%	0.001%
46	6.331	1590	1604	1625	rVV	211108	416052	46.18%	6.316%
47	6.405	1625	1627	1630	rVB2	404	234	0.03%	0.004%
48	6.453	1638	1642	1646	rBV2	263	247	0.03%	0.004%
49	6.508	1657	1659	1662	rBV	149	48	0.01%	0.001%
50	6.540	1666	1669	1671	rBV	74	40	0.00%	0.001%
51	6.588	1682	1684	1688	rVB	184	76	0.01%	0.001%
52	6.610	1688	1691	1693	rBV	108	60	0.01%	0.001%
53	6.733	1727	1729	1730	rBV	118	30	0.00%	0.000%
54	6.826	1755	1758	1760	rBV	103	66	0.01%	0.001%
55	6.858	1763	1768	1769	rBV2	208	171	0.02%	0.003%
56	6.868	1769	1771	1772	rBV2	286	88	0.01%	0.001%
57	6.929	1788	1790	1792	rVB	228	68	0.01%	0.001%
58	7.141	1853	1856	1859	rVB	174	79	0.01%	0.001%
59	7.228	1871	1883	1902	rBV	100054	176210	19.56%	2.675%
60	7.350	1919	1921	1924	rVB2	210	112	0.01%	0.002%
61	7.369	1924	1927	1929	rBV	171	84	0.01%	0.001%
62	7.389	1930	1933	1936	rVB	173	89	0.01%	0.001%
63	7.411	1937	1940	1943	rBV	217	117	0.01%	0.002%
64	7.430	1943	1946	1953	rBV	190	221	0.02%	0.003%
65	7.463	1953	1956	1957	rBV	261	140	0.02%	0.002%
66	7.565	1974	1988	2019	rBV	386981	665871	73.90%	10.109%
67	7.749	2042	2045	2047	rBV2	232	140	0.02%	0.002%
68	7.803	2060	2062	2064	rBV	187	86	0.01%	0.001%
69	7.852	2066	2077	2101	rVB	72391	120868	13.41%	1.835%
70	7.938	2101	2104	2106	rBV	223	156	0.02%	0.002%
71	7.967	2109	2113	2116	rBV2	308	221	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092118\
 Data File : VU026961.D
 Acq On : 21 Sep 2018 02:23
 Operator : MD/SY
 Sample : J5012-18 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C08Q7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

72	8.016	2124	2128	2130	rBV2	222	175	0.02%	0.003%
73	8.035	2132	2134	2137	rBV2	140	98	0.01%	0.001%
74	8.147	2166	2169	2170	rBV	169	97	0.01%	0.001%
75	8.315	2208	2221	2244	rBV	272166	459095	50.95%	6.970%
76	8.520	2282	2285	2289	rBV2	291	253	0.03%	0.004%
77	8.768	2358	2362	2365	rBV2	238	165	0.02%	0.003%
78	8.800	2370	2372	2378	rBV	151	126	0.01%	0.002%
79	8.868	2391	2393	2396	rVB	195	74	0.01%	0.001%
80	8.893	2399	2401	2402	rVV	120	30	0.00%	0.000%
81	8.938	2412	2415	2421	rBV2	384	435	0.05%	0.007%
82	9.089	2449	2462	2489	rBV	376335	619827	68.79%	9.410%
83	9.234	2505	2507	2509	rBV	257	123	0.01%	0.002%
84	9.417	2562	2564	2567	rVB	180	56	0.01%	0.001%
85	9.575	2611	2613	2617	rVB	167	80	0.01%	0.001%
86	9.800	2681	2683	2686	rVB2	160	95	0.01%	0.001%
87	9.858	2699	2701	2704	rVB	313	115	0.01%	0.002%
88	10.093	2771	2774	2776	rBV2	208	132	0.01%	0.002%
89	10.138	2785	2788	2794	rBV	163	161	0.02%	0.002%
90	10.433	2867	2880	2901	rBV	301540	473311	52.53%	7.185%
91	10.523	2907	2908	2909	rBV	126	37	0.00%	0.001%
92	10.954	3040	3042	3044	rVB	252	77	0.01%	0.001%
93	10.996	3052	3055	3059	rBV2	297	251	0.03%	0.004%
94	11.276	3139	3142	3145	rBV	224	136	0.02%	0.002%
95	11.421	3186	3187	3193	rBV2	374	245	0.03%	0.004%
96	11.485	3195	3207	3231	rVV	300538	476774	52.92%	7.238%
97	11.861	3312	3324	3343	rBV	356072	572393	63.53%	8.690%


Sum of corrected areas: 6587042

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092118\
Data File : VU026961.D
Acq On : 21 Sep 2018 02:23
Operator : MD/SY
Sample : J5012-18 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C08Q7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

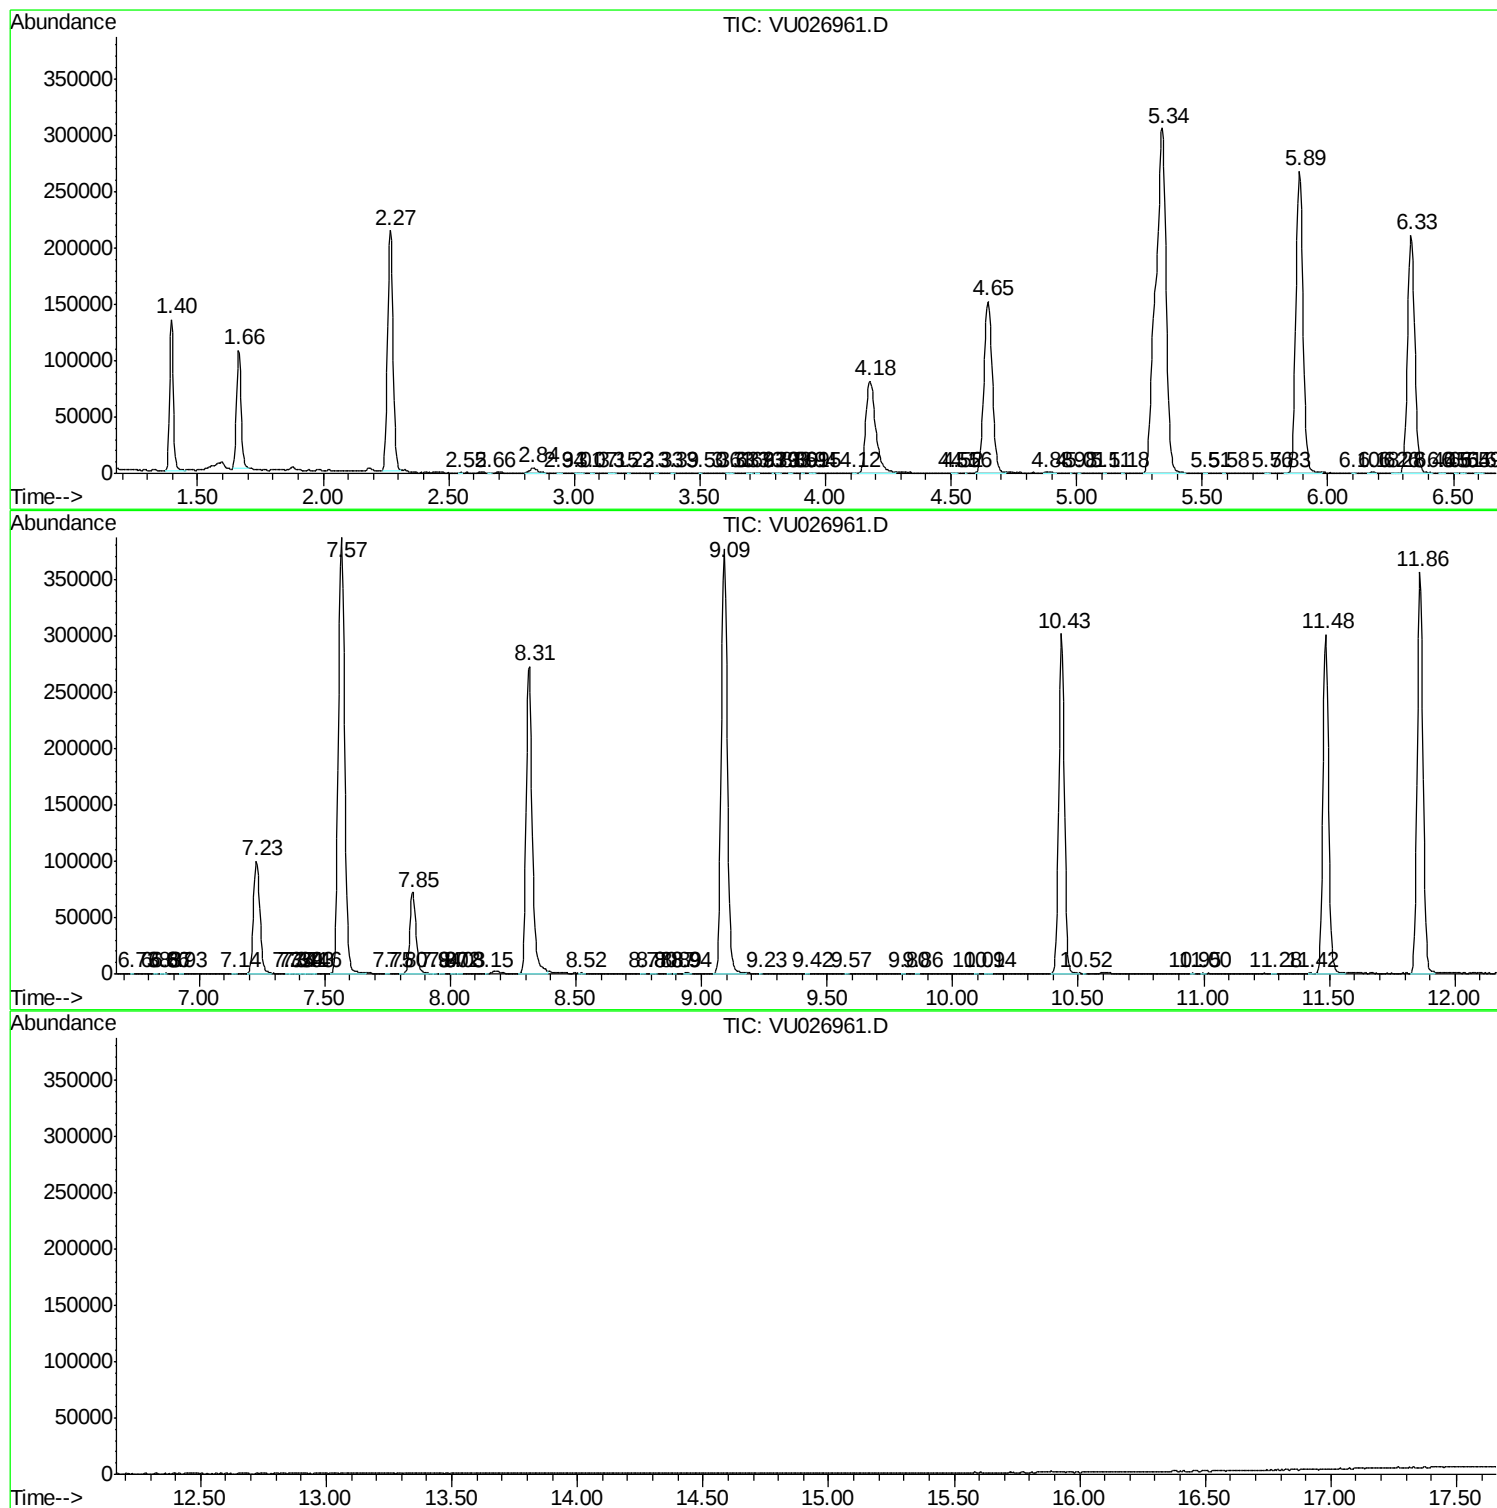

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092118\
Data File : VU026961.D
Acq On : 21 Sep 2018 02:23
Operator : MD/SY
Sample : J5012-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Q7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092118\
Data File : VU026961.D
Acq On : 21 Sep 2018 02:23
Operator : MD/SY
Sample : J5012-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C08Q7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc