


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092118\
Data File : VU026924.D
Acq On : 20 Sep 2018 07:53
Operator : MD/SY
Sample : BFB44
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Title : VOC Analysis
Last Update : Fri Sep 21 18:17:02 2018

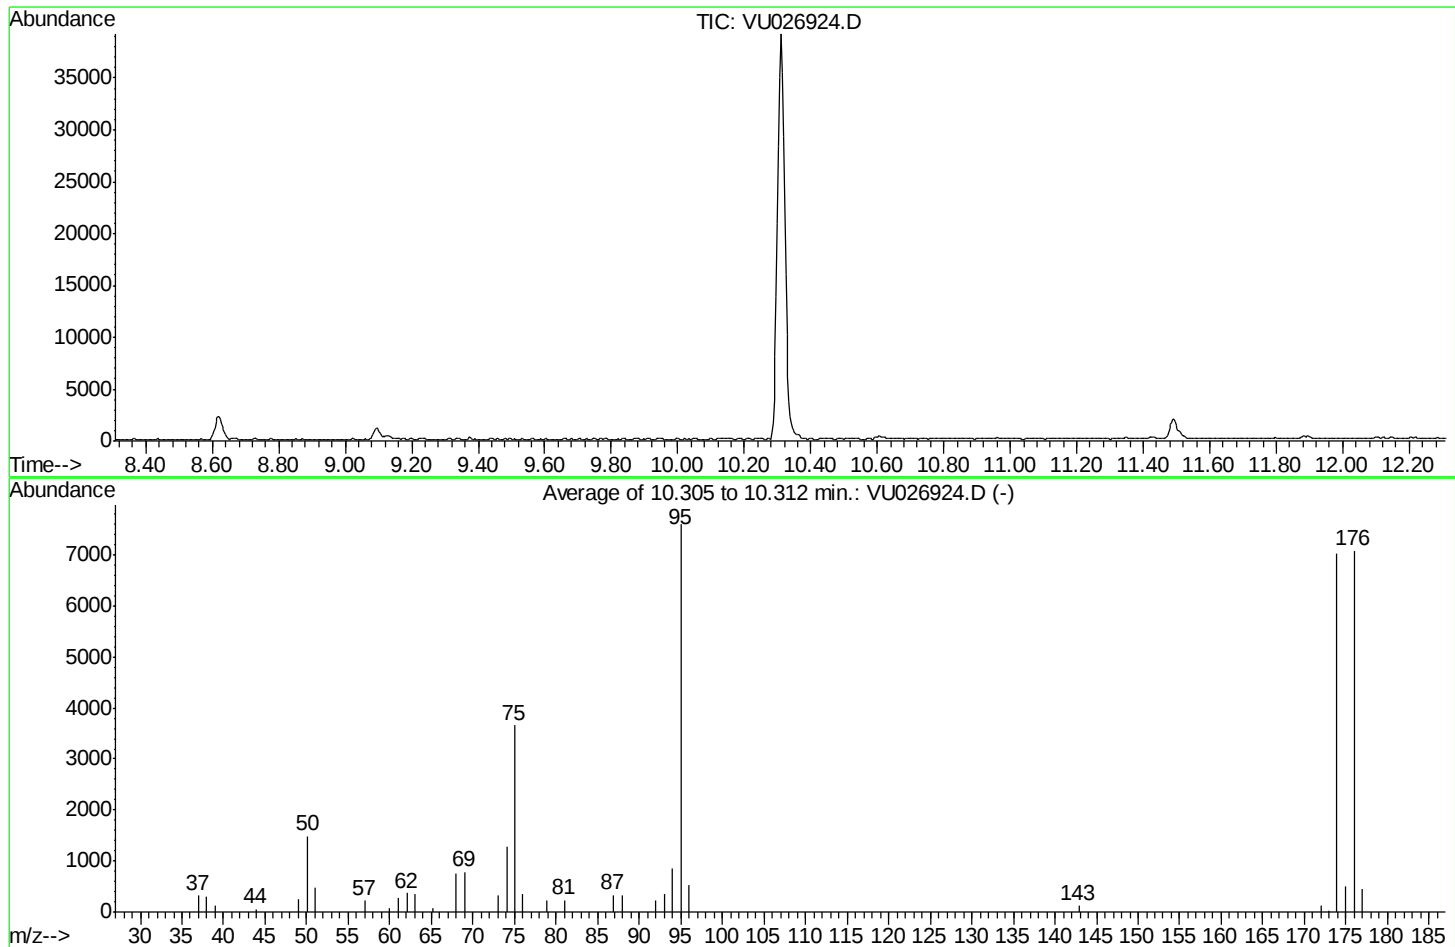

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	1485	PASS
75	95	30	80	48.1	3654	PASS
95	95	100	100	100.0	7600	PASS
96	95	5	9	6.9	527	PASS
173	174	0.00	2	0.5	34	PASS
174	95	50	120	92.6	7038	PASS
175	174	5	9	7.0	493	PASS
176	174	95	101	100.6	7078	PASS
177	176	5	9	6.3	446	PASS

m/z	Abundance
44.00	202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
37.00	302.0
38.00	321.0
39.00	134.0
43.90	280.0
49.00	257.0
50.10	1403.0
51.00	444.0
57.00	210.0
61.00	286.0
62.10	389.0
63.00	321.0
68.00	692.0
69.00	782.0
73.00	311.0
74.10	1179.0
75.00	3389.0
76.00	377.0
78.90	220.0
81.00	214.0
86.80	325.0
87.90	304.0
91.90	207.0
93.00	334.0
94.00	783.0
95.00	7094.0
96.00	481.0
142.80	129.0
172.00	131.0
173.90	6422.0
174.90	488.0
176.00	6421.0
176.90	385.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
37.00	339.0
38.00	318.0
39.00	135.0
43.90	273.0
49.00	250.0
50.10	1570.0
51.00	490.0
57.00	229.0
59.90	108.0
60.90	290.0
62.10	385.0
63.00	354.0
65.10	106.0
68.00	764.0
69.00	823.0
73.00	333.0
74.10	1335.0
75.00	3761.0
76.00	380.0
78.90	235.0
81.00	241.0
86.80	351.0
87.90	322.0
91.90	227.0
93.00	364.0
94.00	865.0
95.00	7873.0
96.00	547.0
142.80	127.0
172.00	134.0
173.90	7267.0
174.90	508.0
176.00	7294.0
177.00	444.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
37.00	337.0
38.00	279.0
39.00	143.0
43.90	243.0
48.90	249.0
50.10	1482.0
51.00	476.0
57.00	226.0
59.90	106.0
60.90	291.0
62.00	331.0
63.00	358.0
65.10	111.0
68.00	774.0
69.00	750.0
73.00	326.0
74.10	1336.0
75.00	3812.0
76.00	319.0
78.90	229.0
81.00	248.0
86.90	327.0
87.90	336.0
91.90	219.0
93.00	366.0
94.00	879.0
95.00	7833.0
96.00	553.0
142.90	105.0
171.90	148.0
173.00	103.0
173.90	7427.0
175.00	483.0
176.00	7521.0
176.90	510.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44