
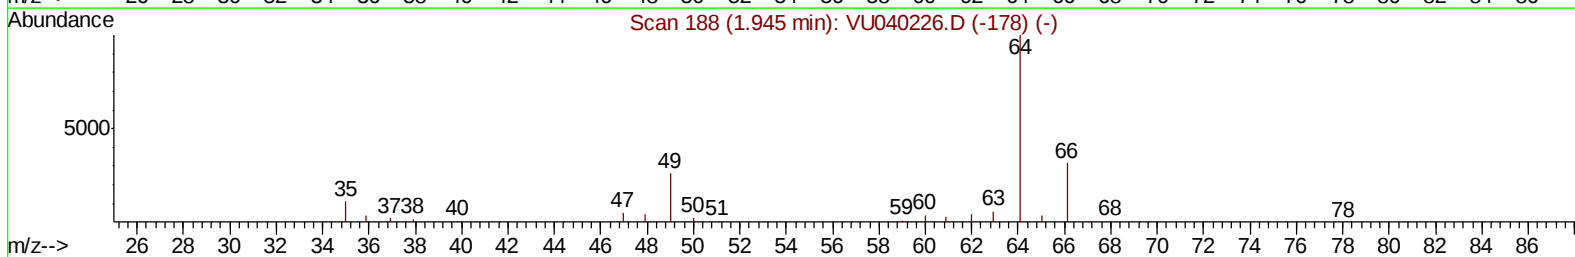
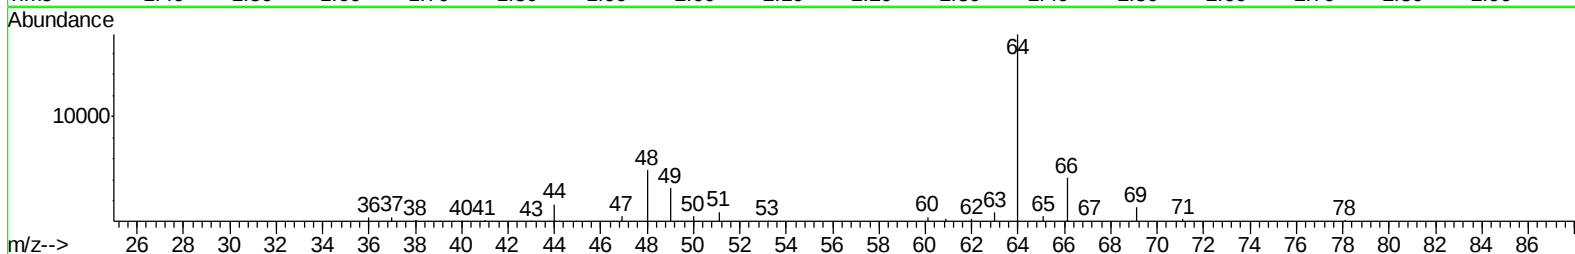


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092120\
Data File : VU040240.D
Acq On : 21 Sep 2020 17:45
Operator : SY/MD
Sample : L4046-16
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Sep 22 07:16:39 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Sep 22 07:07:10 2020
Response via : Initial Calibration

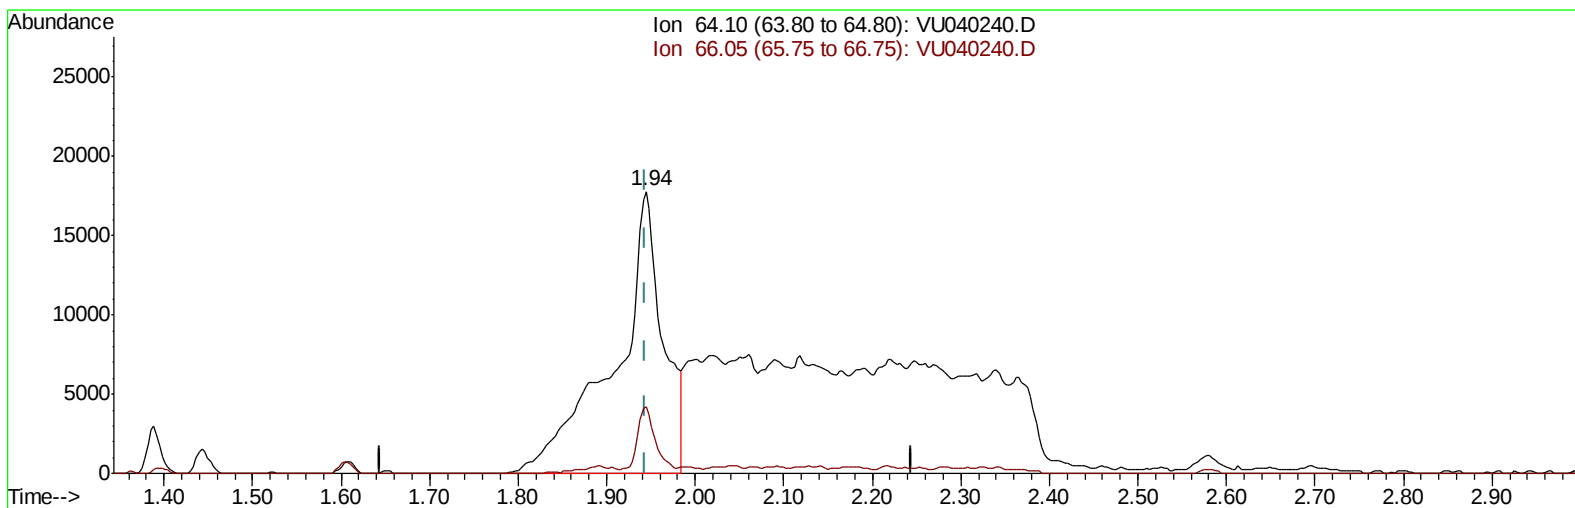

TIC: VU040240.D

(8) Chloroethane (T)

1.944min (-0.000) 8.64ug/L

response 66874

Ion	Exp%	Act%
64.10	100	100
66.05	32.40	23.69
0.00	0.00	0.00
0.00	0.00	0.00