
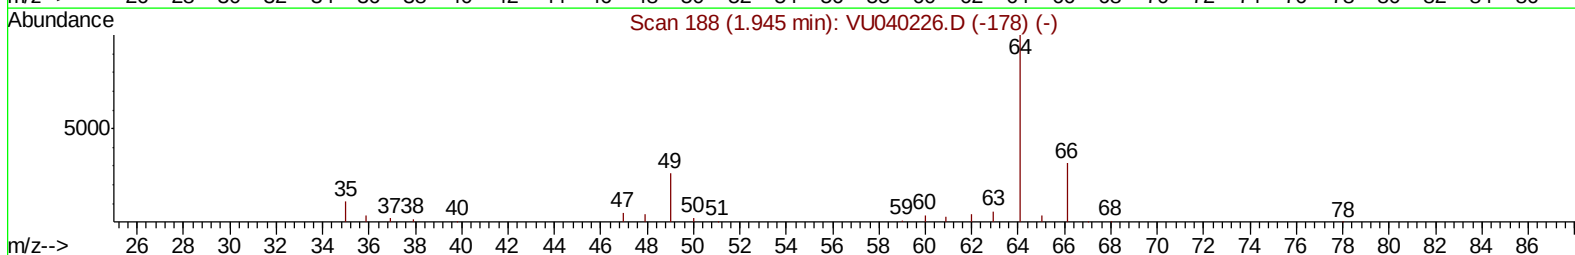
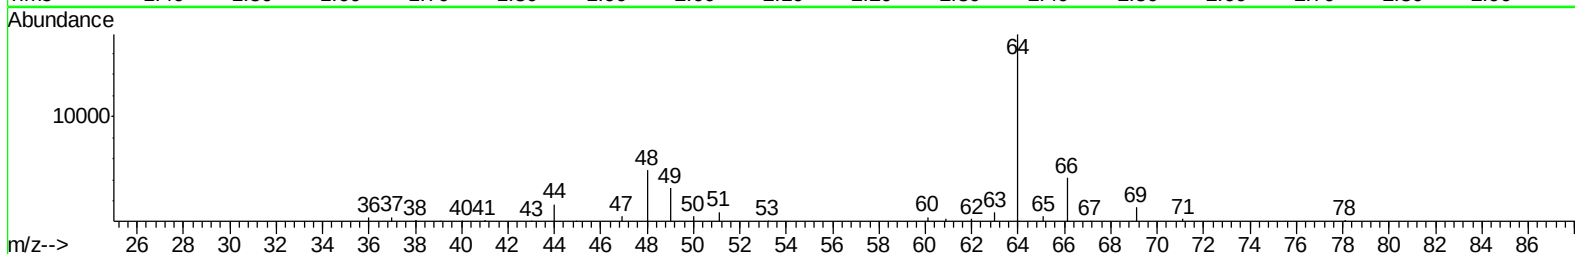


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092120\
 Data File : VU040240.D
 Acq On : 21 Sep 2020 17:45
 Operator : SY/MD
 Sample : L4046-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Sep 22 07:16:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Sep 22 07:07:10 2020
 Response via : Initial Calibration

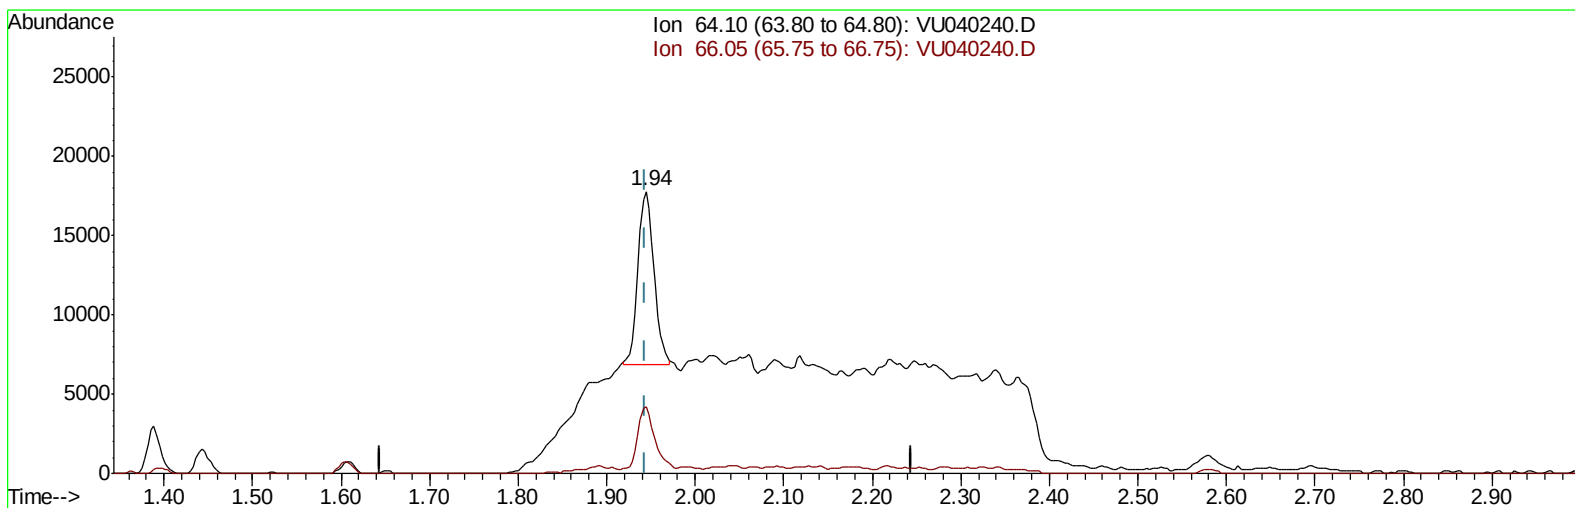

TIC: VU040240.D

(8) Chloroethane (T)

1.944min (-0.000) 1.78ug/L m

response 13770

Ion	Exp%	Act%
64.10	100	100
66.05	32.40	23.69
0.00	0.00	0.00
0.00	0.00	0.00