


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092120\
 Data File : VU040225.D
 Acq On : 21 Sep 2020 09:41
 Operator : SY/MD
 Sample : BFB05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB05

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Sep 22 07:07:10 2020

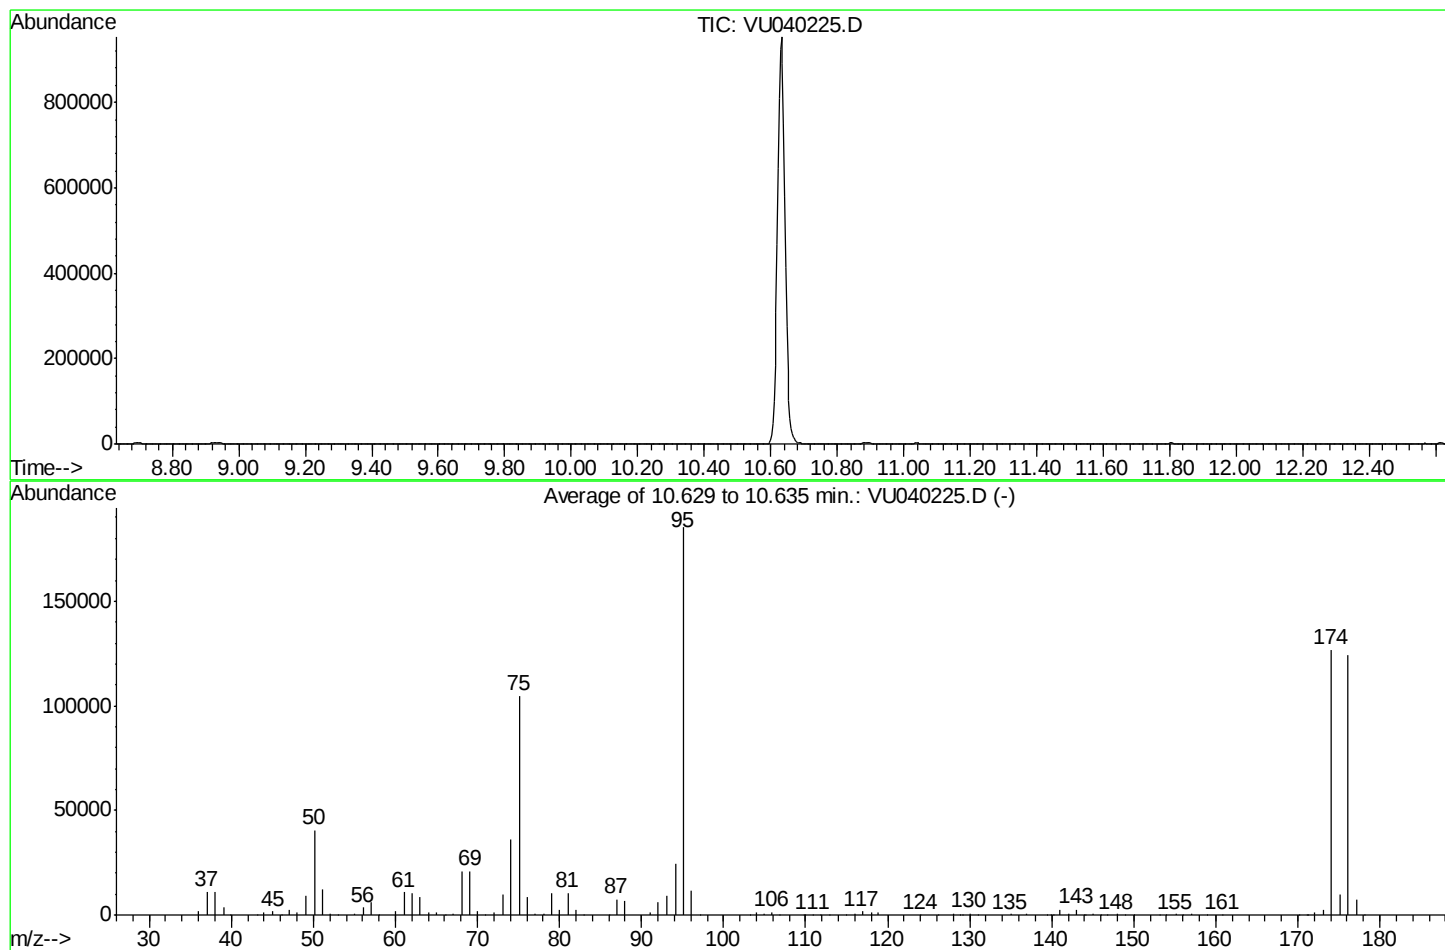

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	40605	PASS
75	95	30	80	56.6	104946	PASS
95	95	100	100	100.0	185301	PASS
96	95	5	9	6.3	11624	PASS
173	174	0.00	2	1.7	2202	PASS
174	95	50	120	68.5	126850	PASS
175	174	5	9	7.9	9959	PASS
176	174	95	101	97.8	124008	PASS
177	176	5	9	6.1	7565	PASS

m/z	Abundance
36.00	2104.0
37.10	11663.0
38.10	11244.0
39.00	3903.0
40.10	203.0
43.10	130.0
44.10	1757.0
45.10	1872.0
46.10	280.0
47.00	2559.0
48.00	1430.0
49.10	9649.0
50.10	41280.0
51.10	12086.0
52.00	627.0
53.10	157.0
55.00	710.0
56.10	3555.0
57.10	6310.0
58.10	295.0
60.00	2274.0
61.10	10845.0
62.10	10893.0
63.00	8573.0
64.00	1023.0
65.00	1317.0
66.10	258.0
67.00	640.0
68.10	21552.0
69.10	20840.0
70.00	1590.0
72.10	1347.0
73.10	9737.0
74.10	37128.0
75.10	105408.0
76.10	8643.0
77.00	1098.0
78.10	644.0
79.00	10694.0
79.90	2466.0
81.00	10560.0
81.90	2303.0
83.00	243.0
86.10	259.0
87.00	7599.0
88.00	6356.0
91.00	1050.0
92.00	6018.0
93.10	9292.0
94.10	24536.0
95.10	185920.0
96.10	11906.0
97.10	247.0
103.20	142.0
103.90	1131.0
105.00	417.0
105.90	1498.0
106.90	189.0
109.80	147.0
110.90	243.0
111.90	226.0
113.00	251.0
114.90	230.0
116.00	819.0
117.00	1826.0
118.00	984.0
118.90	1232.0
128.00	738.0
128.90	336.0
130.10	800.0
131.00	260.0
135.00	611.0
136.90	350.0
139.80	172.0
140.20	199.0
141.00	2425.0
142.00	292.0
143.10	2400.0
143.90	210.0
145.10	562.0
145.90	325.0
146.80	126.0
148.00	439.0
148.90	152.0
150.00	201.0
153.10	284.0
153.90	155.0
155.10	398.0
156.00	116.0
157.00	345.0
159.00	383.0
161.00	160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

171.10	281.0
172.10	1268.0
173.10	2009.0
174.10	125256.0
175.10	10133.0
176.10	120344.0
177.10	7336.0
178.10	201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	2098.0
37.10	11648.0
38.10	11354.0
39.10	4164.0
39.90	219.0
43.10	149.0
44.10	1762.0
45.00	1812.0
46.20	281.0
47.00	2704.0
48.00	1498.0
49.10	9665.0
50.10	41976.0
51.10	12479.0
52.00	620.0
53.00	114.0
55.00	695.0
56.00	3753.0
57.10	6511.0
58.00	275.0
60.00	2219.0
61.00	11134.0
62.10	10869.0
63.00	8510.0
64.10	954.0
65.00	1217.0
66.10	205.0
67.00	653.0
68.10	21192.0
69.10	21784.0
70.10	1681.0
72.00	1352.0
73.10	9966.0
74.10	36744.0
75.10	108472.0
76.10	8659.0
77.00	932.0
78.10	902.0
79.00	10805.0
79.90	2548.0
81.00	10868.0
81.90	2389.0
82.90	210.0
86.10	215.0
87.00	7786.0
88.00	6959.0
91.00	1044.0
92.00	6169.0
93.10	9483.0
94.10	25160.0
95.10	191808.0
96.10	11972.0
97.10	286.0
104.00	1108.0
105.00	428.0
105.90	1471.0
106.90	229.0
110.00	199.0
110.90	291.0
111.80	230.0
112.80	230.0
114.90	237.0
116.00	911.0
117.00	1777.0
118.00	1048.0
118.90	1295.0
124.00	116.0
126.20	102.0
128.00	753.0
128.80	269.0
129.20	289.0
130.00	805.0
131.00	261.0
135.00	607.0
136.90	433.0
139.80	199.0
141.00	2462.0
142.10	348.0
143.00	2586.0
143.90	168.0
145.10	515.0
145.90	278.0
146.80	140.0
148.00	447.0
148.90	171.0
150.00	264.0
153.10	237.0
153.90	170.0
155.10	390.0
157.00	370.0
158.90	341.0
160.80	194.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

170.10	117.0
171.30	250.0
172.00	1258.0
173.10	2360.0
174.10	131048.0
175.10	10267.0
176.10	128640.0
177.10	7787.0
178.10	191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	1926.0
37.00	10606.0
38.00	10155.0
39.10	3917.0
39.90	225.0
43.10	107.0
44.00	1585.0
45.00	1636.0
46.20	213.0
47.10	2441.0
48.00	1293.0
49.00	8717.0
50.10	38560.0
51.10	11678.0
52.00	526.0
55.00	615.0
56.00	3537.0
57.10	6110.0
58.00	290.0
60.00	1918.0
61.10	10216.0
62.00	10065.0
63.00	8030.0
64.10	870.0
65.00	1063.0
67.00	661.0
68.10	19032.0
69.10	20680.0
70.10	1554.0
71.00	127.0
72.10	1223.0
73.10	9154.0
74.10	34016.0
75.10	100960.0
76.10	8060.0
77.10	770.0
78.10	1013.0
79.00	9688.0
80.00	2338.0
81.00	10018.0
82.00	2179.0
82.90	179.0
86.10	194.0
87.00	7230.0
88.00	6648.0
91.00	977.0
92.10	5911.0
93.10	8627.0
94.10	23456.0
95.10	178176.0
96.10	10996.0
97.10	304.0
104.00	931.0
105.00	358.0
105.90	1211.0
106.80	237.0
110.00	266.0
110.90	328.0
111.80	226.0
112.80	226.0
114.90	230.0
116.00	888.0
116.90	1484.0
118.00	963.0
118.90	1179.0
124.00	124.0
126.20	152.0
128.00	682.0
128.80	223.0
129.10	225.0
130.00	737.0
131.10	262.0
135.00	462.0
136.90	415.0
139.40	125.0
139.90	177.0
141.00	2227.0
142.10	371.0
143.00	2661.0
144.10	165.0
145.10	421.0
146.00	285.0
146.80	119.0
148.00	416.0
148.90	135.0
150.00	296.0
153.00	135.0
153.90	145.0
155.10	325.0
157.00	342.0
158.90	211.0
160.80	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

170.20	116.0
172.00	1100.0
173.10	2238.0
174.10	124248.0
175.10	9479.0
176.10	123040.0
177.10	7574.0
178.10	170.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
43.90	424.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05