

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092121\
 Data File : VU044741.D
 Acq On : 21 Sep 2021 17:06
 Operator : SY/MD
 Sample : M3777-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AF8

Quant Time: Sep 22 01:43:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 22 01:40:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	117362	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	116874	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	51563	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	30215	4.363	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.200%
7) Chloroethane-d5	1.916	69	28397	4.018	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.400%
11) 1,1-Dichloroethene-d2	2.571	65	13370	3.823	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.400%
20) 2-Butanone-d5	4.639	46	116239	40.043	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.080%
24) Chloroform-d	5.070	84	62617	4.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	5.710	65	36441	4.196	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.000%
32) Benzene-d6	5.735	84	114254	3.834	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.600%
36) 1,2-Dichloropropane-d6	6.697	67	40478	4.136	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.800%
41) Toluene-d8	7.902	98	88366	3.406	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.200%#
43) trans-1,3-Dichloroprop...	8.182	79	12088	3.504	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.000%
46) 2-Hexanone-d5	8.642	63	82544	37.228	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.460%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	35017	4.035	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.800%
66) 1,2-Dichlorobenzene-d4	12.198	152	33688	3.959	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	79.200%#
Target Compounds					Qvalue	
13) Acetone	2.645	43	7024	3.715	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092121\
Data File : VU044741.D
Acq On : 21 Sep 2021 17:06
Operator : SY/MD
Sample : M3777-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF8

Quant Time: Sep 22 01:43:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 22 01:40:07 2021
Response via : Initial Calibration

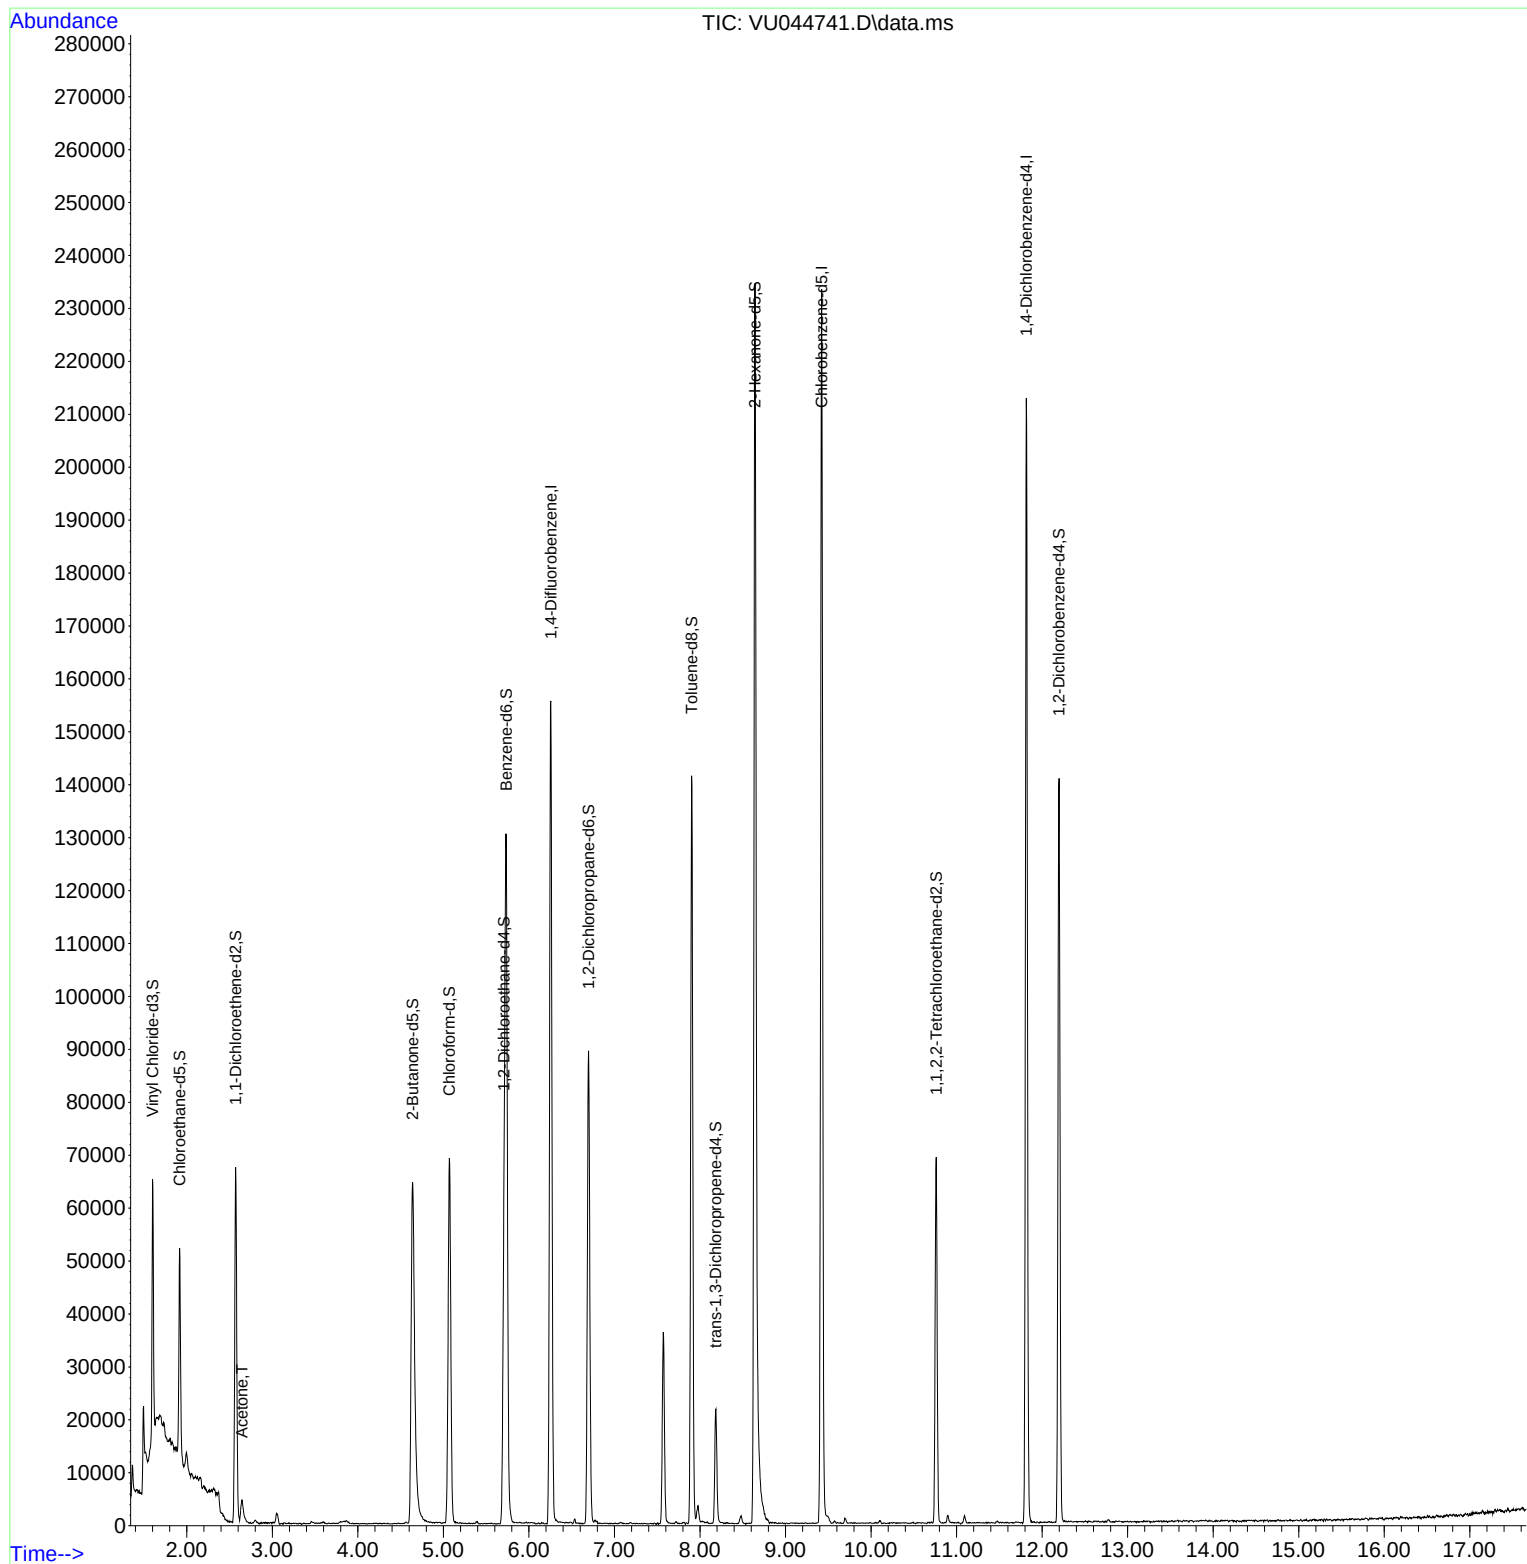

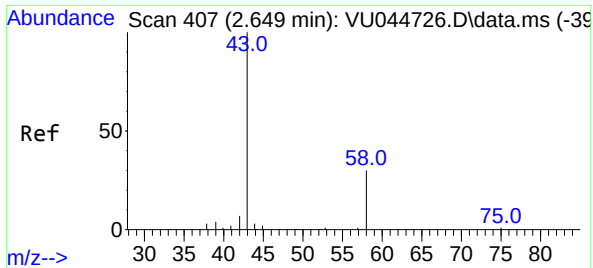

#13
 Acetone
 Concen: 3.715 ug/L
 RT: 2.645 min Scan# 406
 Delta R.T. -0.003 min
 Lab File: VU044741.D
 Acq: 21 Sep 2021 17:06

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AF8

Tgt Ion:	43	Resp:	7024
Ion	Ratio	Lower	Upper
43	100		
58	27.8	0.0	42.4

