

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092121\
 Data File : VU044744.D
 Acq On : 21 Sep 2021 18:19
 Operator : SY/MD
 Sample : M3777-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY6

Quant Time: Sep 22 01:43:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 22 01:40:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	116732	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.424	117	119089	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	49439	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	29469	4.279	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.600%
7) Chloroethane-d5	1.916	69	27839	3.961	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.200%
11) 1,1-Dichloroethene-d2	2.572	65	12716	3.655	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%
20) 2-Butanone-d5	4.642	46	120379	41.693	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.380%
24) Chloroform-d	5.070	84	61859	4.270	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.400%
26) 1,2-Dichloroethane-d4	5.710	65	37518	4.343	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.800%
32) Benzene-d6	5.736	84	115409	3.801	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.000%
36) 1,2-Dichloropropane-d6	6.697	67	41457	4.157	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.200%
41) Toluene-d8	7.903	98	90519	3.424	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.400%#
43) trans-1,3-Dichloroprop...	8.186	79	12270	3.491	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.800%
46) 2-Hexanone-d5	8.642	63	84874	37.567	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.140%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	35923	4.063	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.200%
66) 1,2-Dichlorobenzene-d4	12.198	152	34530	4.233	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.600%
Target Compounds						Qvalue
13) Acetone	2.649	43	3452	1.836	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092121\
Data File : VU044744.D
Acq On : 21 Sep 2021 18:19
Operator : SY/MD
Sample : M3777-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY6

Quant Time: Sep 22 01:43:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 22 01:40:07 2021
Response via : Initial Calibration

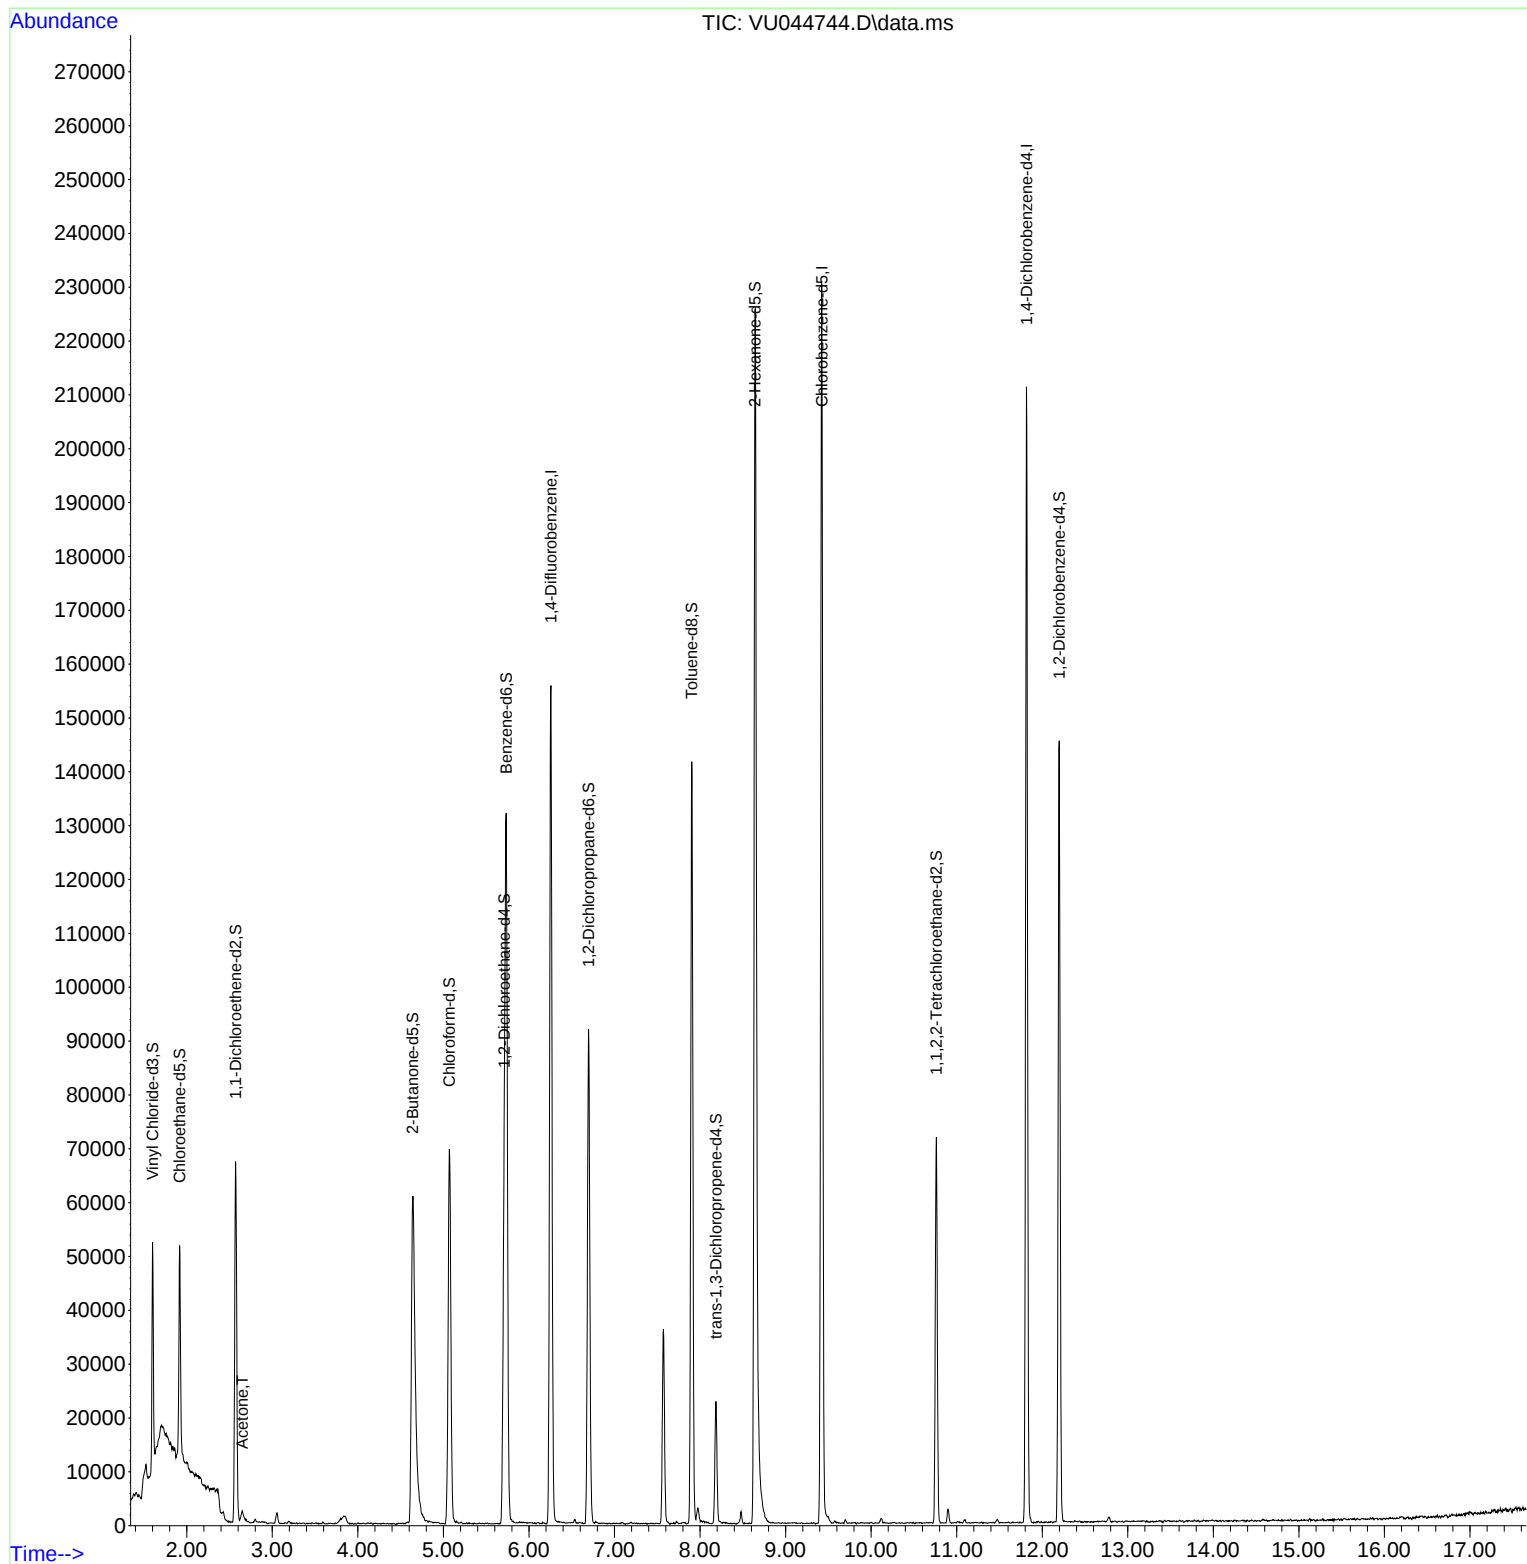

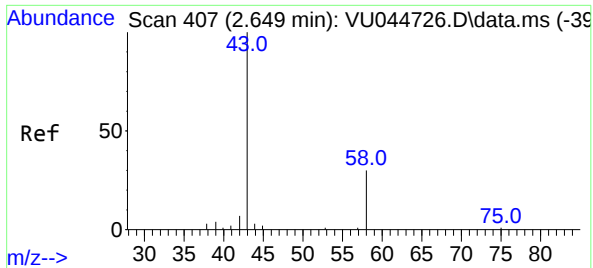

#13
 Acetone
 Concen: 1.836 ug/L
 RT: 2.649 min Scan# 407
 Delta R.T. 0.000 min
 Lab File: VU044744.D
 Acq: 21 Sep 2021 18:19

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY6

Tgt Ion:	43	Resp:	3452
Ion	Ratio	Lower	Upper
43	100		
58	15.8	0.0	42.4

