


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092121\
Data File : VU044725.D
Acq On : 21 Sep 2021 09:47
Operator : SY/MD
Sample : BFB022
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB022

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 22 01:40:07 2021

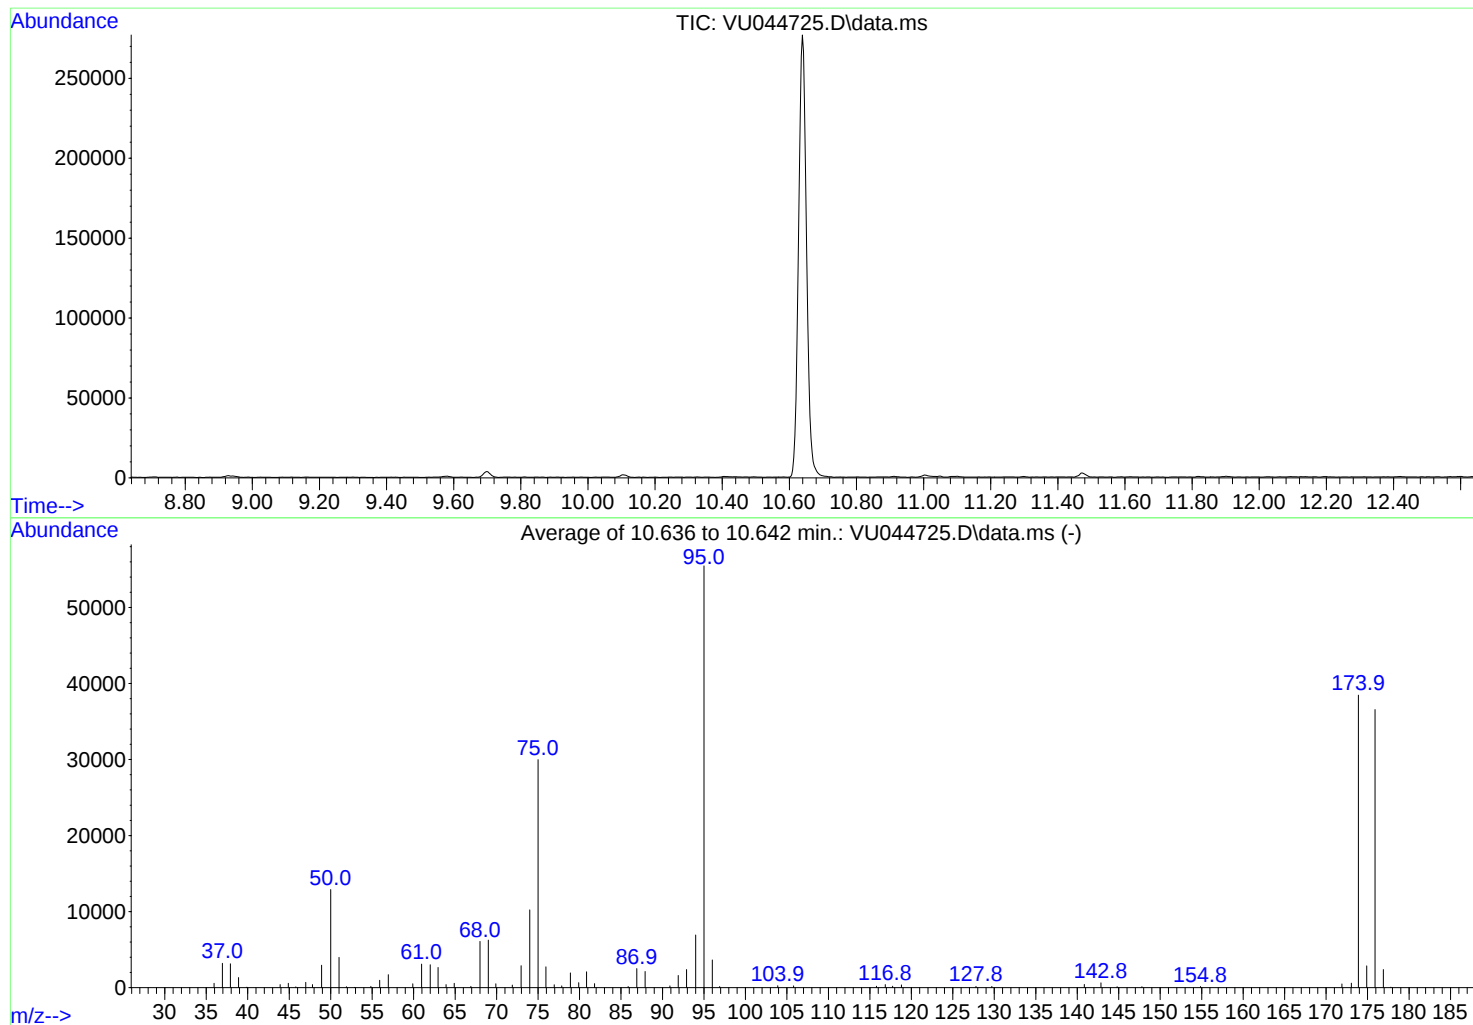

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.3	12900	PASS
75	95	30	80	54.0	29981	PASS
95	95	100	100	100.0	55475	PASS
96	95	5	9	6.6	3638	PASS
173	174	0.00	2	1.5	580	PASS
174	95	50	120	69.4	38475	PASS
175	174	5	9	7.4	2860	PASS
176	174	95	101	95.1	36571	PASS
177	176	5	9	6.5	2376	PASS

m/z	Abundance
39.90	115.0
43.90	343.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	563.0
36.90	3218.0
37.90	3103.0
38.90	1323.0
39.90	165.0
43.90	781.0
44.90	584.0
45.80	125.0
47.00	639.0
47.80	378.0
48.90	3003.0
50.00	12944.0
51.00	3952.0
51.90	122.0
54.90	169.0
55.90	915.0
57.00	1618.0
59.90	468.0
61.00	3046.0
62.00	3001.0
63.00	2603.0
63.90	371.0
64.90	575.0
66.90	155.0
68.00	5906.0
69.00	6248.0
69.90	535.0
71.90	334.0
72.90	2887.0
74.00	10249.0
75.00	29824.0
75.90	2732.0
76.90	416.0
77.90	205.0
78.90	1852.0
79.90	651.0
80.80	2055.0
81.80	538.0
85.80	155.0
86.90	2525.0
87.90	2032.0
90.90	228.0
91.90	1588.0
92.90	2371.0
94.00	6862.0
95.00	54376.0
96.00	3548.0
96.90	156.0
103.90	254.0
105.80	210.0
115.80	172.0
116.90	379.0
117.70	204.0
118.80	382.0
127.80	148.0
129.70	172.0
140.80	435.0
142.90	652.0
144.80	127.0
147.80	139.0
154.90	122.0
171.90	455.0
173.00	537.0
173.90	36816.0
174.90	2775.0
175.90	35096.0
176.90	2326.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
36.00	593.0
36.90	3282.0
37.90	3297.0
38.90	1350.0
39.90	174.0
43.90	772.0
44.90	581.0
45.80	113.0
47.00	716.0
47.80	411.0
48.90	3055.0
50.00	13320.0
51.00	4118.0
51.90	125.0
54.80	174.0
55.90	976.0
57.00	1746.0
59.90	521.0
60.90	3190.0
62.00	3063.0
62.90	2719.0
63.90	409.0
64.90	590.0
66.90	174.0
68.00	6275.0
69.00	6426.0
69.90	513.0
71.90	336.0
73.00	3003.0
74.00	10479.0
75.00	30848.0
75.90	2810.0
77.00	397.0
77.90	230.0
78.90	2005.0
79.90	678.0
80.90	2134.0
81.80	553.0
85.90	152.0
86.90	2598.0
87.90	2177.0
90.90	252.0
91.90	1636.0
92.90	2440.0
94.00	7183.0
95.00	57168.0
96.00	3714.0
96.90	165.0
103.90	260.0
105.80	238.0
115.80	191.0
116.80	399.0
117.80	213.0
118.80	365.0
127.80	185.0
129.70	174.0
140.80	448.0
142.80	646.0
144.80	134.0
147.80	141.0
154.80	152.0
171.90	504.0
173.00	602.0
173.90	39680.0
174.90	2916.0
175.90	37632.0
176.90	2429.0
177.80	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
36.00	573.0
37.00	3121.0
37.90	3023.0
38.90	1288.0
39.90	198.0
43.90	703.0
44.90	537.0
45.80	102.0
47.00	710.0
47.80	434.0
48.90	2775.0
50.00	12437.0
51.00	3859.0
51.90	126.0
52.90	103.0
54.90	192.0
55.90	989.0
56.90	1740.0
59.90	544.0
60.90	3042.0
62.00	2952.0
62.90	2604.0
63.90	415.0
64.90	549.0
66.90	195.0
68.00	6058.0
69.00	6052.0
69.90	467.0
71.90	333.0
73.00	2789.0
74.00	9969.0
75.00	29272.0
76.00	2642.0
76.90	346.0
77.80	234.0
78.90	1965.0
79.90	616.0
80.90	2048.0
81.80	493.0
85.90	118.0
86.90	2420.0
87.90	2170.0
90.90	239.0
91.90	1546.0
92.90	2337.0
94.00	6756.0
95.00	54880.0
96.00	3651.0
96.90	126.0
103.90	247.0
105.80	249.0
115.80	205.0
116.80	440.0
117.80	186.0
118.80	306.0
127.80	202.0
129.70	164.0
140.90	396.0
142.80	610.0
144.80	128.0
147.80	122.0
154.80	159.0
171.90	520.0
173.10	600.0
173.90	38928.0
174.90	2888.0
175.90	36984.0
176.90	2372.0
177.80	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022