

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092123\
 Data File : VU055450.D
 Acq On : 21 Sep 2023 17:00
 Operator : MD/SY
 Sample : VIBLK140
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK140

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	113	rVB	150021	179179	13.42%	1.669%
2	1.907	184	192	211	rBV	153225	208640	15.63%	1.944%
3	2.563	384	396	413	rBV	262854	432343	32.39%	4.028%
4	3.039	530	544	562	rBV2	53313	100640	7.54%	0.938%
5	4.624	1025	1037	1082	rBV	157927	490722	36.76%	4.572%
6	5.058	1156	1172	1194	rBV	265255	591070	44.28%	5.507%
7	5.721	1357	1378	1411	rBV2	508536	1334880	100.00%	12.437%
8	6.245	1528	1541	1562	rBV	335139	661767	49.58%	6.165%
9	6.534	1619	1631	1646	rVB6	18957	39449	2.96%	0.368%
10	6.689	1665	1679	1696	rBV	312884	614194	46.01%	5.722%
11	7.563	1939	1951	1981	rBV	146534	272236	20.39%	2.536%
12	7.795	2013	2023	2038	rBV4	10962	20414	1.53%	0.190%
13	7.894	2038	2054	2074	rBV	606934	1077984	80.76%	10.043%
14	8.177	2130	2142	2168	rBV	86299	161761	12.12%	1.507%
15	8.634	2270	2284	2321	rBV5	470485	1204994	90.27%	11.226%
16	9.415	2514	2527	2557	rBV	508599	877834	65.76%	8.178%
17	9.698	2604	2615	2627	rBV3	9750	16535	1.24%	0.154%
18	10.483	2850	2859	2872	rBV2	9338	14795	1.11%	0.138%
19	10.753	2931	2943	2959	rBV	227715	371267	27.81%	3.459%
20	11.090	3039	3048	3063	rVB2	9871	14563	1.09%	0.136%
21	11.470	3157	3166	3177	rBV3	11904	20395	1.53%	0.190%
22	11.746	3242	3252	3260	rBV2	12663	19873	1.49%	0.185%
23	11.811	3260	3272	3305	rVB	532560	891950	66.82%	8.310%
24	12.190	3377	3390	3416	rBV	556014	945679	70.84%	8.811%
25	13.222	3701	3711	3724	rBV2	19981	33013	2.47%	0.308%
26	13.843	3893	3904	3917	rBV3	29549	49245	3.69%	0.459%
27	14.090	3971	3981	4001	rBV2	21334	41924	3.14%	0.391%
28	14.331	4046	4056	4070	rBV3	26494	46158	3.46%	0.430%




Sum of corrected areas: 10733504

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092123\
Data File : VU055450.D
Acq On : 21 Sep 2023 17:00
Operator : MD/SY
Sample : VIBLK140
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK140

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

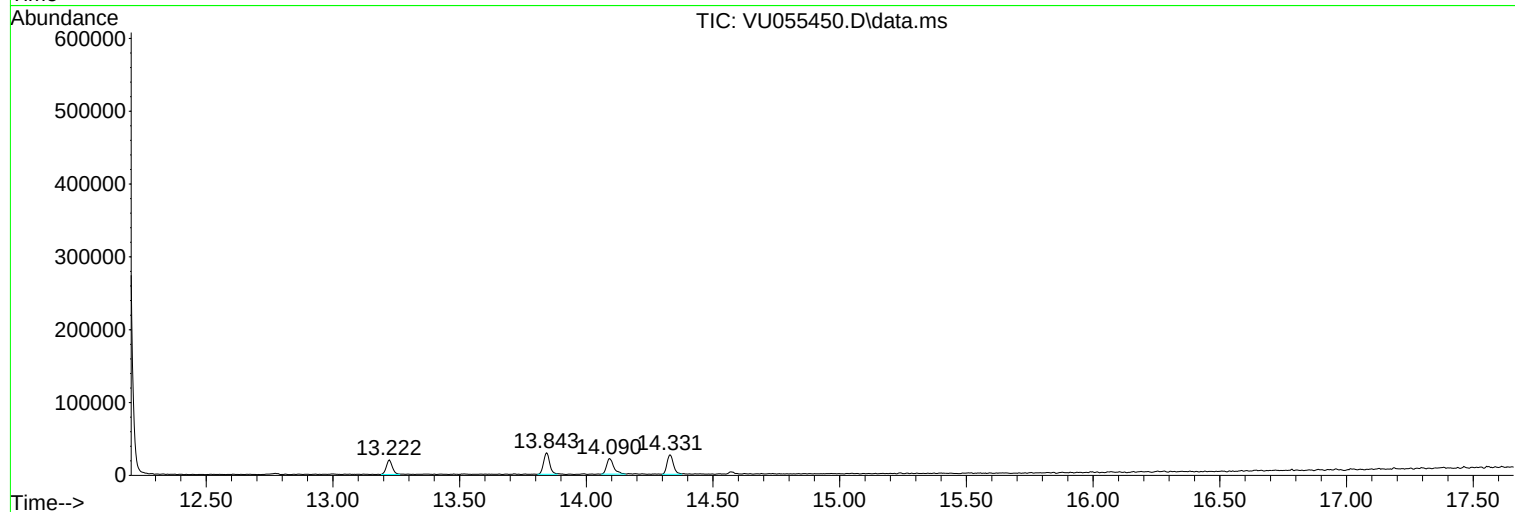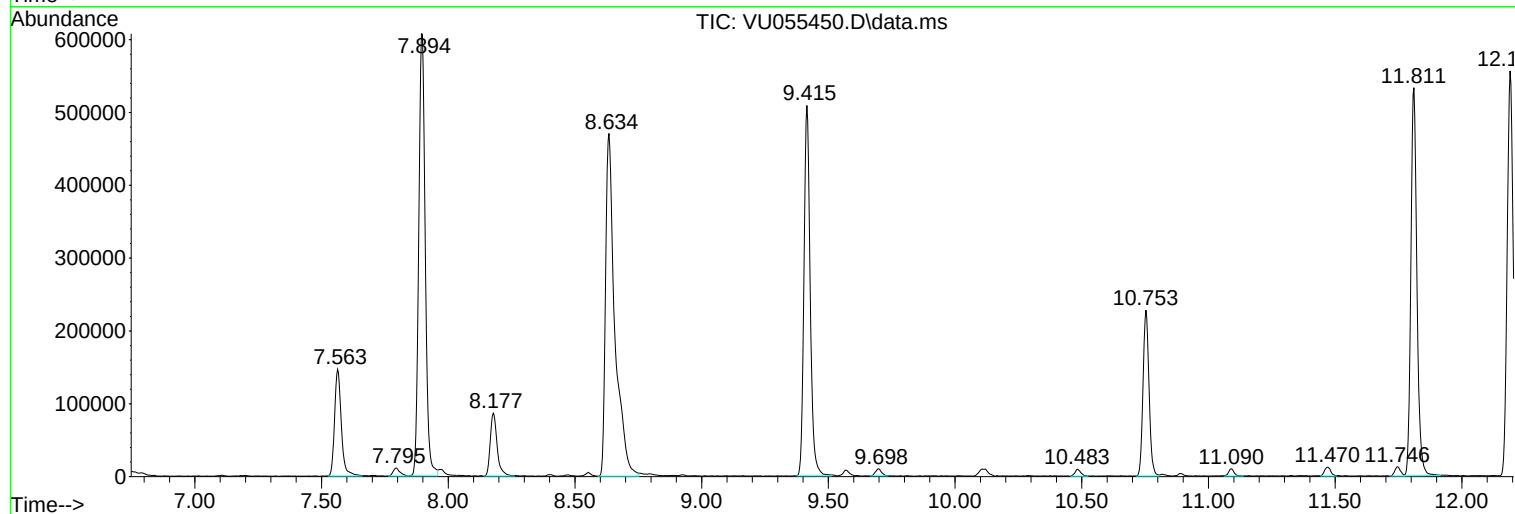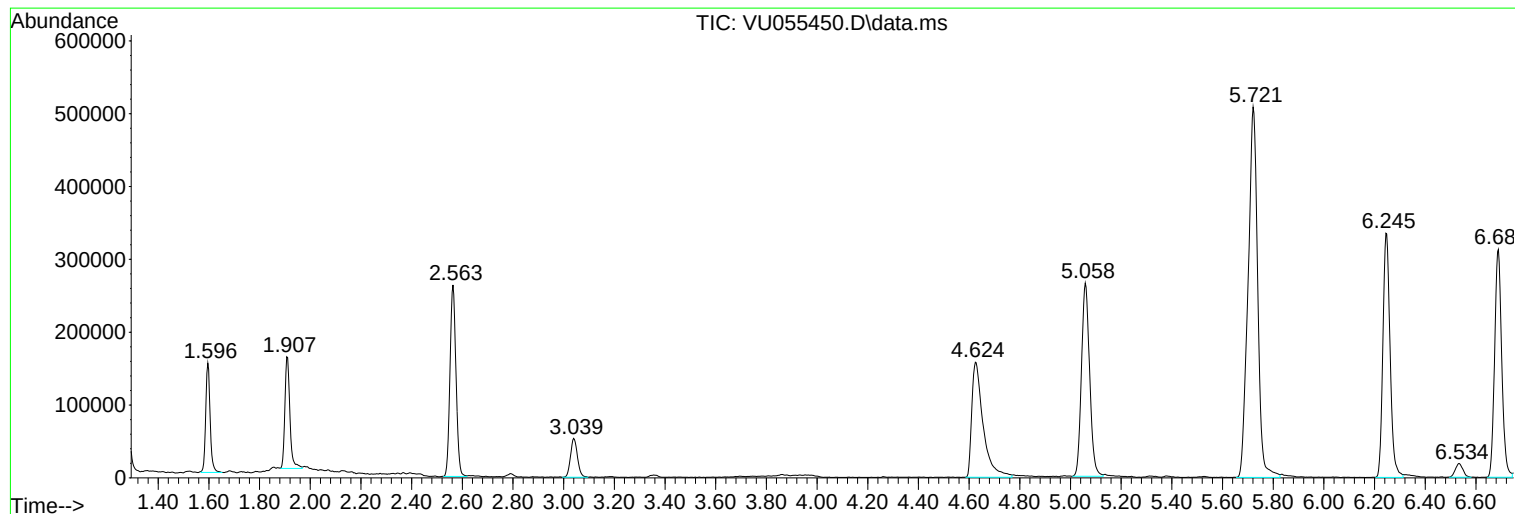

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092123\
Data File : VU055450.D
Acq On : 21 Sep 2023 17:00
Operator : MD/SY
Sample : VIBLK140
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK140

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092123\
Data File : VU055450.D
Acq On : 21 Sep 2023 17:00
Operator : MD/SY
Sample : VIBLK140
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK140

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------