

Data File : VU027018.D
Acq On : 22 Sep 2018 16:11
Operator : MD/SY
Sample : J4958-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BPSI-HN-MW24IR-20180914

Quant Time: Sep 24 02:51:04 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 22 01:31:57 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	96824	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	160378	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	154578	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	70954	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.31	65	96598	49.57	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.14%	
35) Dibromofluoromethane	4.88	113	67246	48.37	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.74%	
50) Toluene-d8	7.57	98	248212	46.85	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.70%	
62) 4-Bromofluorobenzene	10.31	95	83386	45.87	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.74%	


Target Compounds						Qvalue
7) Trichlorofluoromethane	1.89	101	6106	2.642	ug/l	98
9) 1,1,2-Trichlorotrifluoroet	2.29	101	562	0.396	ug/l #	65
11) Tert butyl alcohol	2.84	59	1547	3.463	ug/l #	72
12) 1,1-Dichloroethene	2.29	96	1920	1.436	ug/l	94
14) Allyl chloride	2.44	41	4557	1.680	ug/l #	68
16) Acetone	2.32	43	4261	Below Cal		99
18) Methyl Acetate	2.44	43	11142	4.017	ug/l #	55
19) Methyl tert-butyl Ether	3.00	73	7320	1.490	ug/l	94
24) 1,1-Dichloroethane	3.45	63	2788	0.873	ug/l #	84
25) 2-Butanone	4.20	43	728	0.445	ug/l #	53
26) 2,2-Dichloropropane	4.20	77	921	0.370	ug/l #	55
27) cis-1,2-Dichloroethene	4.24	96	701	0.435	ug/l	50
30) Chloroform	4.67	83	738	0.249	ug/l #	82
31) Cyclohexane	4.99	56	2567	0.312	ug/l #	1
32) 1,1,1-Trichloroethane	4.92	97	520	0.220	ug/l #	41
36) 1,1-Dichloropropene	4.99	75	9358	4.372	ug/l #	50
37) Ethyl Acetate	4.20	43	728	0.251	ug/l #	70
38) Carbon Tetrachloride	4.98	117	10253	5.034	ug/l #	17
44) Trichloroethene	6.19	130	10541	7.609	ug/l	95
51) 4-Methyl-2-Pentanone	7.57	43	1212	0.426	ug/l #	1
60) Dibromochloromethane	8.23	129	7920	5.109	ug/l #	11
64) Tetrachloroethene	8.23	164	7652	6.424	ug/l	93
76) 1,2,3-Trichloropropane	10.31	75	45063	20.905	ug/l #	35
81) trans-1,4-Dichloro-2-buten	10.31	75	45063	66.901	ug/l #	100
89) n-Butylbenzene	11.89	91	61	2.404	ug/l #	33
95) Naphthalene	13.77	128	19	1.692	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU027018.D
Acq On : 22 Sep 2018 16:11
Operator : MD/SY
Sample : J4958-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BPSI-HN-MW24IR-20180914

Quant Time: Sep 24 02:51:04 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 22 01:31:57 2018
Response via : Initial Calibration

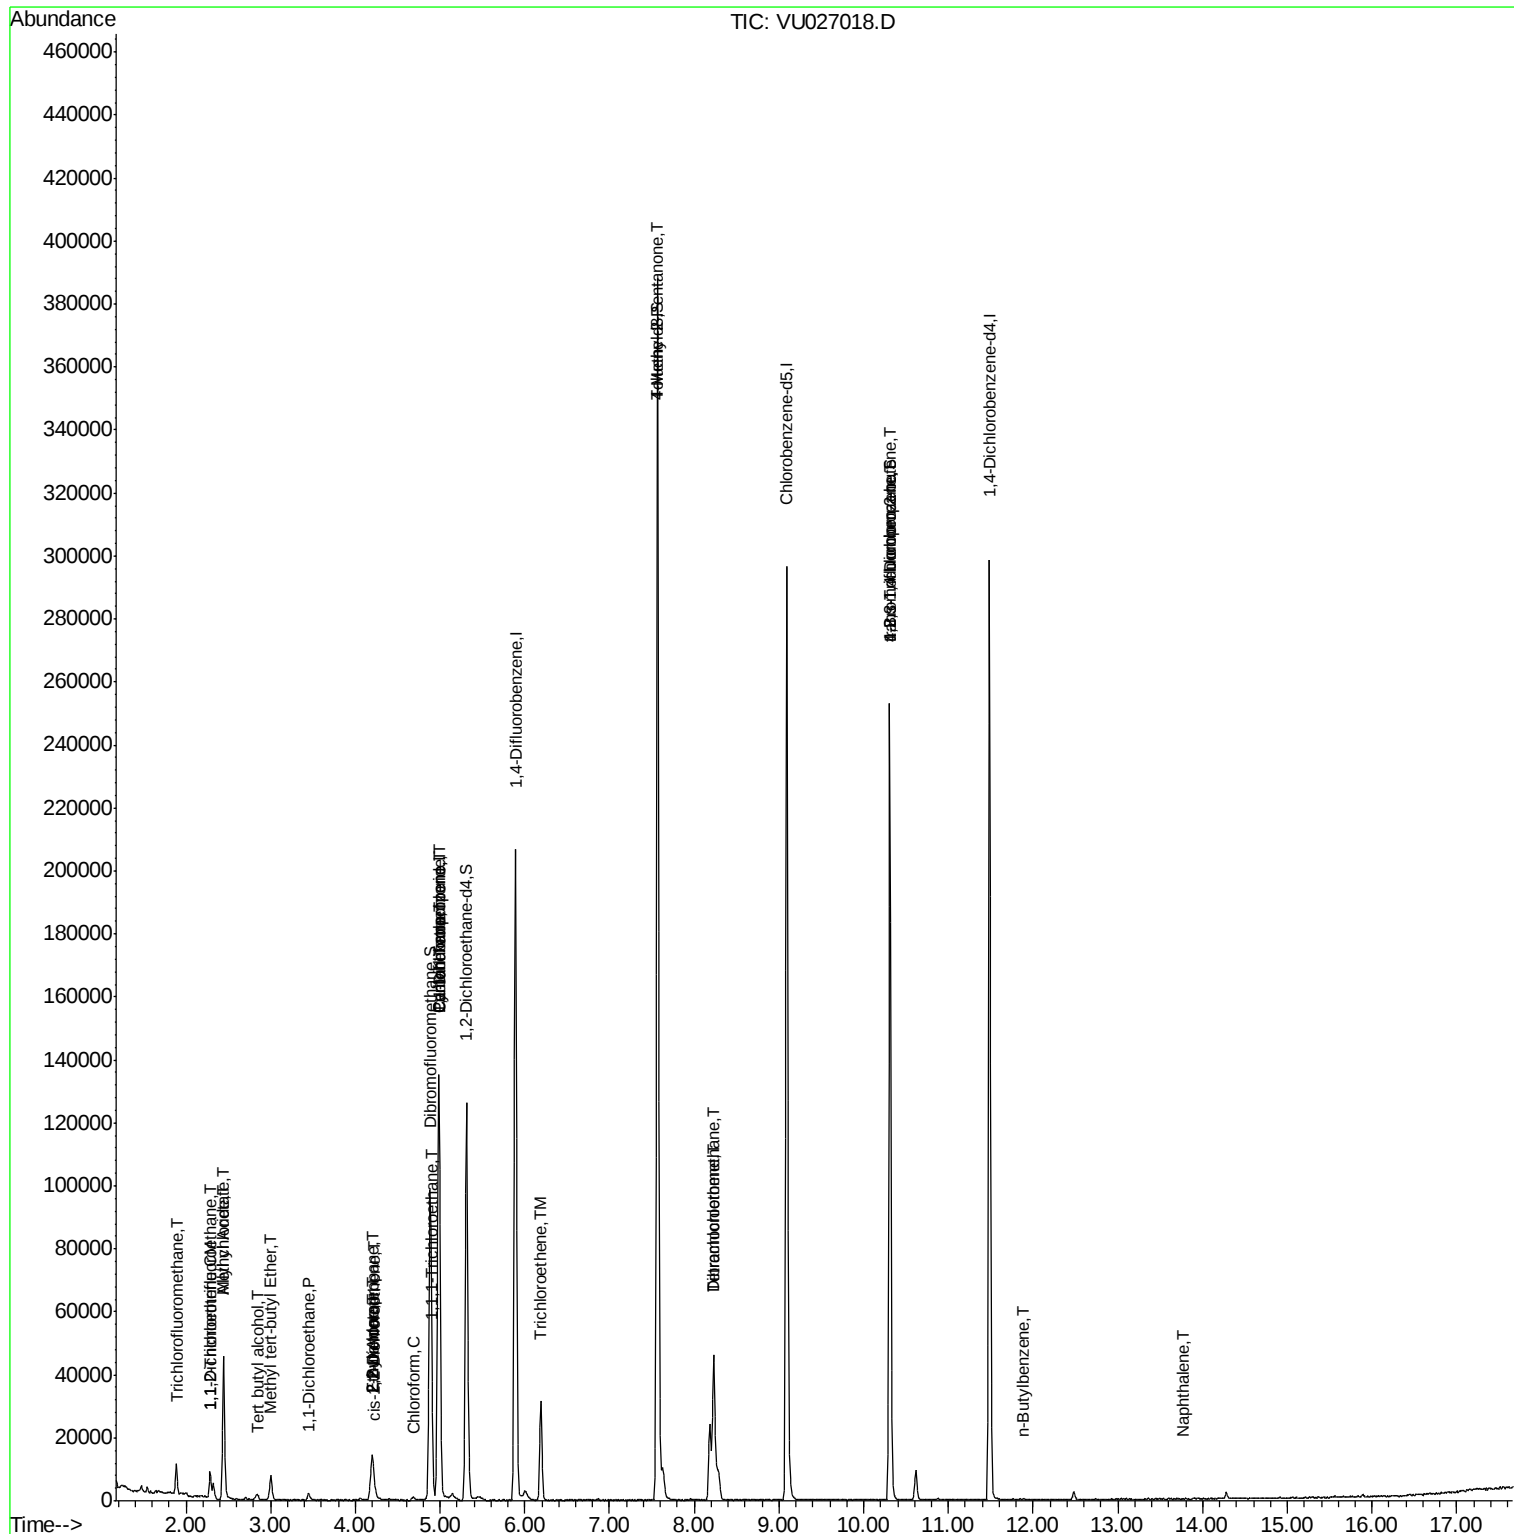



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.99 min Scan# 1186

Delta R.T. 0.00 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11

Instrument :

MSVOA_U

ClientSampleId :


BPSI-HN-MW24IR-20180914

Tgt Ion:168 Resp: 96824

Ion Ratio Lower Upper

168 100

99 63.9 48.1 72.1

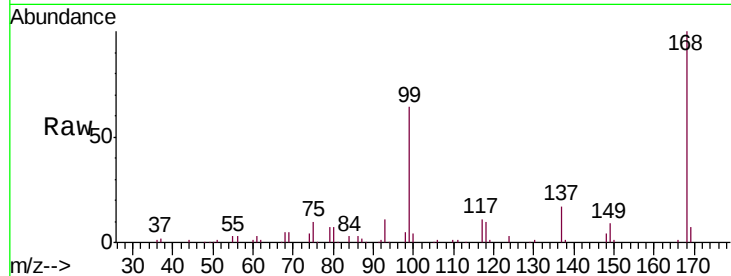

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VU0

4.99

40000

30000

20000

10000



0

4.90

5.00

5.10

Time-->



#7

Trichlorofluoromethane

Concen: 2.642 ug/l

RT: 1.89 min Scan# 222

Delta R.T. 0.00 min

Lab File: VU027018.D


Acq: 22 Sep 2018 16:11

Tgt Ion:101 Resp: 6106

Ion Ratio Lower Upper

101 100

103 63.4 52.2 78.2



Abundance Ion 100.90 (100.60 to 101.60): V

Ion 102.80 (102.50 to 103.50): V

1.89

5000

4000

3000

2000


1000


0

1.85

1.90

Time-->



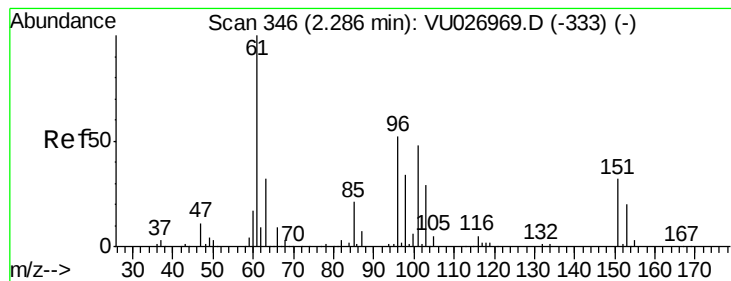

#9

1,1,2-Trichlorotrifluoroethane

Concen: 0.396 ug/l

RT: 2.29 min Scan# 347

Delta R.T. 0.00 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11

Instrument :

MSVOA_U

ClientSampleId :

BPSI-HN-MW24IR-20180914





Tgt Ion: 101 Resp: 562

Ion Ratio Lower Upper

101 100

85 18.1 36.2 54.2#

151 42.7 54.5 81.7#

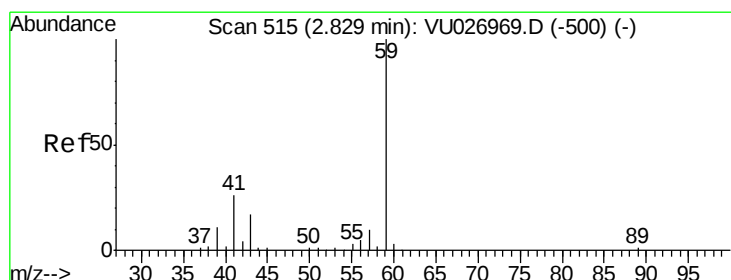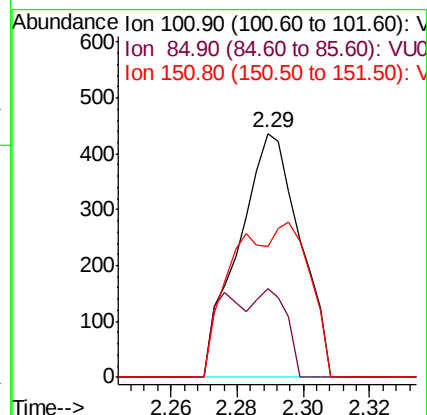

#11

Tert butyl alcohol

Concen: 3.463 ug/l

RT: 2.84 min Scan# 518

Delta R.T. 0.01 min

Lab File: VU027018.D




Acq: 22 Sep 2018 16:11


Tgt Ion: 59 Resp: 1547

Ion Ratio Lower Upper

59 100

57 0.0 8.5 12.7#

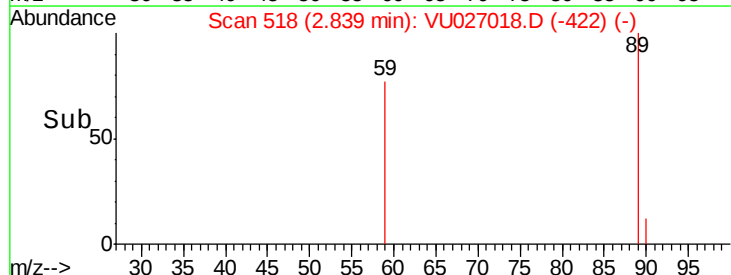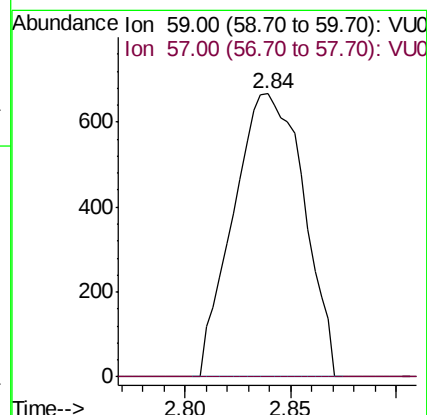



#12

1,1-Dichloroethene

Concen: 1.436 ug/l

RT: 2.29 min Scan# 346

Delta R.T. 0.00 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11

Instrument :

MSVOA_U

ClientSampleId :

BPSI-HN-MW24IR-20180914


Tgt Ion: 96 Resp: 1920

Ion Ratio Lower Upper

96 100

61 205.2 156.1 234.1




98 67.2 51.4 77.0

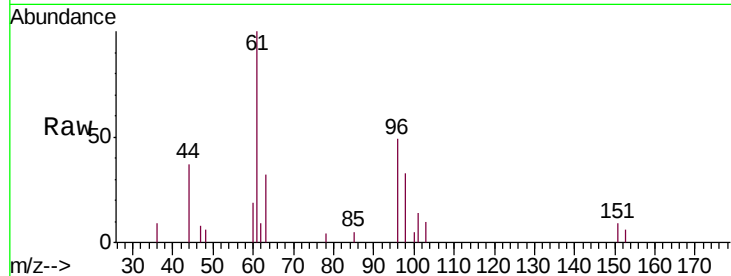

Abundance Ion 95.90 (95.60 to 96.60): VU0

Ion 60.90 (60.60 to 61.60): VU0

Ion 97.90 (97.60 to 98.60): VU0

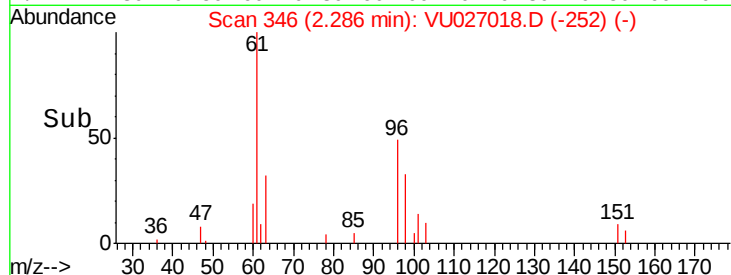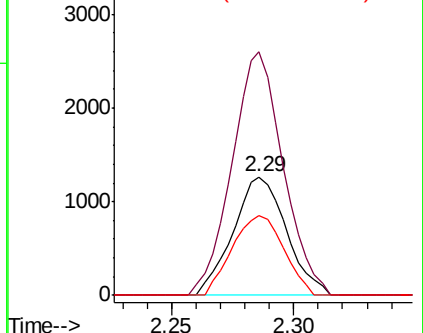

#14

Allyl chloride

Concen: 1.680 ug/l

RT: 2.44 min Scan# 394

Delta R.T. -0.15 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11


Tgt Ion: 41 Resp: 4557

Ion Ratio Lower Upper

41 100

39 85.0 55.7 83.5#



76 0.0 26.5 39.7#




Abundance Ion 41.00 (40.70 to 41.70): VU0

Ion 39.00 (38.70 to 39.70): VU0

Ion 75.90 (75.60 to 76.60): VU0

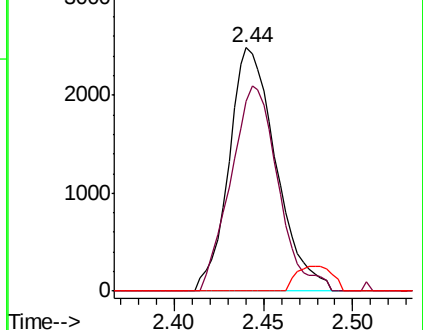



#16

Acetone

Concen: Below Cal

RT: 2.32 min Scan# 357

Delta R.T. -0.00 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11

Instrument :

MSVOA_U

ClientSampleId :





BPSI-HN-MW24IR-20180914

Tgt Ion: 43 Resp: 4261

Ion Ratio Lower Upper

43 100

58 30.4 24.6 36.8

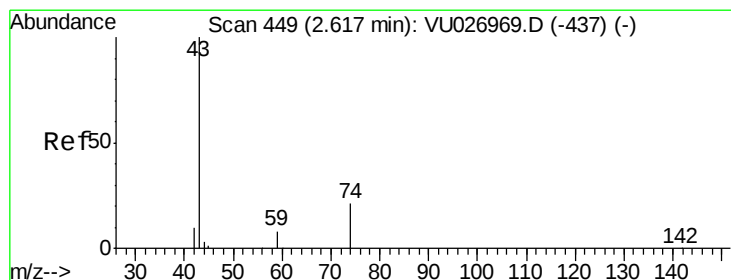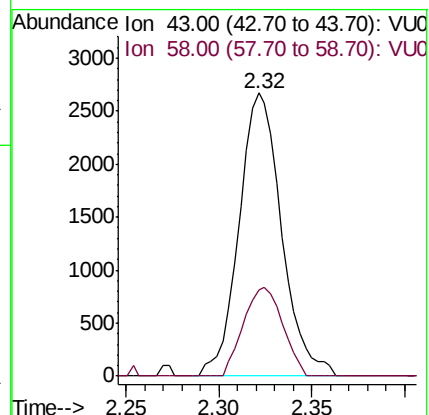

#18

Methyl Acetate

Concen: 4.017 ug/l

RT: 2.44 min Scan# 395

Delta R.T. -0.17 min

Lab File: VU027018.D




Acq: 22 Sep 2018 16:11


Tgt Ion: 43 Resp: 11142

Ion Ratio Lower Upper

43 100

74 0.0 16.6 25.0#



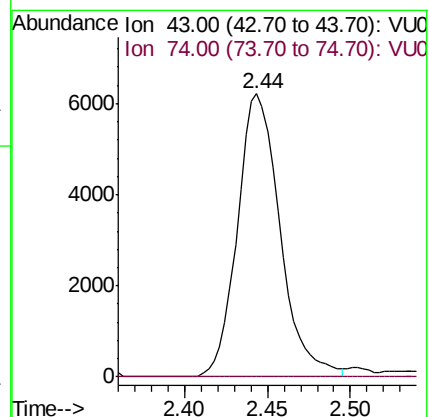
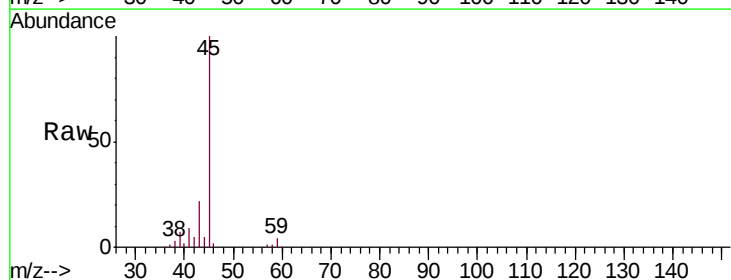


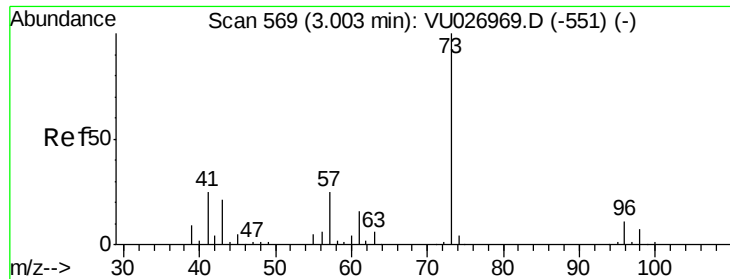

#19
Methyl tert-butyl Ether
Concen: 1.490 ug/l
RT: 3.00 min Scan# 569
Delta R.T. 0.00 min
Lab File: VU027018.D
Acq: 22 Sep 2018 16:11




Instrument :
MSVOA_U
ClientSampleId :
BPSI-HN-MW24IR-20180914


Tgt Ion: 73 Resp: 7320
Ion Ratio Lower Upper
73 100
57 21.6 19.8 29.6

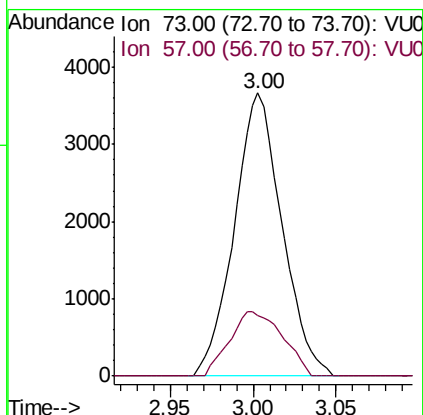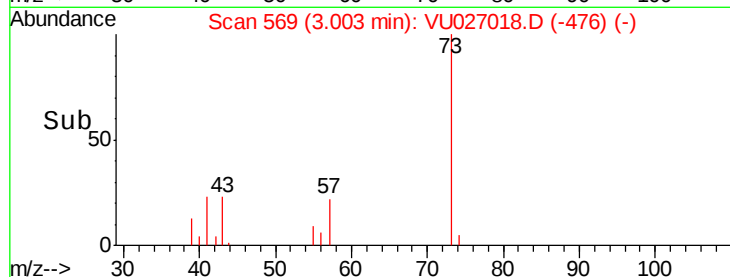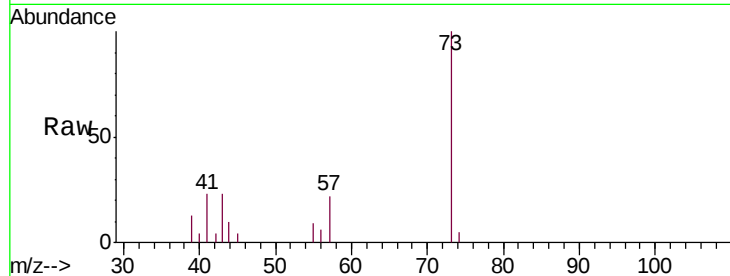

#24
1,1-Dichloroethane
Concen: 0.873 ug/l
RT: 3.45 min Scan# 708
Delta R.T. 0.00 min
Lab File: VU027018.D
Acq: 22 Sep 2018 16:11

Tgt Ion: 63 Resp: 2788
Ion Ratio Lower Upper
63 100
98 0.0 3.3 9.8#
100 0.0 2.0 5.8#


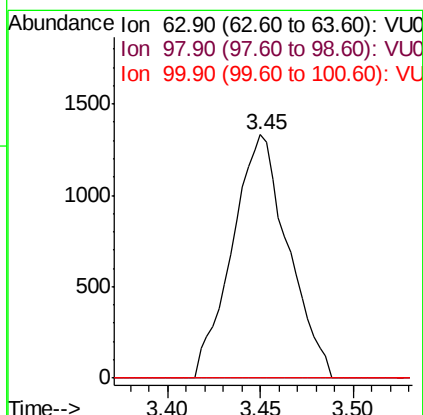
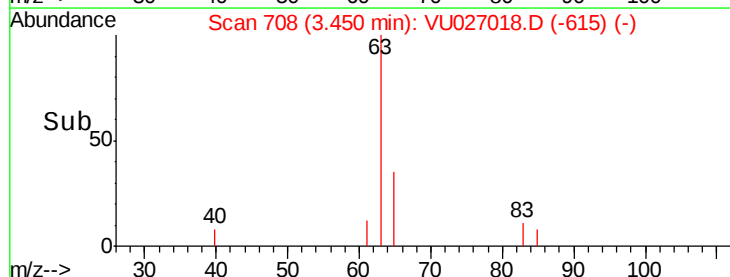



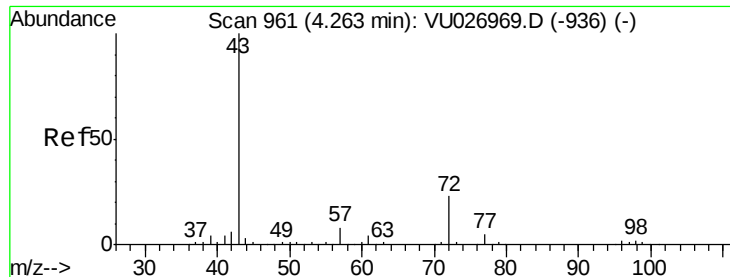

#25
 2-Butanone
 Concen: 0.445 ug/l
 RT: 4.20 min Scan# 941
 Delta R.T. -0.06 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11




Instrument :
 MSVOA_U
 ClientSampleId :
 BPSI-HN-MW24IR-20180914


Tgt Ion: 43 Resp: 728
 Ion Ratio Lower Upper
 43 100
 72 0.0 18.4 27.6#

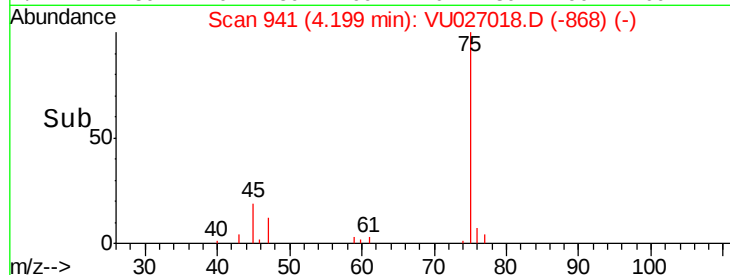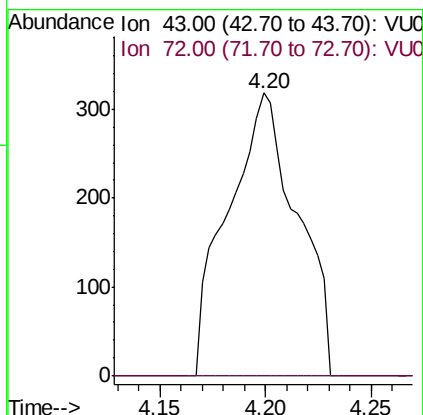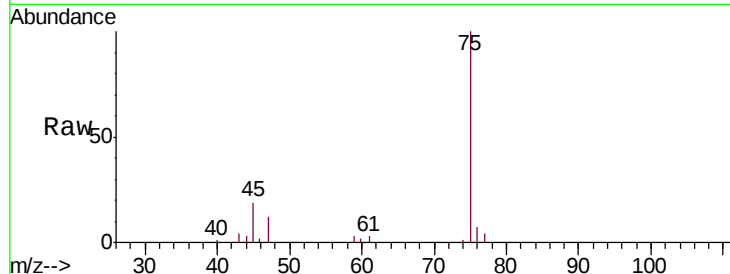

#26
 2,2-Dichloropropane
 Concen: 0.370 ug/l
 RT: 4.20 min Scan# 941
 Delta R.T. -0.03 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11

Tgt Ion: 77 Resp: 921
 Ion Ratio Lower Upper
 77 100
 97 0.0 10.5 31.5#

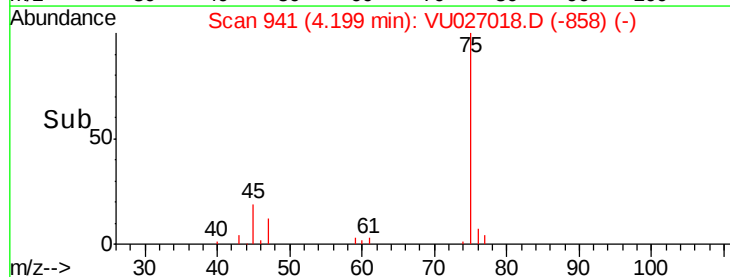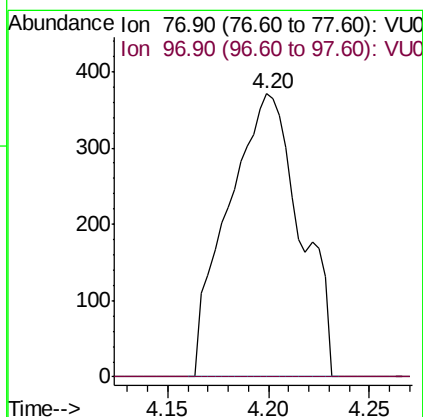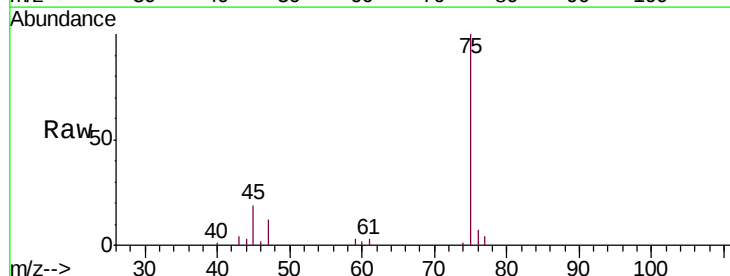




#27


cis-1,2-Dichloroethene
 Concen: 0.435 ug/l
 RT: 4.24 min Scan# 953
 Delta R.T. 0.01 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11

Instrument :
 MSVOA_U
 ClientSampleId :
 BPSI-HN-MW24IR-20180914



Tgt Ion: 96 Resp: 701
 Ion Ratio Lower Upper
 96 100
 61 254.8 0.0 337.2
 98 51.8 0.0 127.6

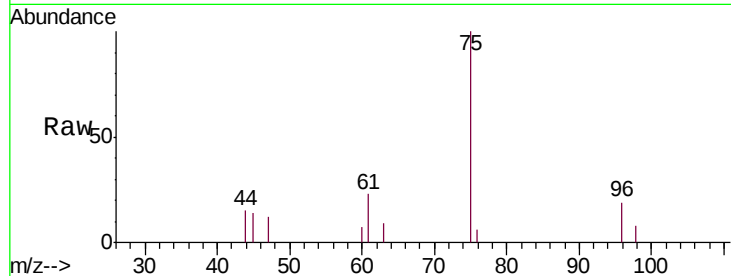

Abundance Ion 95.90 (95.60 to 96.60): VU0
 Ion 60.90 (60.60 to 61.60): VU0
 Ion 97.90 (97.60 to 98.60): VU0

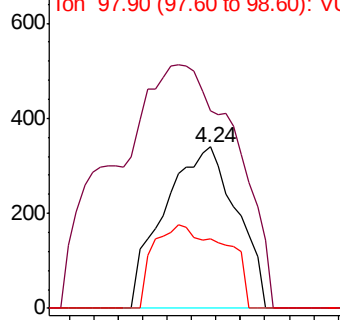


Time-->




#30

Chloroform
 Concen: 0.249 ug/l
 RT: 4.67 min Scan# 1089
 Delta R.T. 0.00 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11


Tgt Ion: 83 Resp: 738
 Ion Ratio Lower Upper
 83 100
 85 50.0 51.5 77.3#

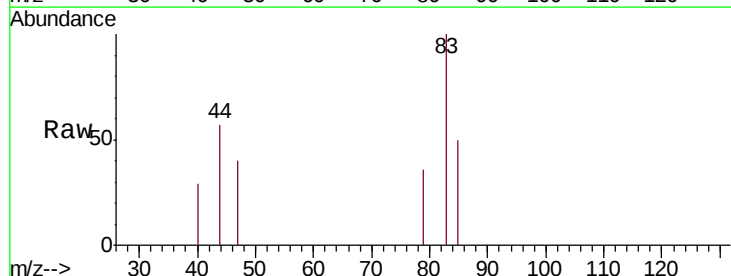


Abundance Ion 82.90 (82.60 to 83.60): VU0
 Ion 84.90 (84.60 to 85.60): VU0

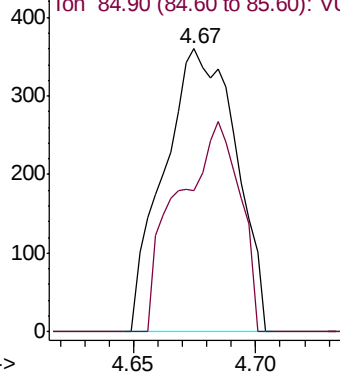

Time-->









#31
Cyclohexane
Concen: 0.312 ug/l
RT: 4.99 min Scan# 1186
Delta R.T. -0.01 min
Lab File: VU027018.D
Acq: 22 Sep 2018 16:11

Instrument :
MSVOA_U
ClientSampleId :
BPSI-HN-MW24IR-20180914

Tgt Ion: 56 Resp: 2567
Ion Ratio Lower Upper
56 100
69 164.7 23.0 34.4#
84 120.6 61.4 92.2#

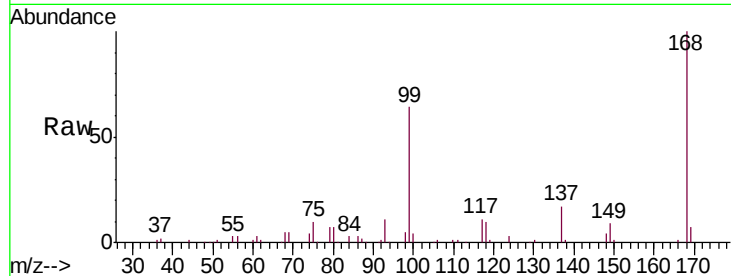


Abundance Ion 56.00 (55.70 to 56.70): VU0
Ion 69.00 (68.70 to 69.70): VU0
Ion 84.00 (83.70 to 84.70): VU0


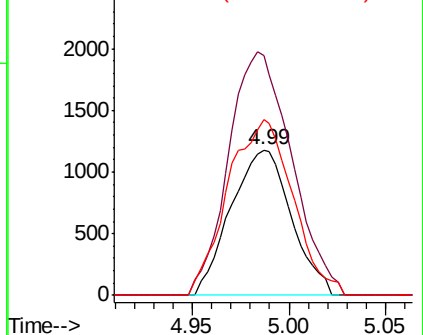



#32
1,1,1-Trichloroethane
Concen: 0.220 ug/l
RT: 4.92 min Scan# 1164
Delta R.T. -0.00 min
Lab File: VU027018.D
Acq: 22 Sep 2018 16:11

Tgt Ion: 97 Resp: 520
Ion Ratio Lower Upper
97 100
99 0.0 51.8 77.6#
61 30.8 41.1 61.7#

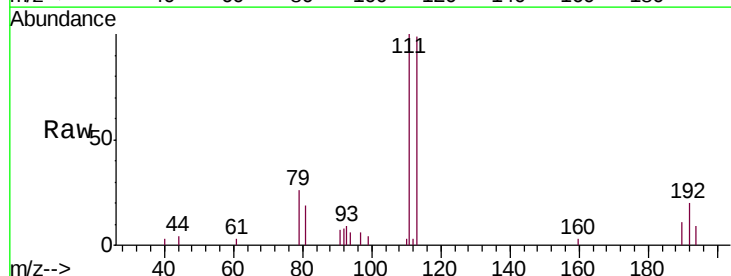

Abundance Ion 96.90 (96.60 to 97.60): VU0
Ion 98.90 (98.60 to 99.60): VU0
Ion 60.90 (60.60 to 61.60): VU0




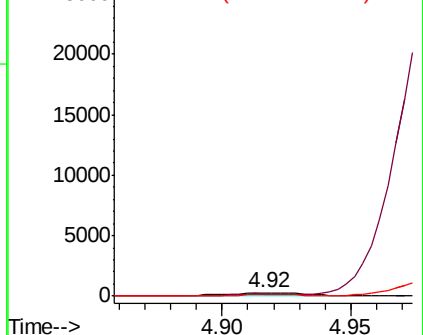


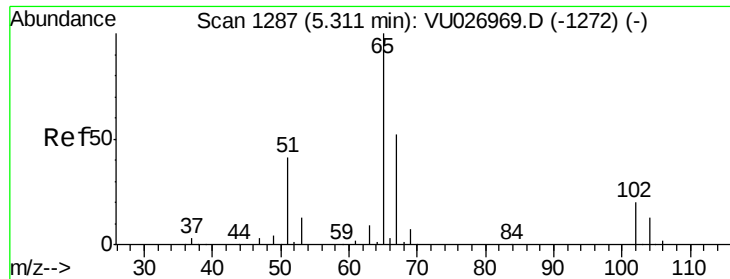

#33
 1,2-Dichloroethane-d4
 Concen: 49.569 ug/l
 RT: 5.31 min Scan# 1287
 Delta R.T. 0.00 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11




Instrument :
 MSVOA_U
 ClientSampleId :
 BPSI-HN-MW24IR-20180914


Tgt Ion: 65 Resp: 96598
 Ion Ratio Lower Upper
 65 100
 67 53.0 0.0 105.6

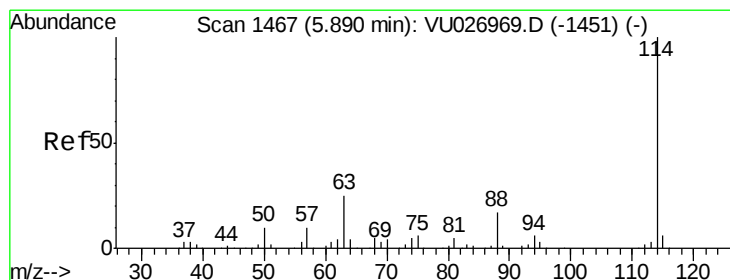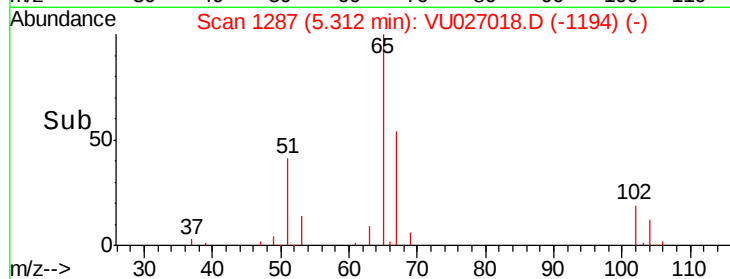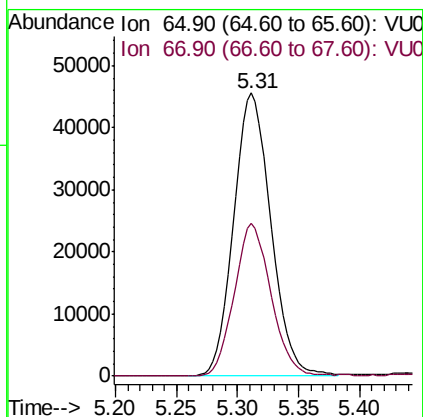

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.89 min Scan# 1467
 Delta R.T. 0.00 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11

Tgt Ion: 114 Resp: 160378
 Ion Ratio Lower Upper
 114 100
 63 24.6 0.0 49.2
 88 17.2 0.0 33.8

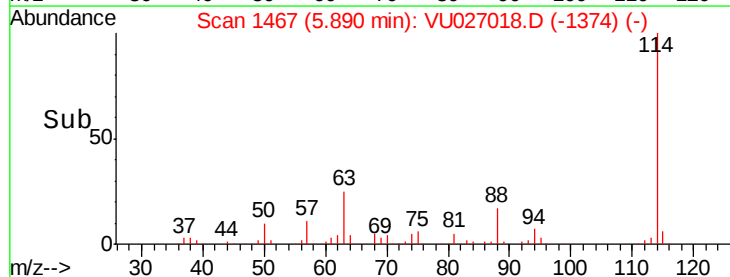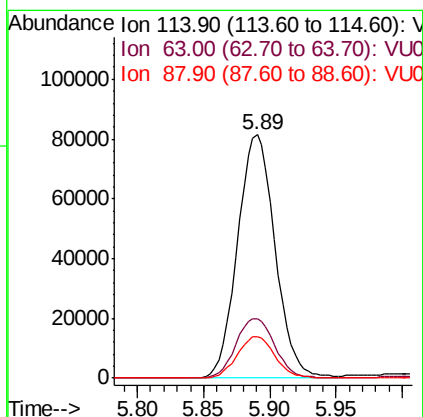

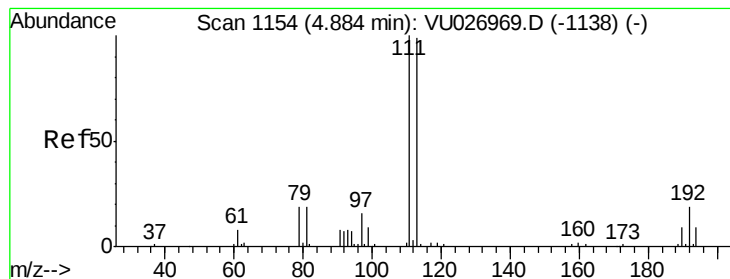

#35

Dibromofluoromethane

Concen: 48.373 ug/l

RT: 4.88 min Scan# 1154

Delta R.T. 0.00 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11

Instrument :

MSVOA_U

ClientSampleId :

BPSI-HN-MW24IR-20180914


Tgt Ion:113 Resp: 67246

Ion Ratio Lower Upper

113 100

111 103.5 82.2 123.4




192 18.4 15.2 22.8



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

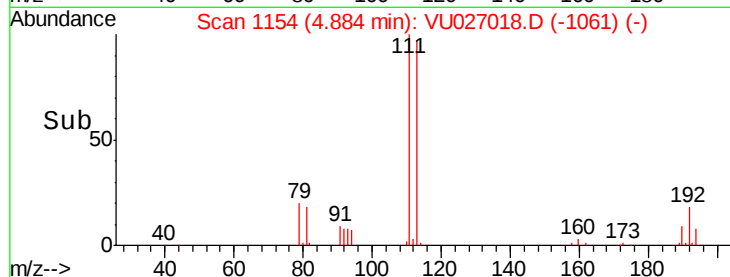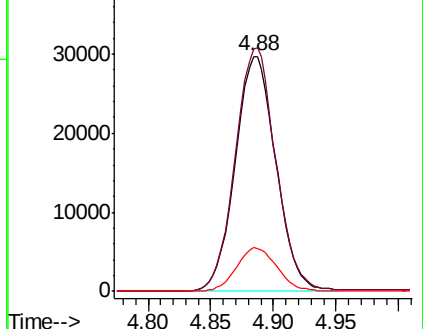

#36

1,1-Dichloropropene

Concen: 4.372 ug/l

RT: 4.99 min Scan# 1186

Delta R.T. -0.15 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11


Tgt Ion: 75 Resp: 9358

Ion Ratio Lower Upper

75 100

110 7.2 16.1 48.2#



77 0.0 24.6 36.8#




Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VU0



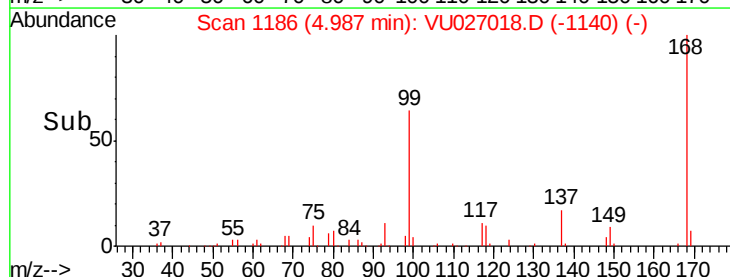
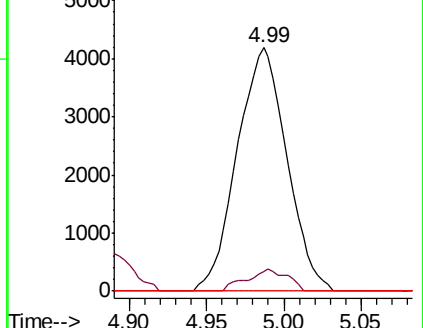




#37
 Ethyl Acetate
 Concen: 0.251 ug/l
 RT: 4.20 min Scan# 941
 Delta R.T. -0.18 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11




Instrument :
 MSVOA_U
 ClientSampleId :
 BPSI-HN-MW24IR-20180914


Tgt Ion: 43 Resp: 728
 Ion Ratio Lower Upper
 43 100
 61 0.0 10.5 15.7#
 70 0.0 7.4 11.0#

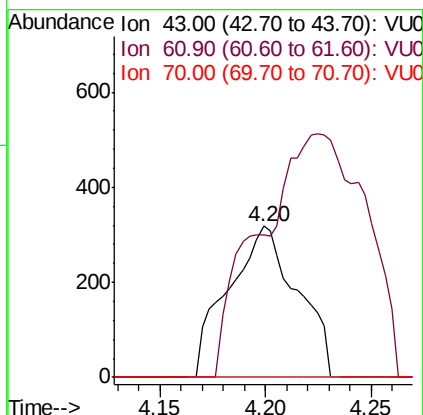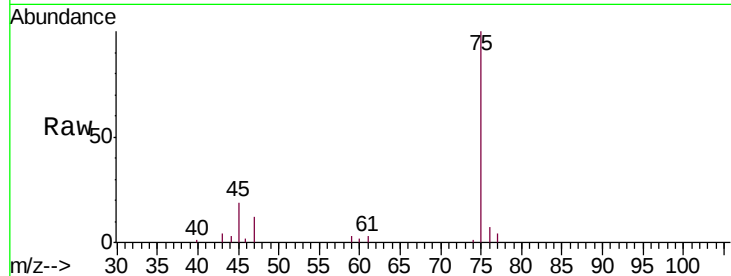

#38
 Carbon Tetrachloride
 Concen: 5.034 ug/l
 RT: 4.98 min Scan# 1185
 Delta R.T. -0.15 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11

Tgt Ion: 117 Resp: 10253
 Ion Ratio Lower Upper
 117 100
 119 5.3 74.4 111.6#
 121 0.0 24.2 36.4#

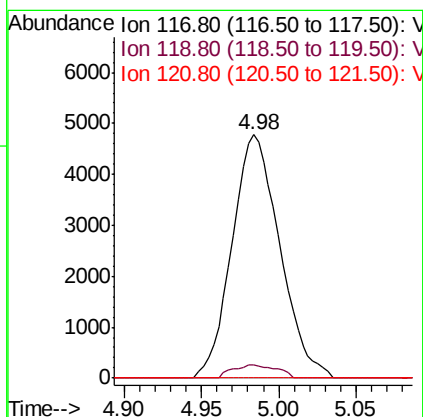



#44

Trichloroethene

Concen: 7.609 ug/l

RT: 6.19 min Scan# 1561

Delta R.T. 0.00 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11

Instrument :

MSVOA_U

ClientSampleId :


BPSI-HN-MW24IR-20180914

Tgt Ion:130 Resp: 10541

Ion Ratio Lower Upper




130 100

95 109.7 0.0 208.8



Abundance Ion 129.80 (129.50 to 130.50): VU026969.D (-1545) (-)

Ion 94.90 (94.60 to 95.60): VU026969.D (-1545) (-)

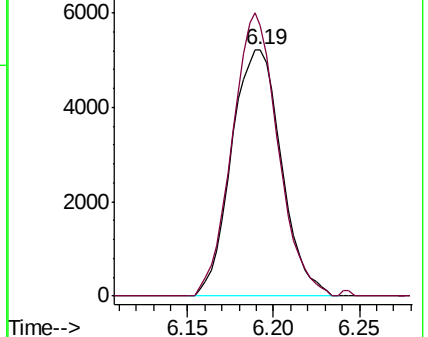

#50

Toluene-d8

Concen: 46.851 ug/l

RT: 7.57 min Scan# 1989

Delta R.T. 0.00 min

Lab File: VU027018.D


Acq: 22 Sep 2018 16:11

Tgt Ion: 98 Resp: 248212

Ion Ratio Lower Upper



98 100


100 64.0 52.1 78.1



Abundance Ion 98.00 (97.70 to 98.70): VU026969.D (-1974) (-)

Ion 100.00 (99.70 to 100.70): VU026969.D (-1974) (-)




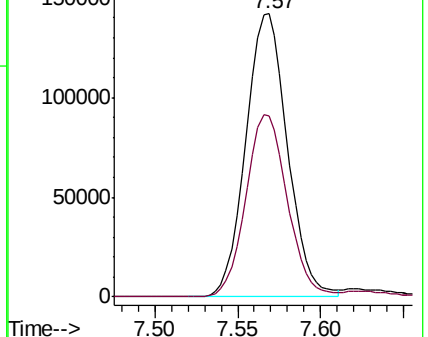




#51
 4-Methyl-2-Pentanone
 Concen: 0.426 ug/l
 RT: 7.57 min Scan# 1988
 Delta R.T. 0.10 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11




Instrument :
 MSVOA_U
 ClientSampleId :
 BPSI-HN-MW24IR-20180914


Tgt Ion: 43 Resp: 1212
 Ion Ratio Lower Upper
 43 100
 58 194.0 29.8 44.6#

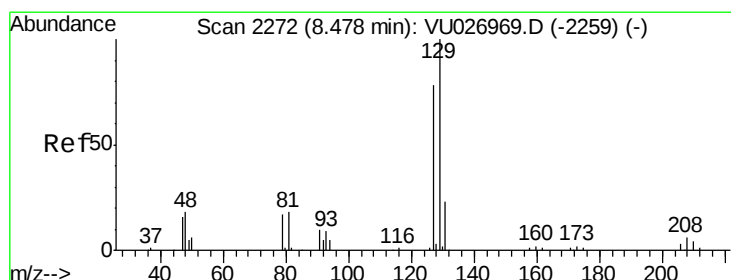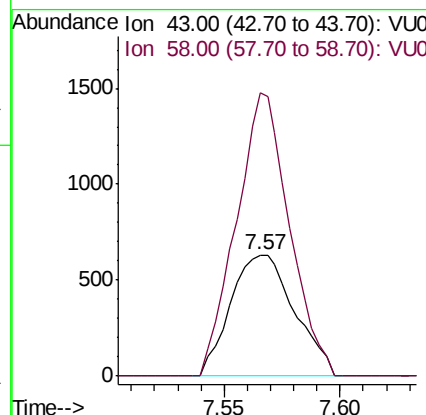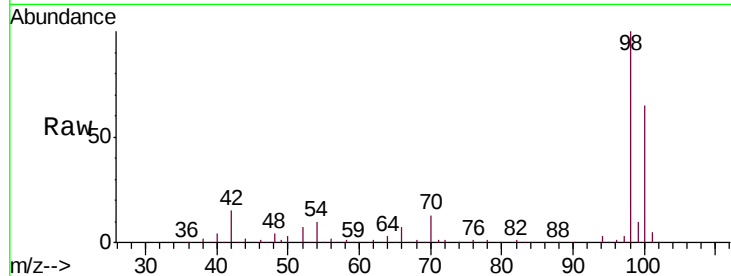

#60
 Dibromochloromethane
 Concen: 5.109 ug/l
 RT: 8.23 min Scan# 2195
 Delta R.T. -0.25 min
 Lab File: VU027018.D
 Acq: 22 Sep 2018 16:11

Tgt Ion: 129 Resp: 7920
 Ion Ratio Lower Upper
 129 100
 127 0.0 38.1 114.5#

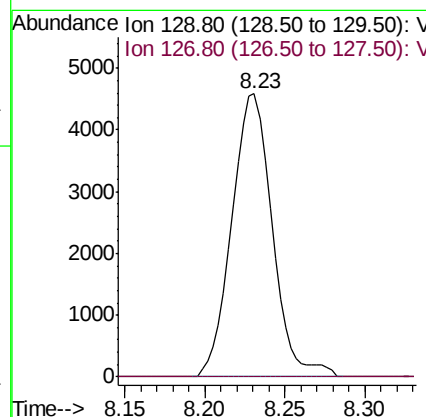

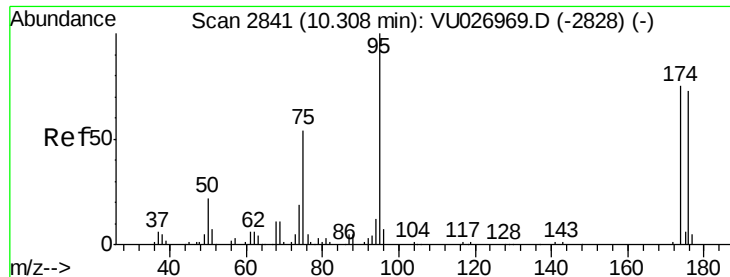

#62

4-Bromofluorobenzene

Concen: 45.870 ug/l

RT: 10.31 min Scan# 2841

Delta R.T. 0.00 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11

Instrument :

MSVOA_U

ClientSampleId :

BPSI-HN-MW24IR-20180914


Tgt Ion: 95 Resp: 83386

Ion Ratio Lower Upper

95 100

174 73.2 0.0 150.2




176 70.0 0.0 145.2

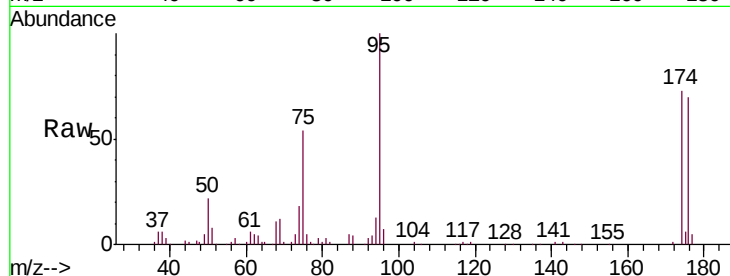

Abundance Ion 94.90 (94.60 to 95.60): VU0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

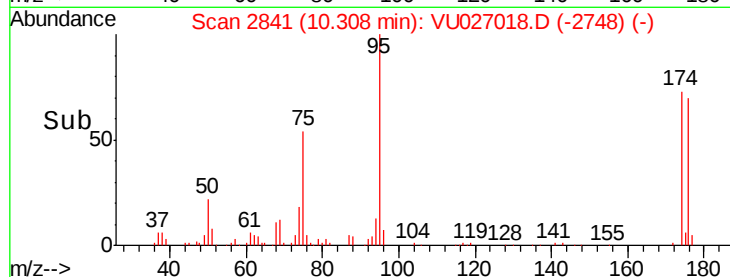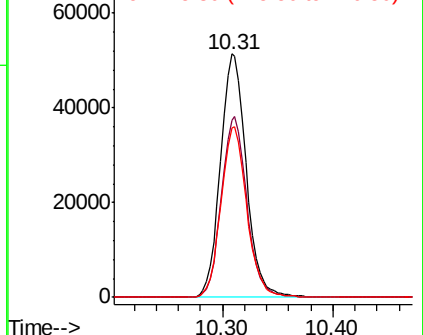

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.09 min Scan# 2463

Delta R.T. 0.00 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11


Tgt Ion: 117 Resp: 154578

Ion Ratio Lower Upper

117 100

82 62.7 48.0 72.0



119 32.3 25.8 38.8




Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VU0

Ion 118.90 (118.60 to 119.60): V

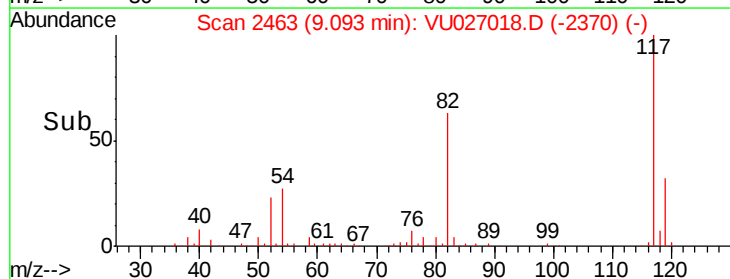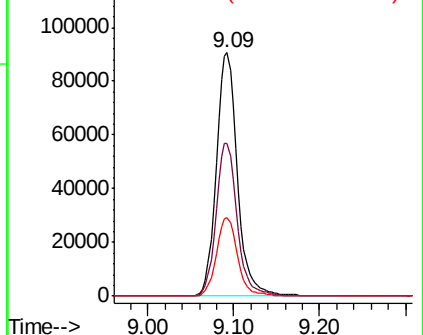


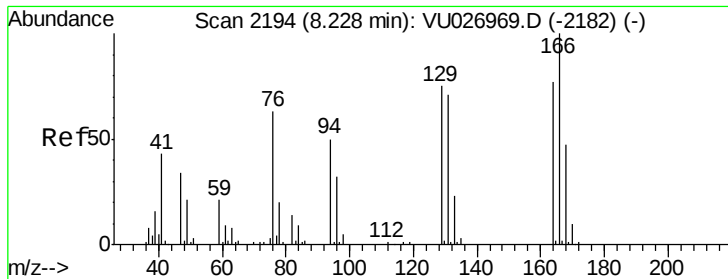




#64
Tetrachloroethene
Concen: 6.424 ug/l
RT: 8.23 min Scan# 2194
Delta R.T. 0.00 min
Lab File: VU027018.D
Acq: 22 Sep 2018 16:11

Instrument :
MSVOA_U
ClientSampleId :
BPSI-HN-MW24IR-20180914

Tgt Ion:164 Resp: 7652
Ion Ratio Lower Upper
164 100
166 136.1 104.4 156.6
129 107.8 78.7 118.1
131 99.9 73.9 110.9

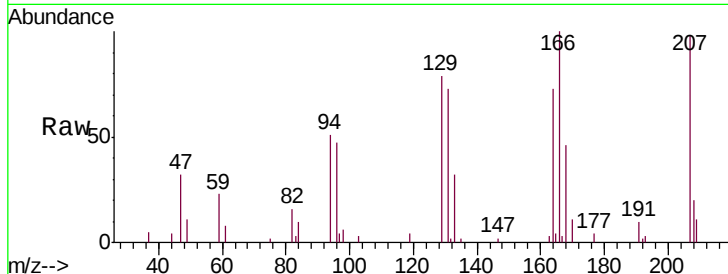


Abundance Ion 163.80 (163.50 to 164.50): V
Ion 165.80 (165.50 to 166.50): V
Ion 128.80 (128.50 to 129.50): V
Ion 130.80 (130.50 to 131.50): V

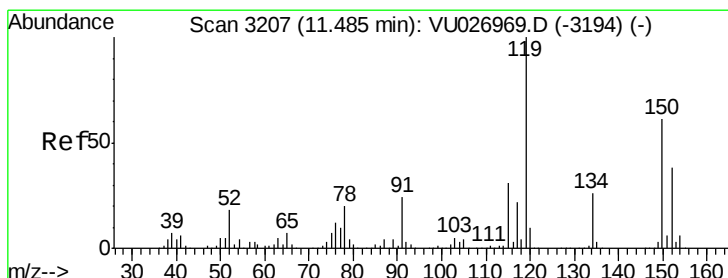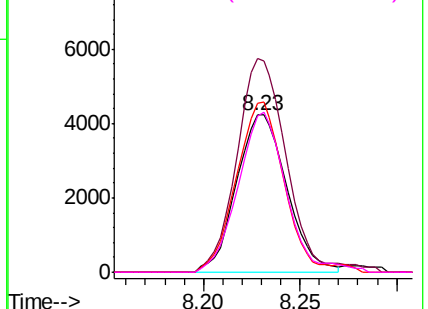
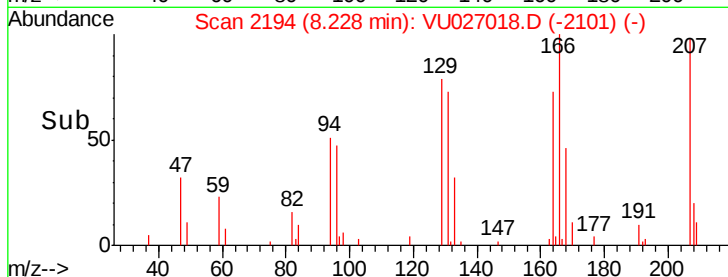



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.48 min Scan# 3207
Delta R.T. 0.00 min
Lab File: VU027018.D
Acq: 22 Sep 2018 16:11

Tgt Ion:152 Resp: 70954
Ion Ratio Lower Upper
152 100
115 61.5 44.9 134.5
150 158.1 0.0 355.8

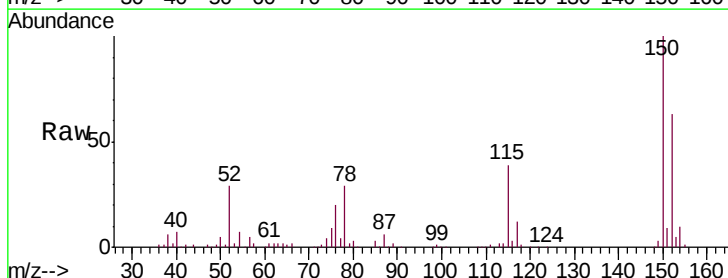

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

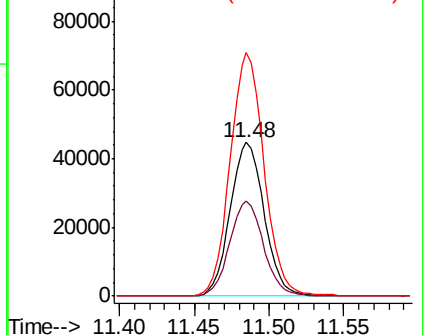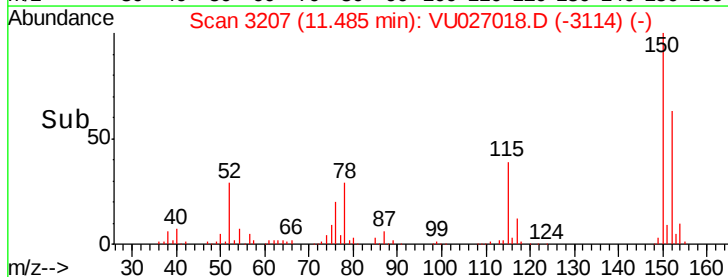

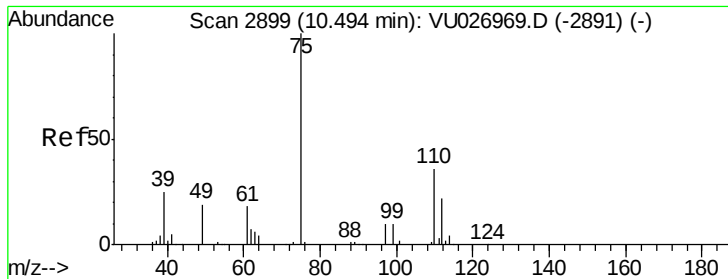

#76

1,2,3-Trichloropropane

Concen: 20.905 ug/l

RT: 10.31 min Scan# 2841

Delta R.T. -0.19 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11

Instrument :

MSVOA_U

ClientSampleId :


BPSI-HN-MW24IR-20180914

Tgt Ion: 75 Resp: 45063

Ion Ratio Lower Upper




75 100

77 1.1 20.9 62.8#

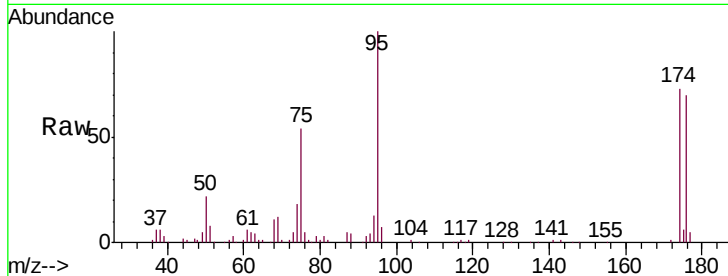

Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 77.00 (76.70 to 77.70): VU0

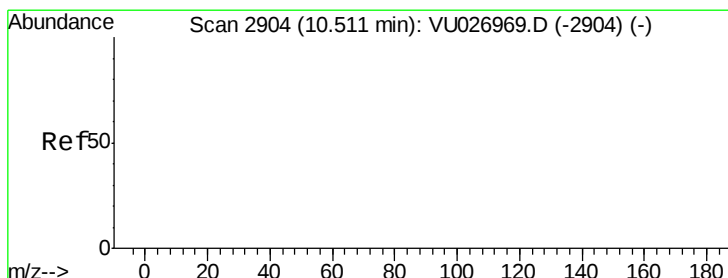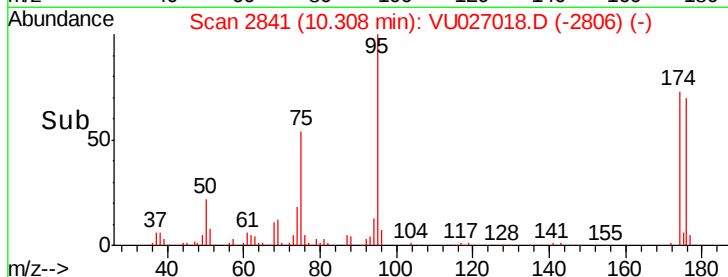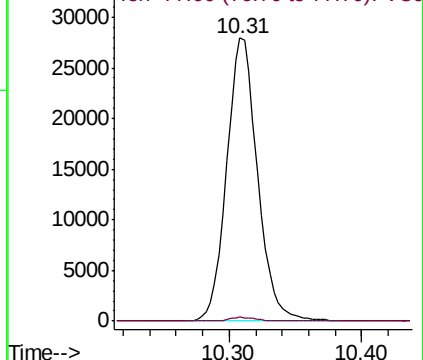

#81

trans-1,4-Dichloro-2-butene

Concen: 66.901 ug/l

RT: 10.31 min Scan# 2841

Delta R.T. -0.21 min

Lab File: VU027018.D

Acq: 22 Sep 2018 16:11


Tgt Ion: 75 Resp: 45063

Ion Ratio Lower Upper

75 100

53 0.0 0.0 0.0



89 0.0 0.0 0.0

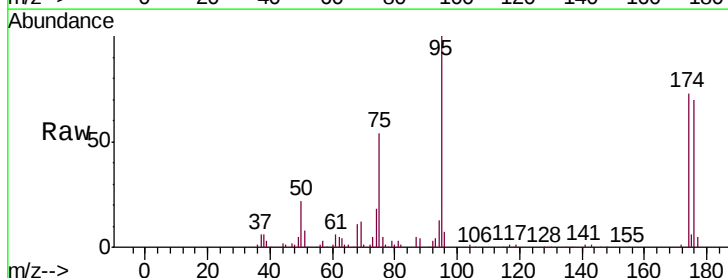


Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 53.00 (52.70 to 53.70): VU0

Ion 88.90 (88.60 to 89.60): VU0



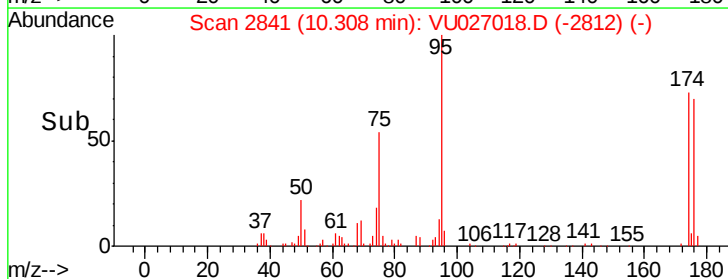
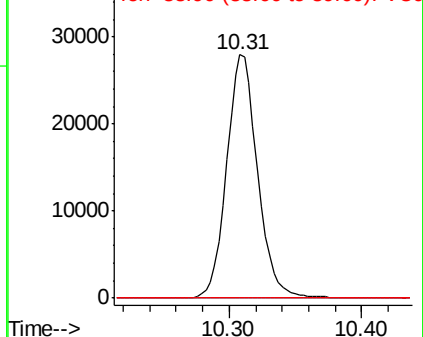




#89
n-Butylbenzene
Concen: 2.404 ug/l
RT: 11.89 min Scan# 3333
Delta R.T. 0.00 min
Lab File: VU027018.D
Acq: 22 Sep 2018 16:11

Instrument :
MSVOA_U
ClientSampleId :
BPSI-HN-MW24IR-20180914

Tgt Ion: 91 Resp: 61
Ion Ratio Lower Upper
91 100
92 0.0 27.1 81.2#
134 0.0 11.7 35.0#

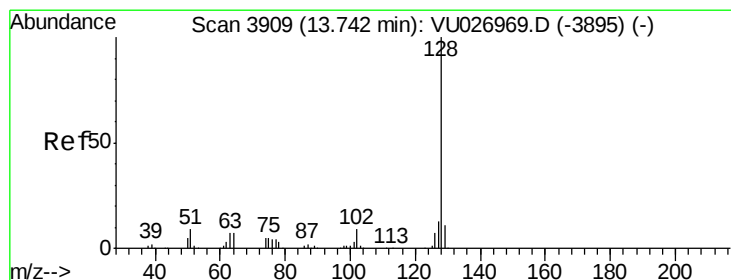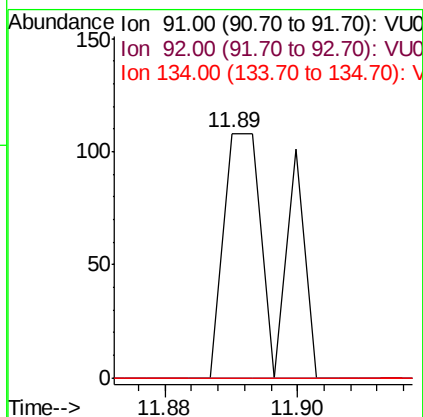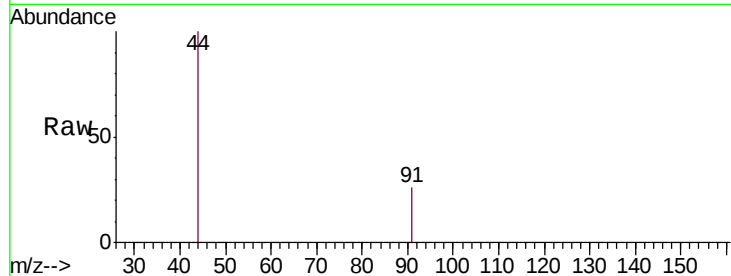

#95
Naphthalene
Concen: 1.692 ug/l
RT: 13.77 min Scan# 3918
Delta R.T. 0.03 min
Lab File: VU027018.D
Acq: 22 Sep 2018 16:11

Tgt Ion: 128 Resp: 19
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.6 12.8#

