



Acetone

Response Ratio

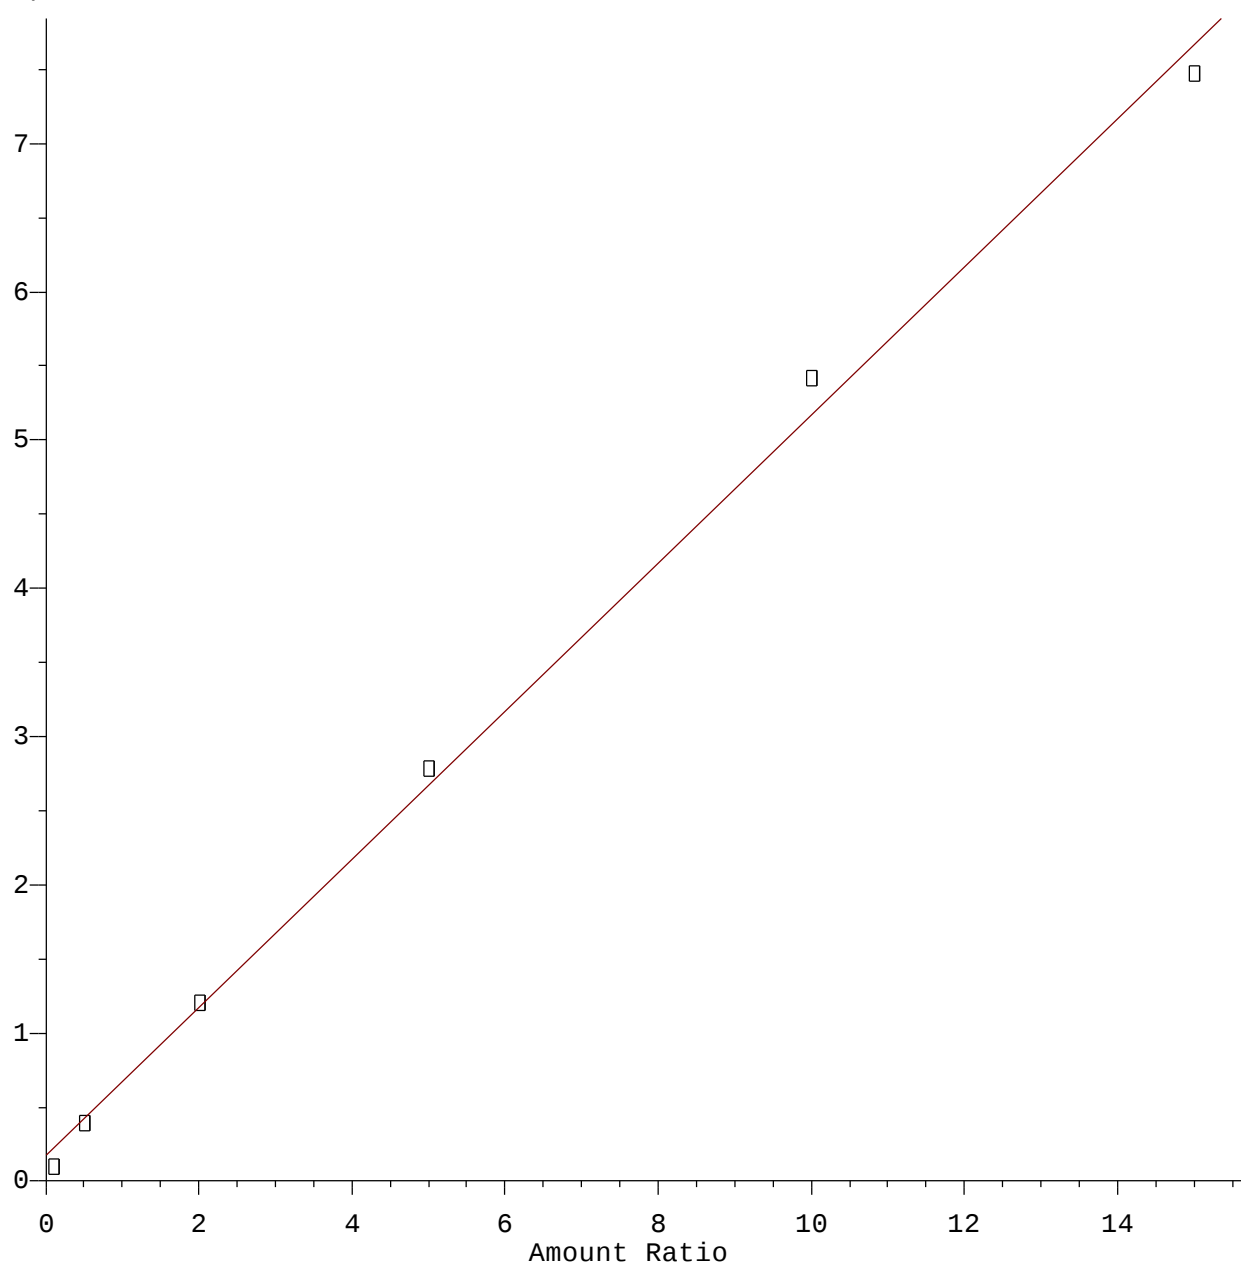


Resp Ratio = $4.99\text{e-}001 * \text{Amt} + 1.77\text{e-}001$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018

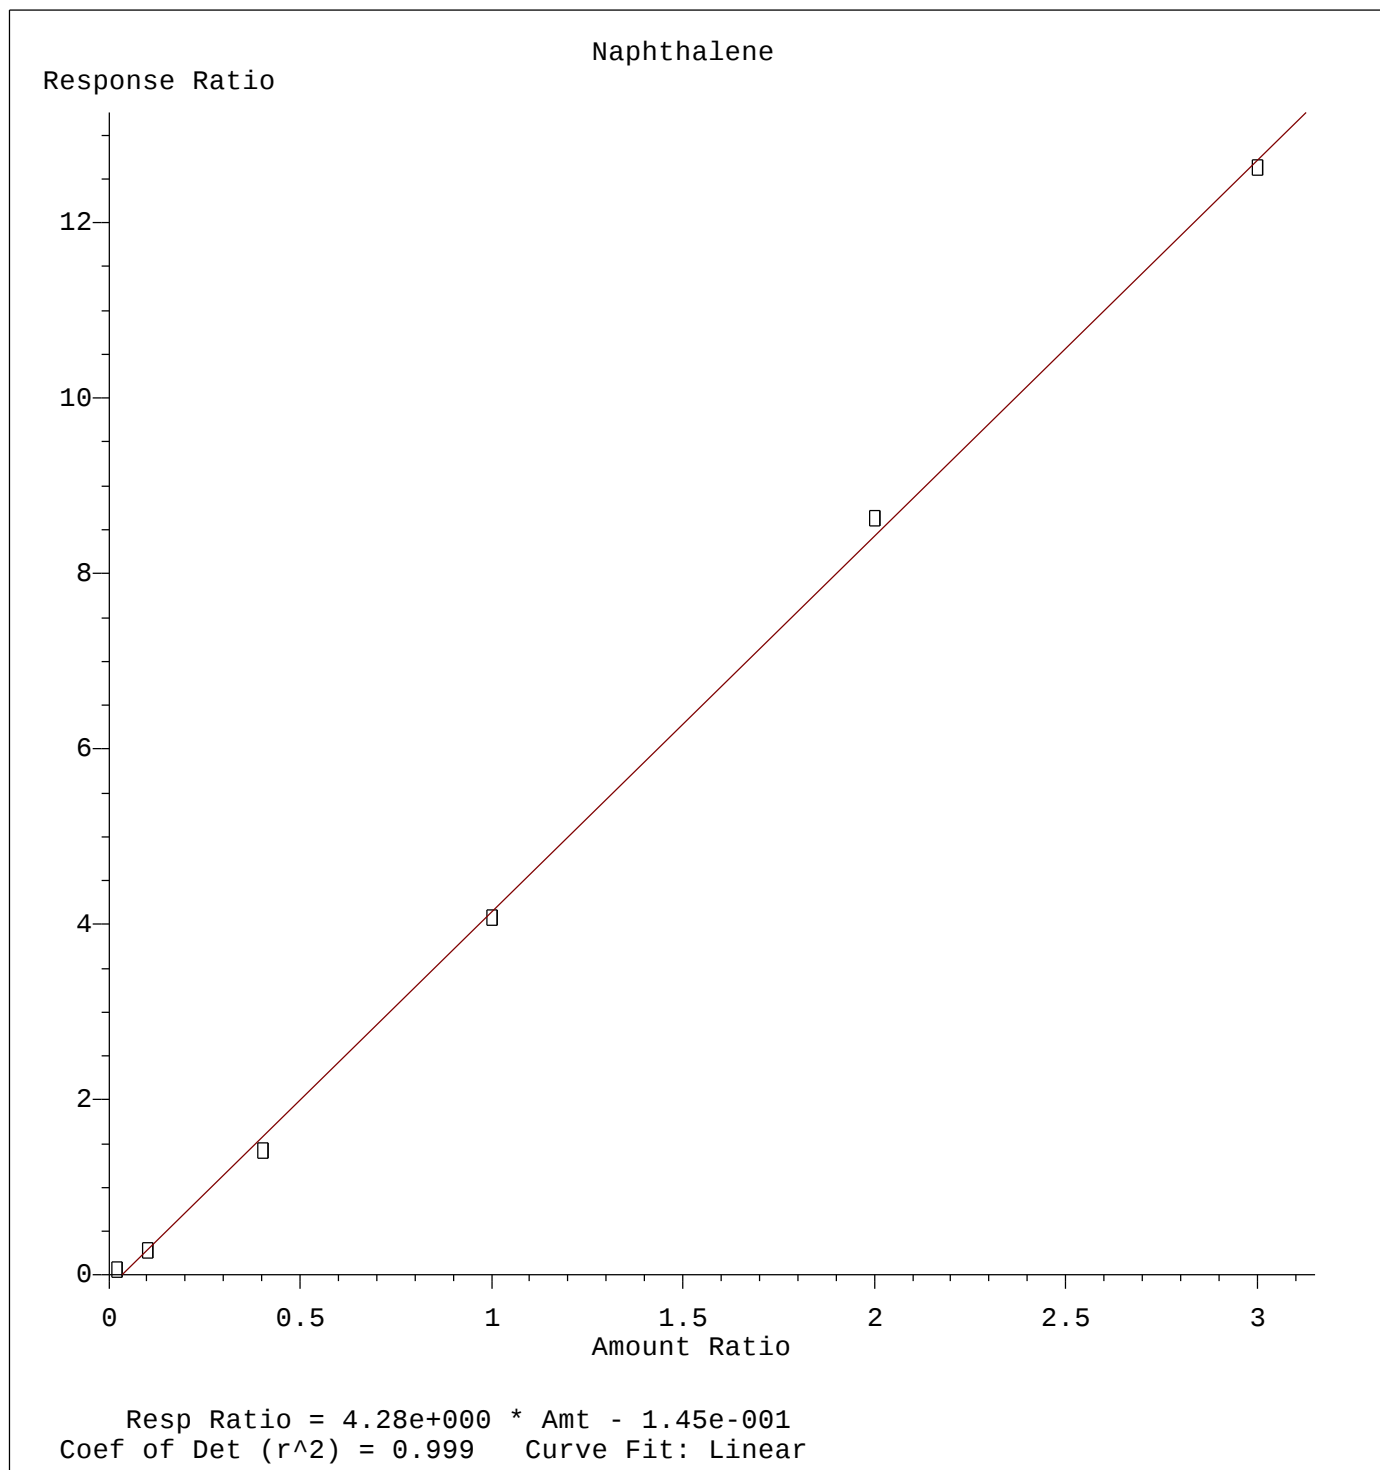


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018

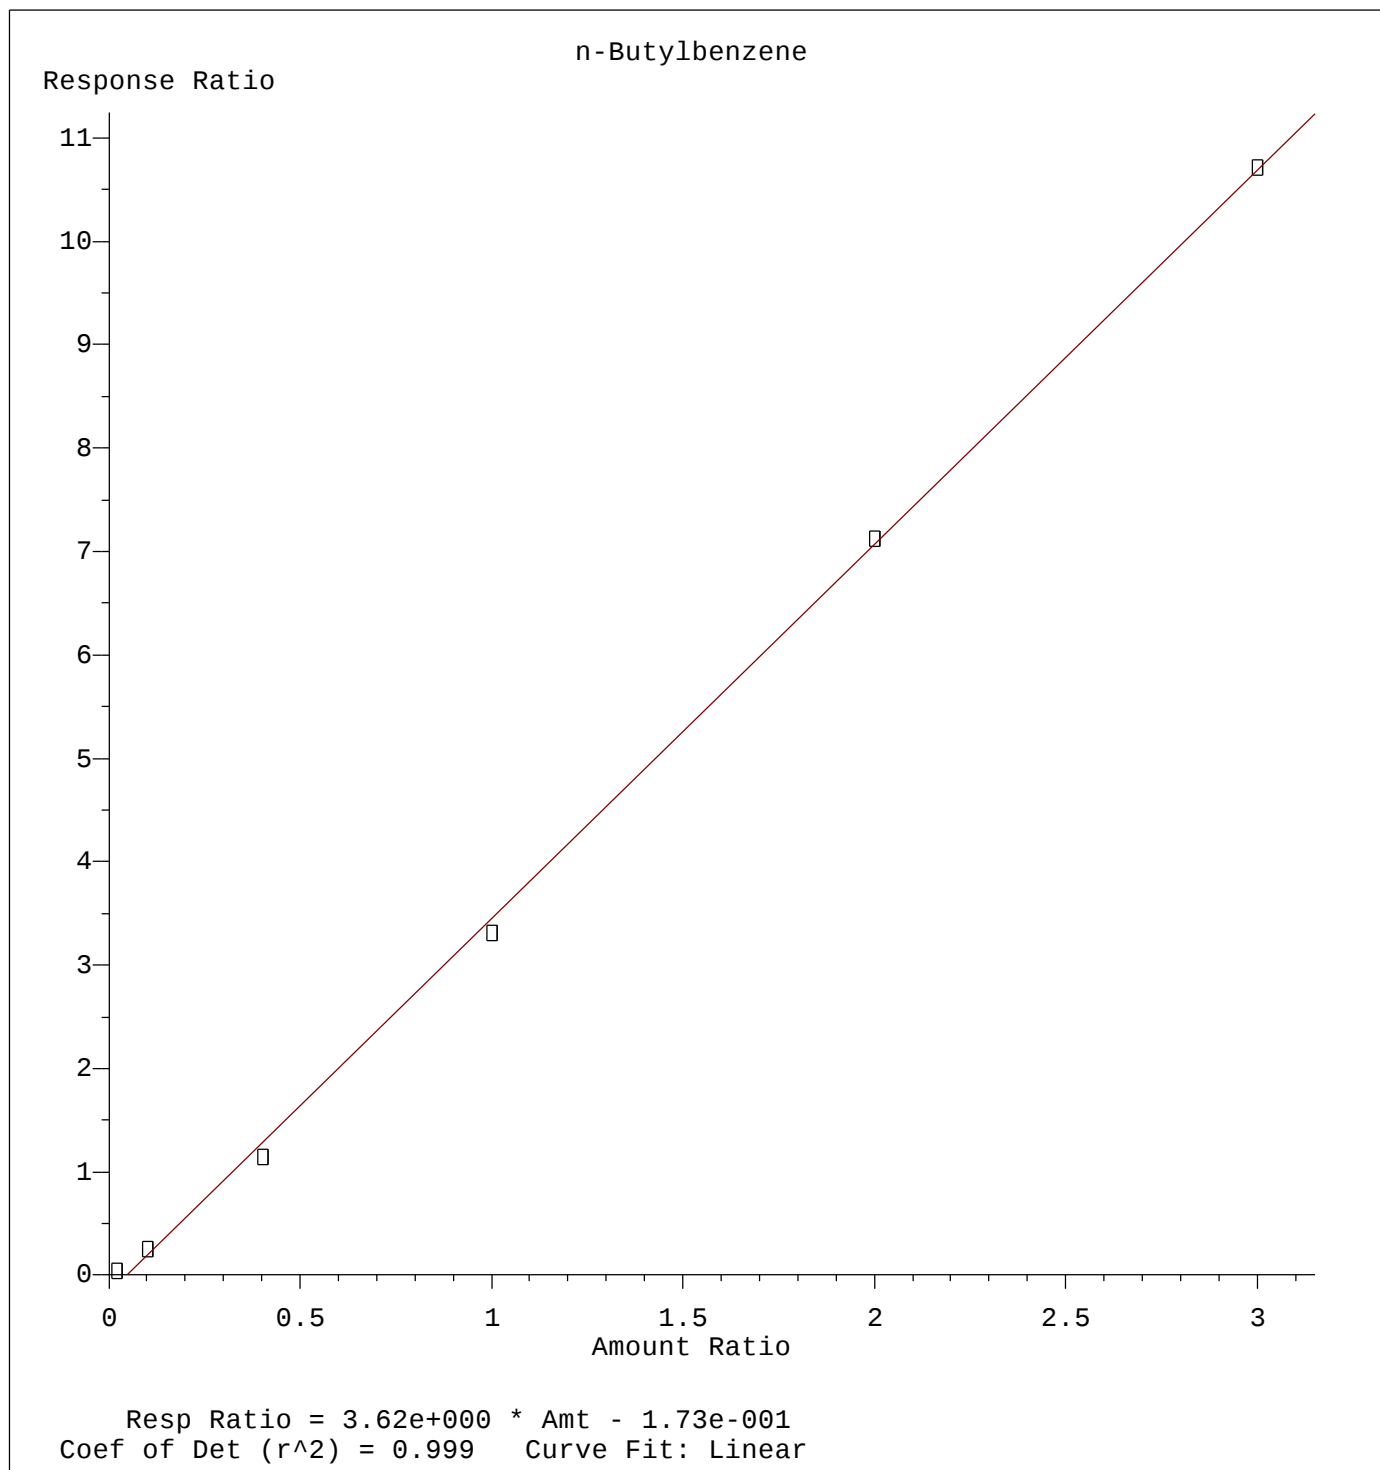

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018


p-Isopropyltoluene

Response Ratio

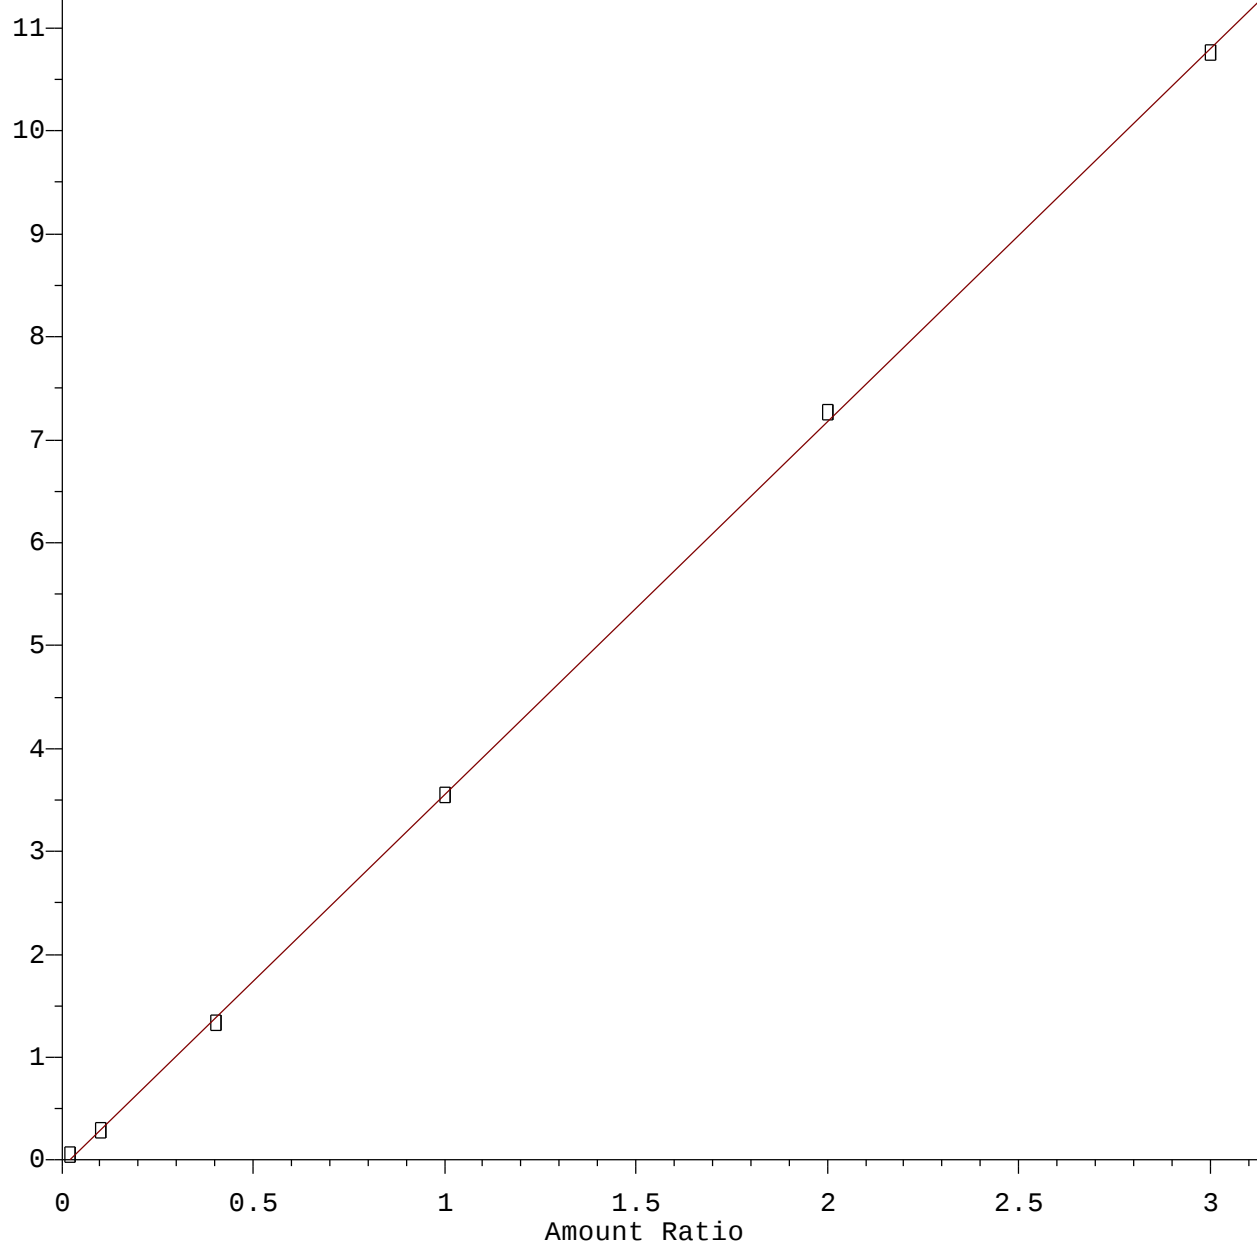

Resp Ratio = 3.62e+000 * Amt - 6.72e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018

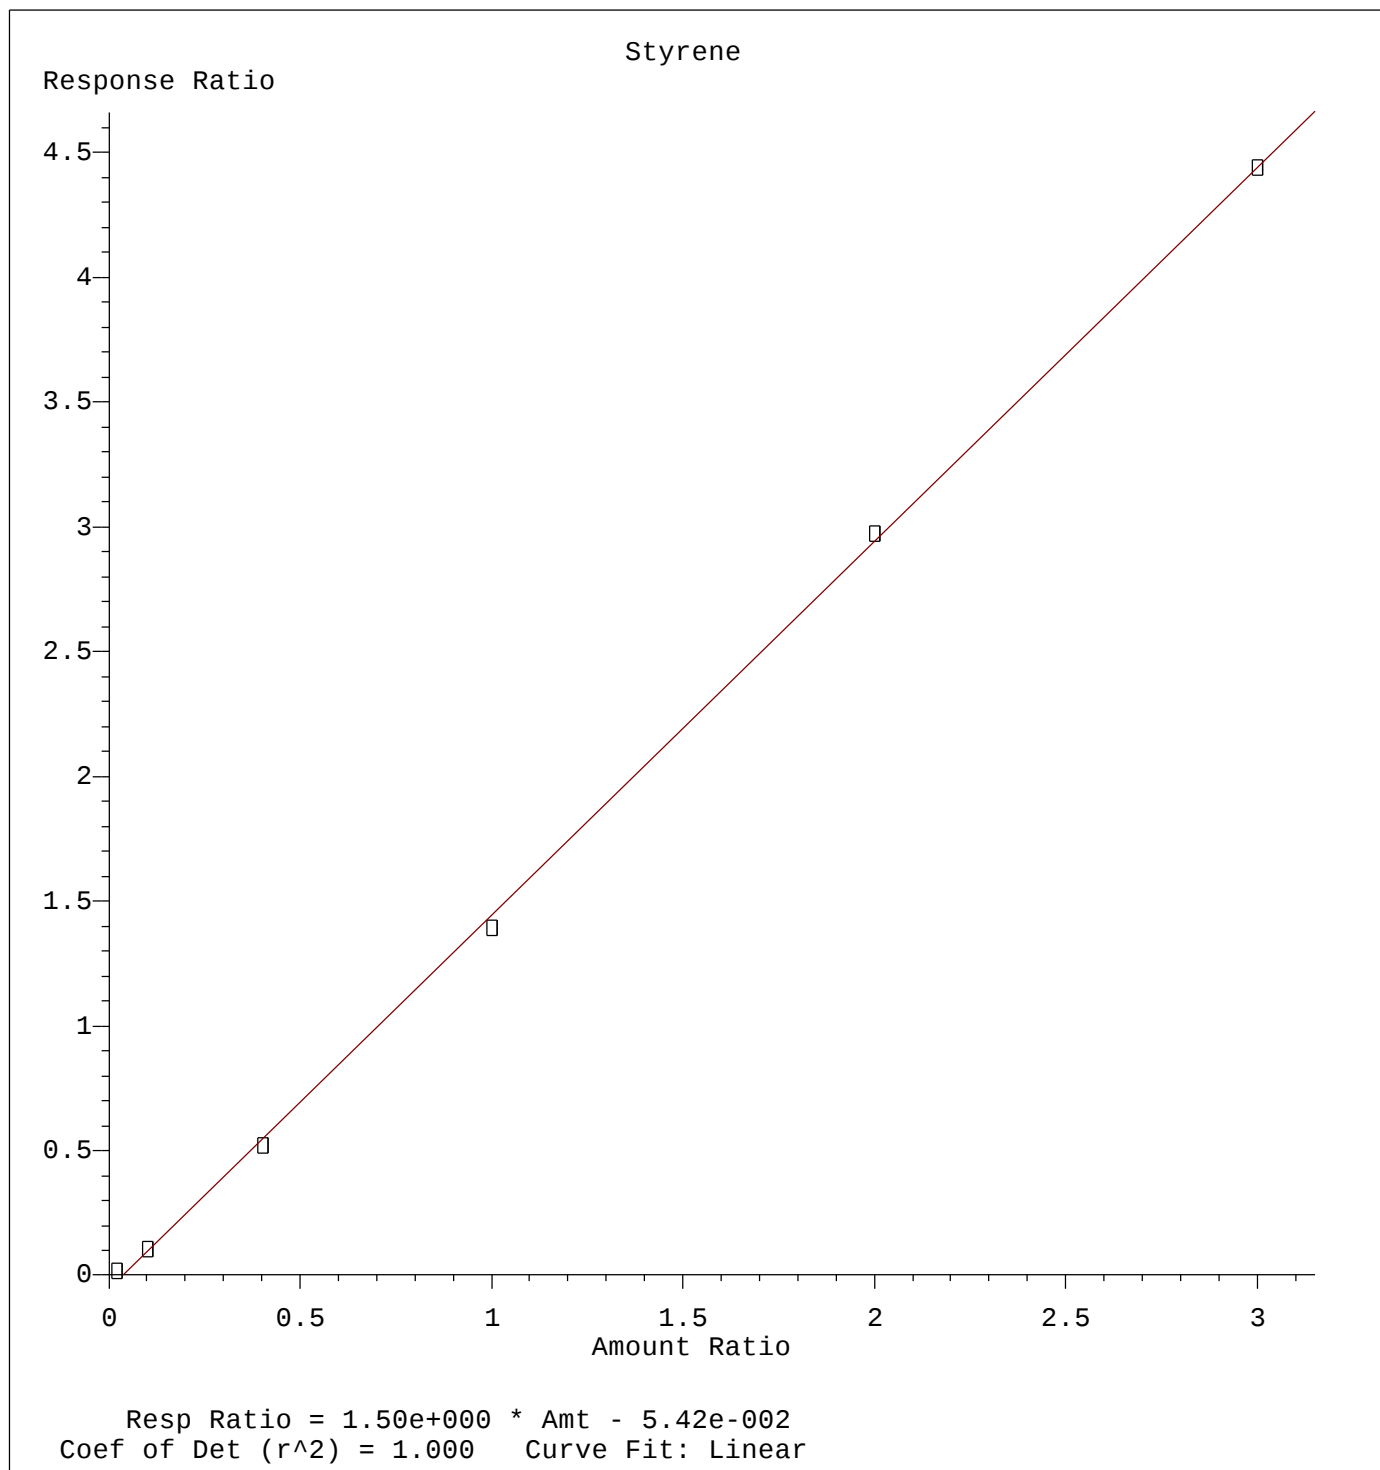

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018


2-Chloroethyl Vinyl ether

Response Ratio

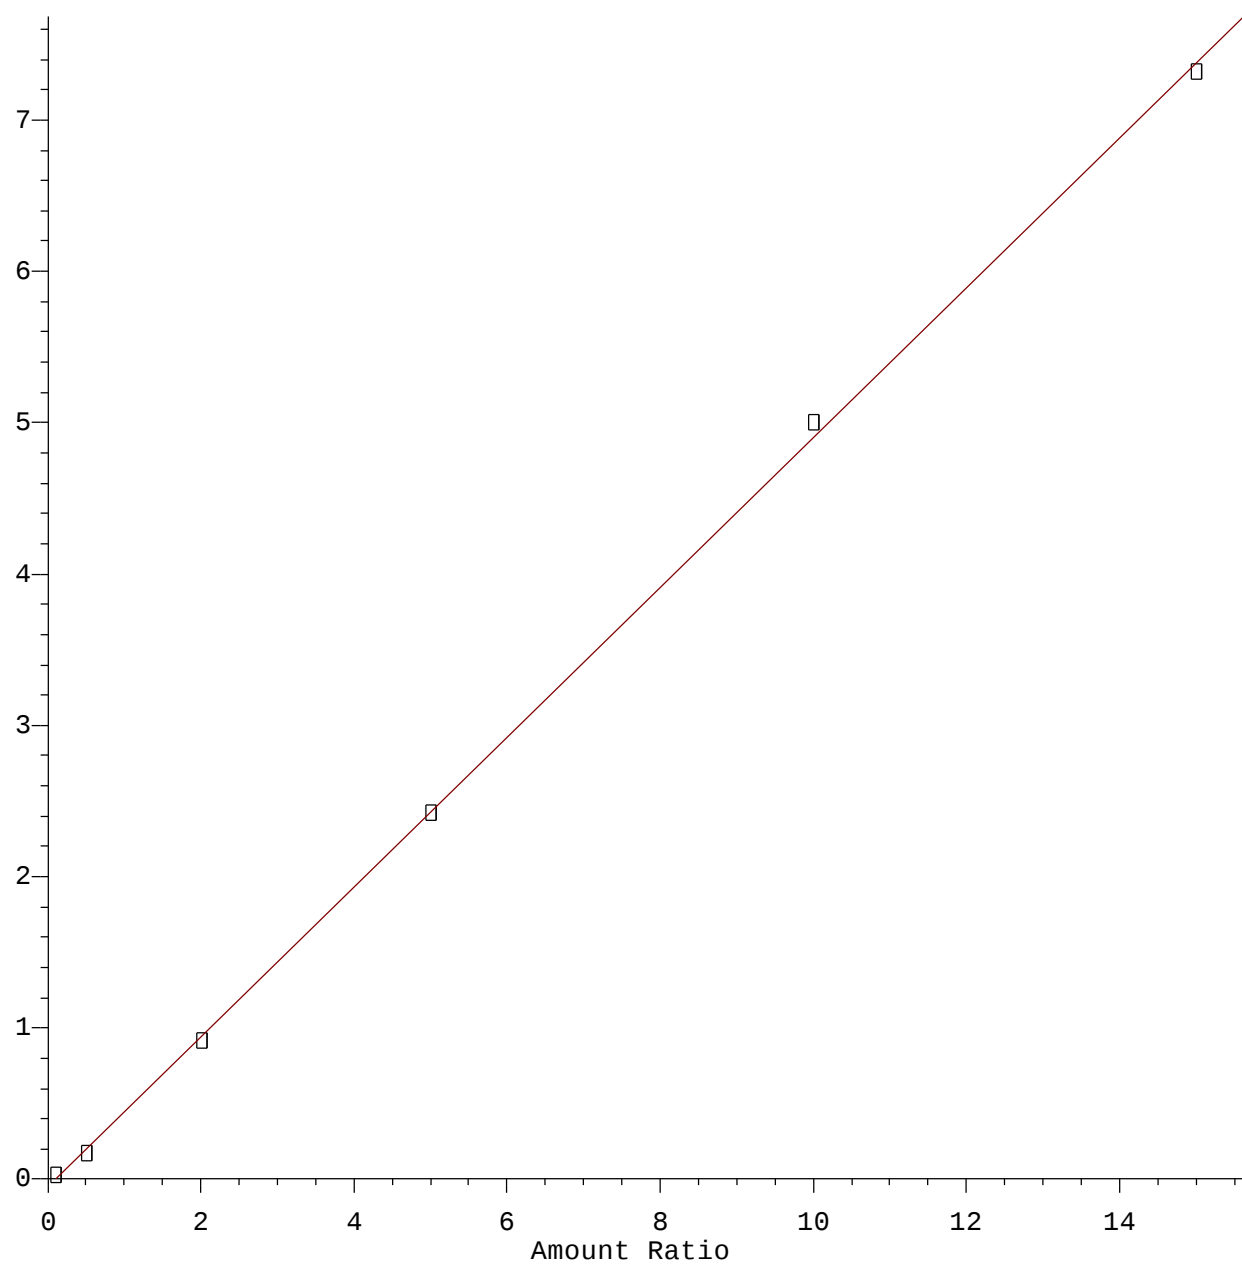


Resp Ratio = $4.95 \times 10^{-1} \times \text{Amt} - 4.81 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018

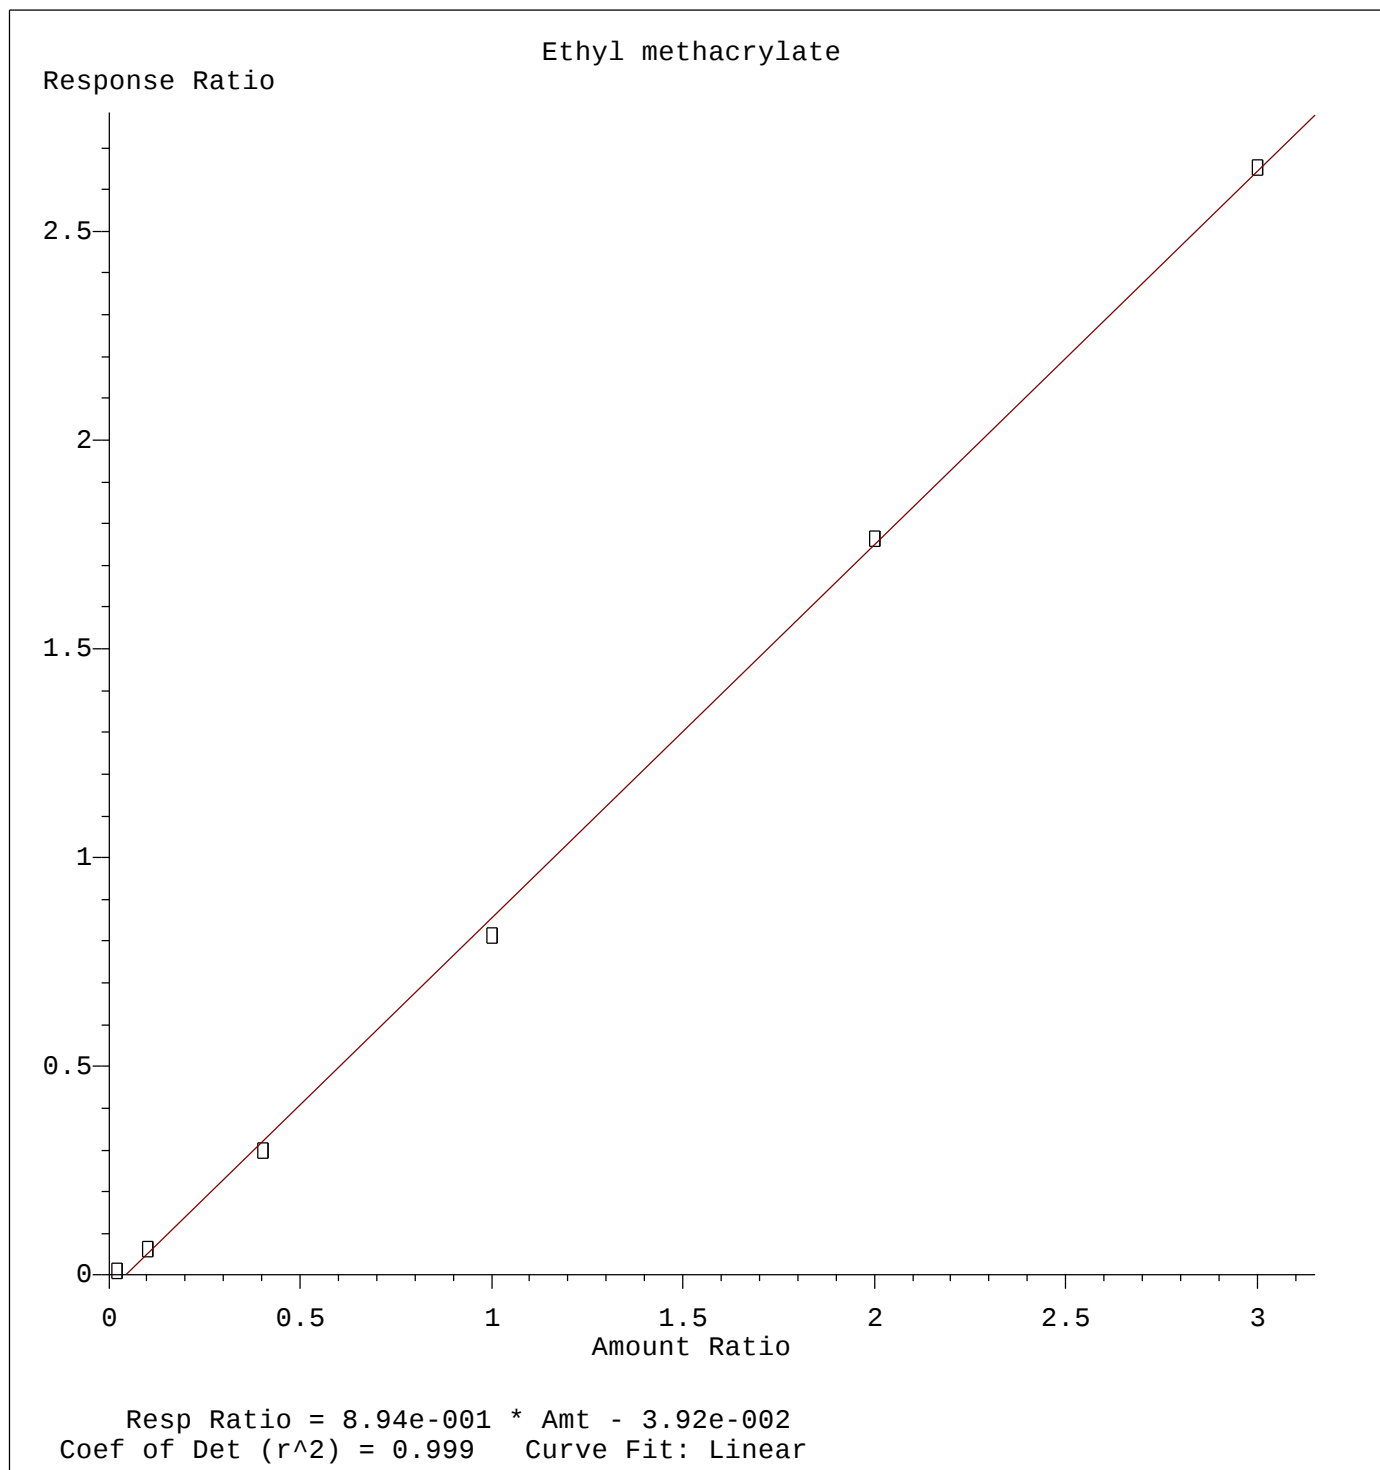


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018

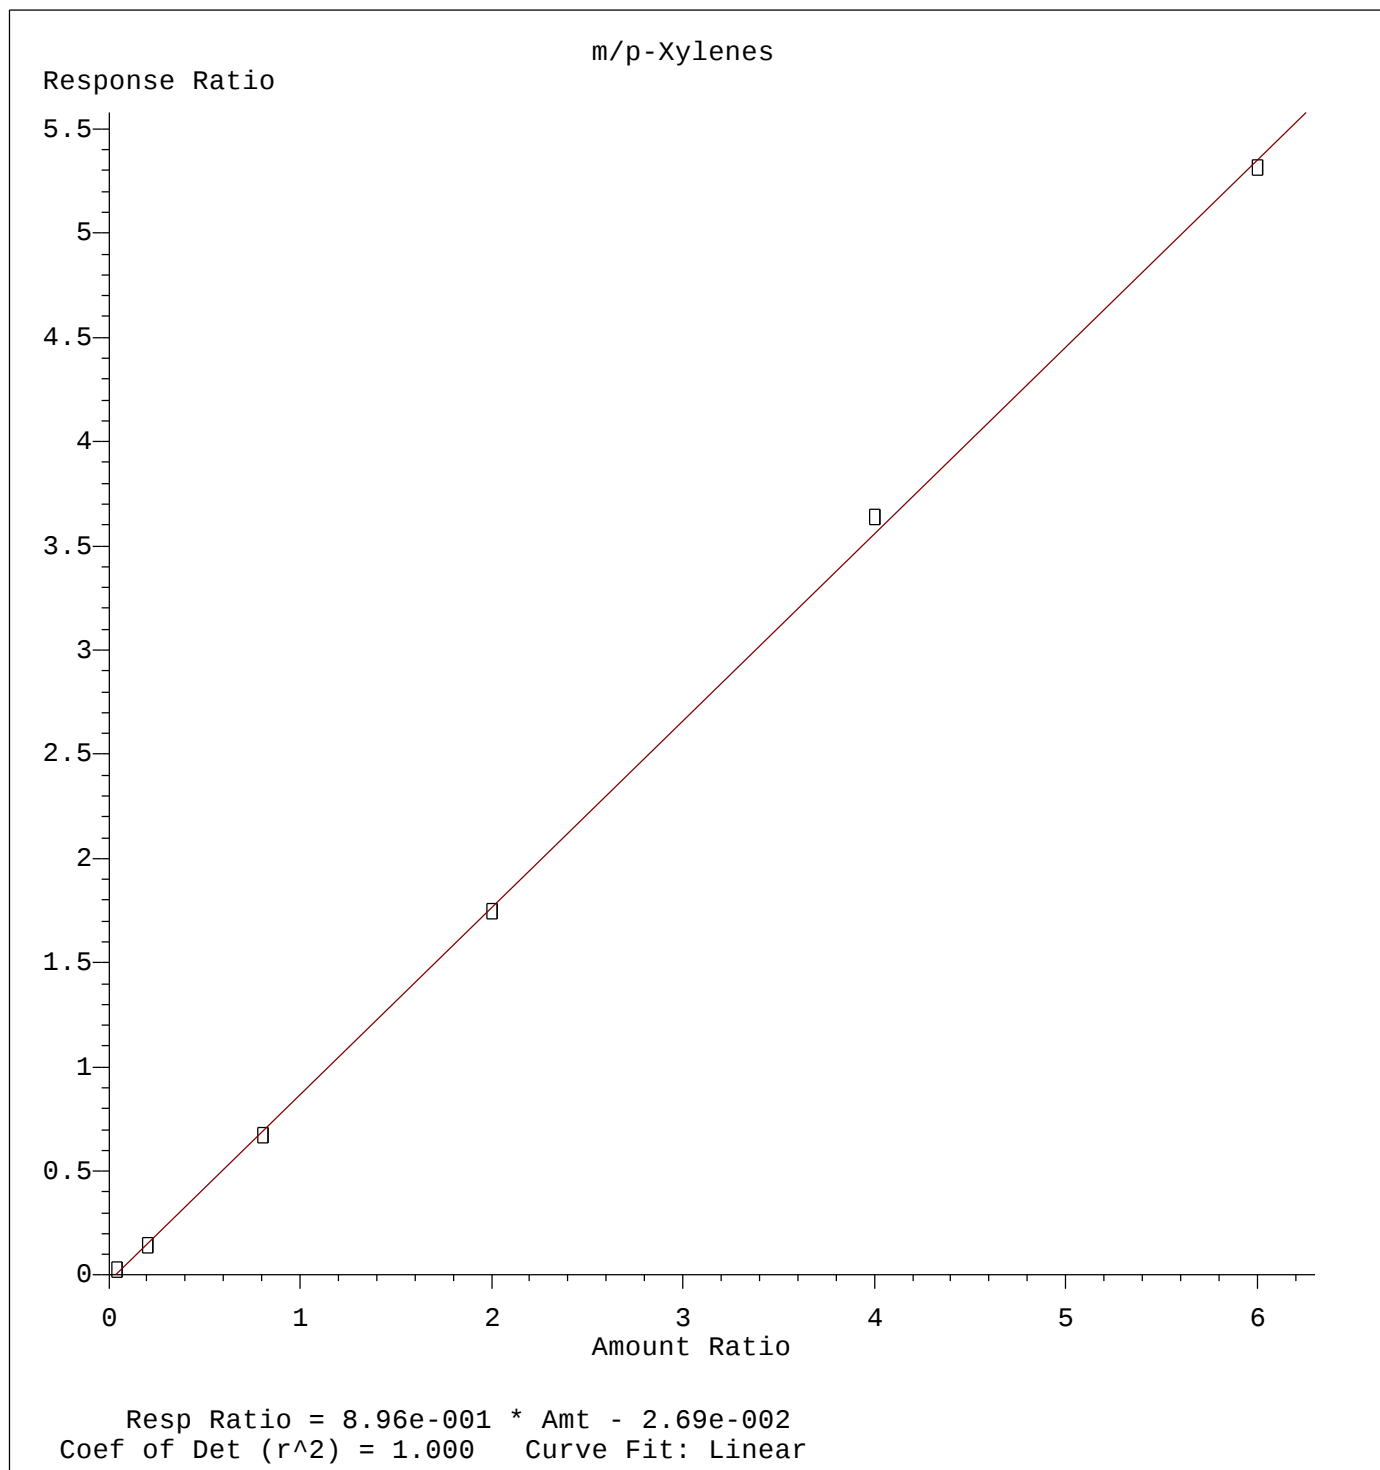


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018

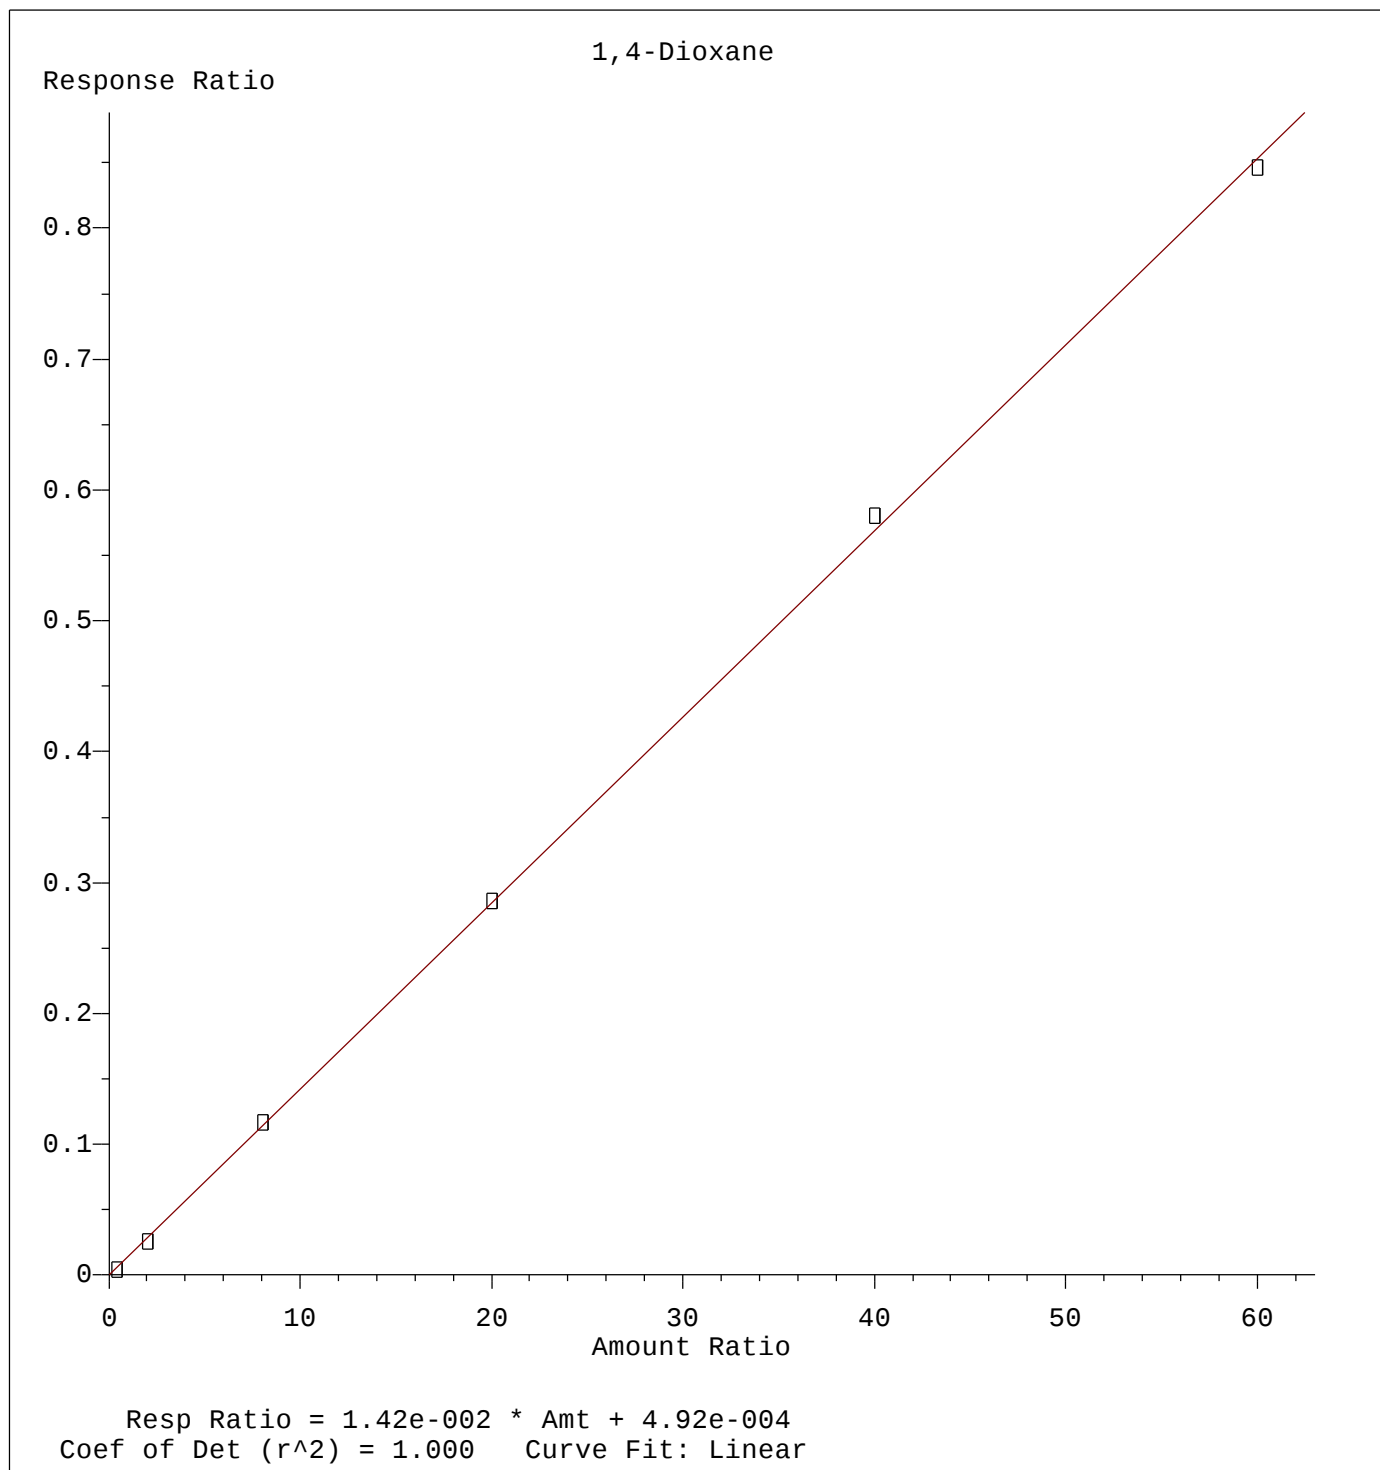

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018

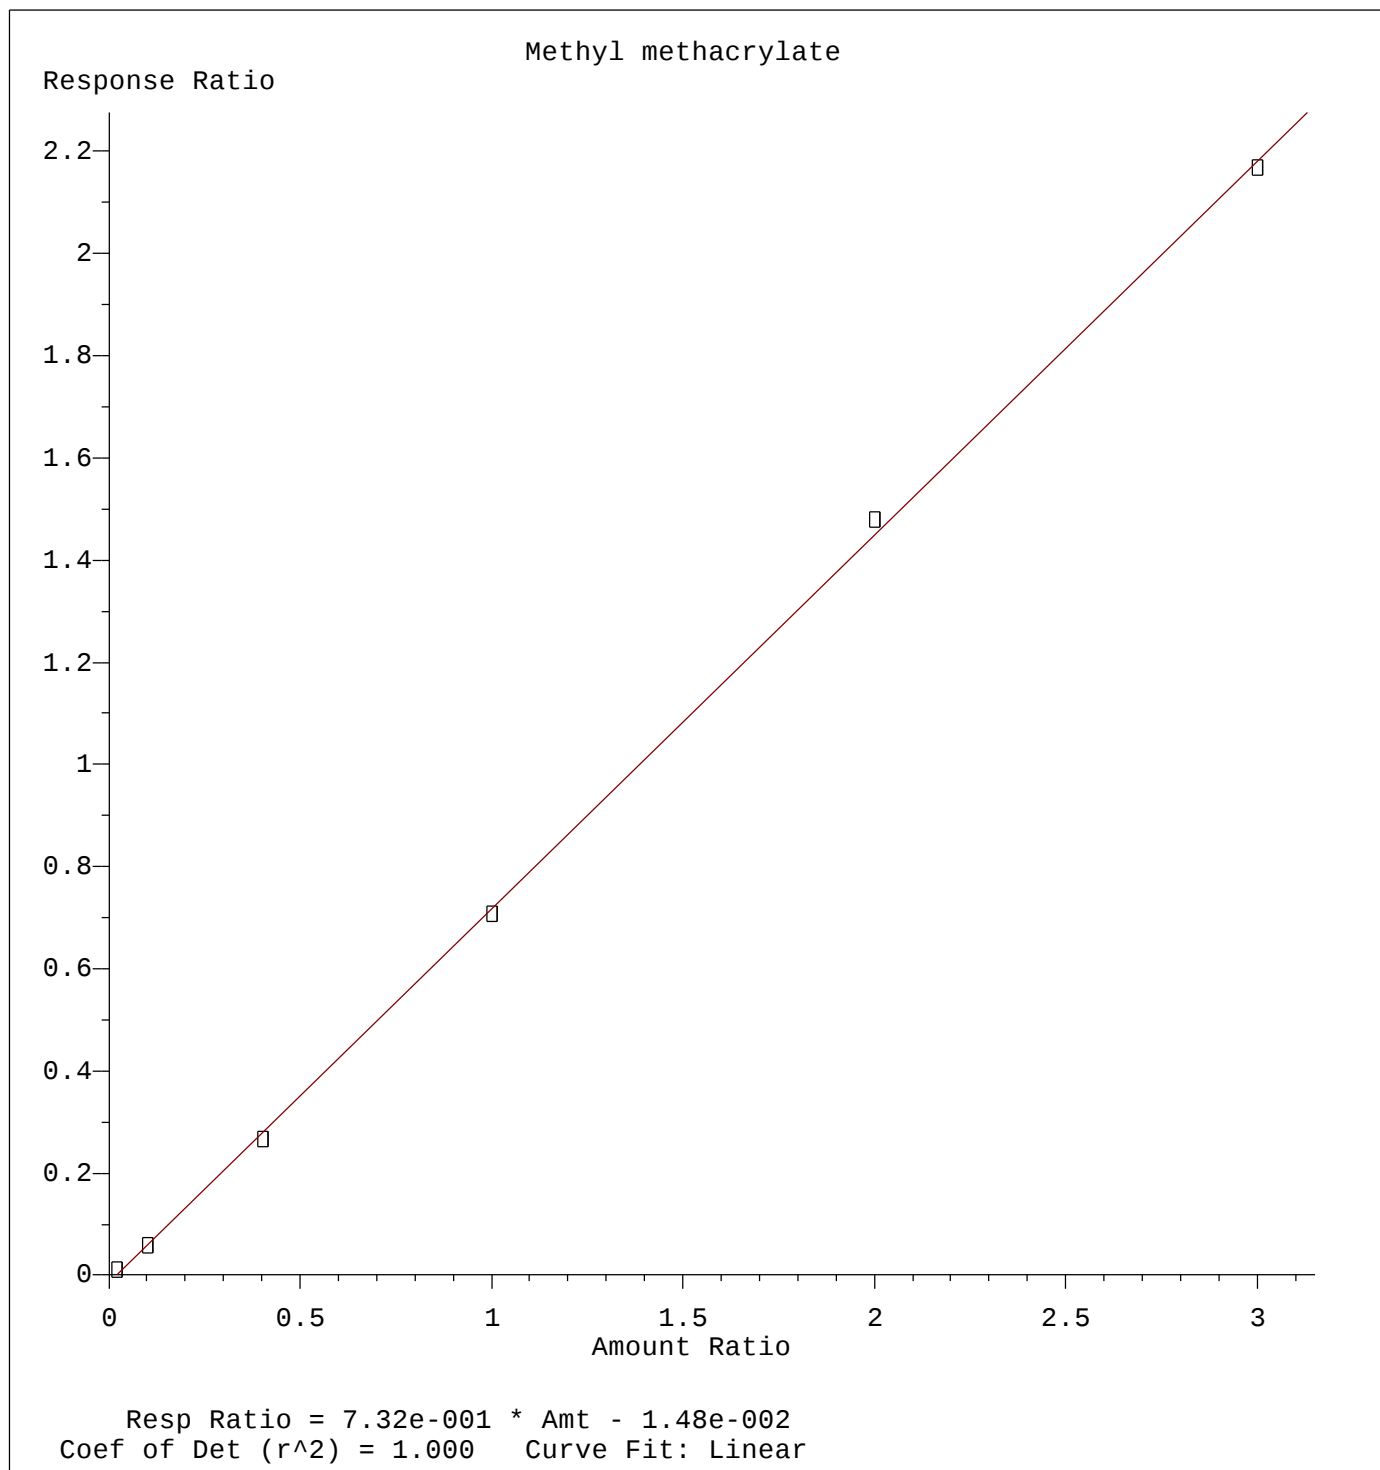

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018

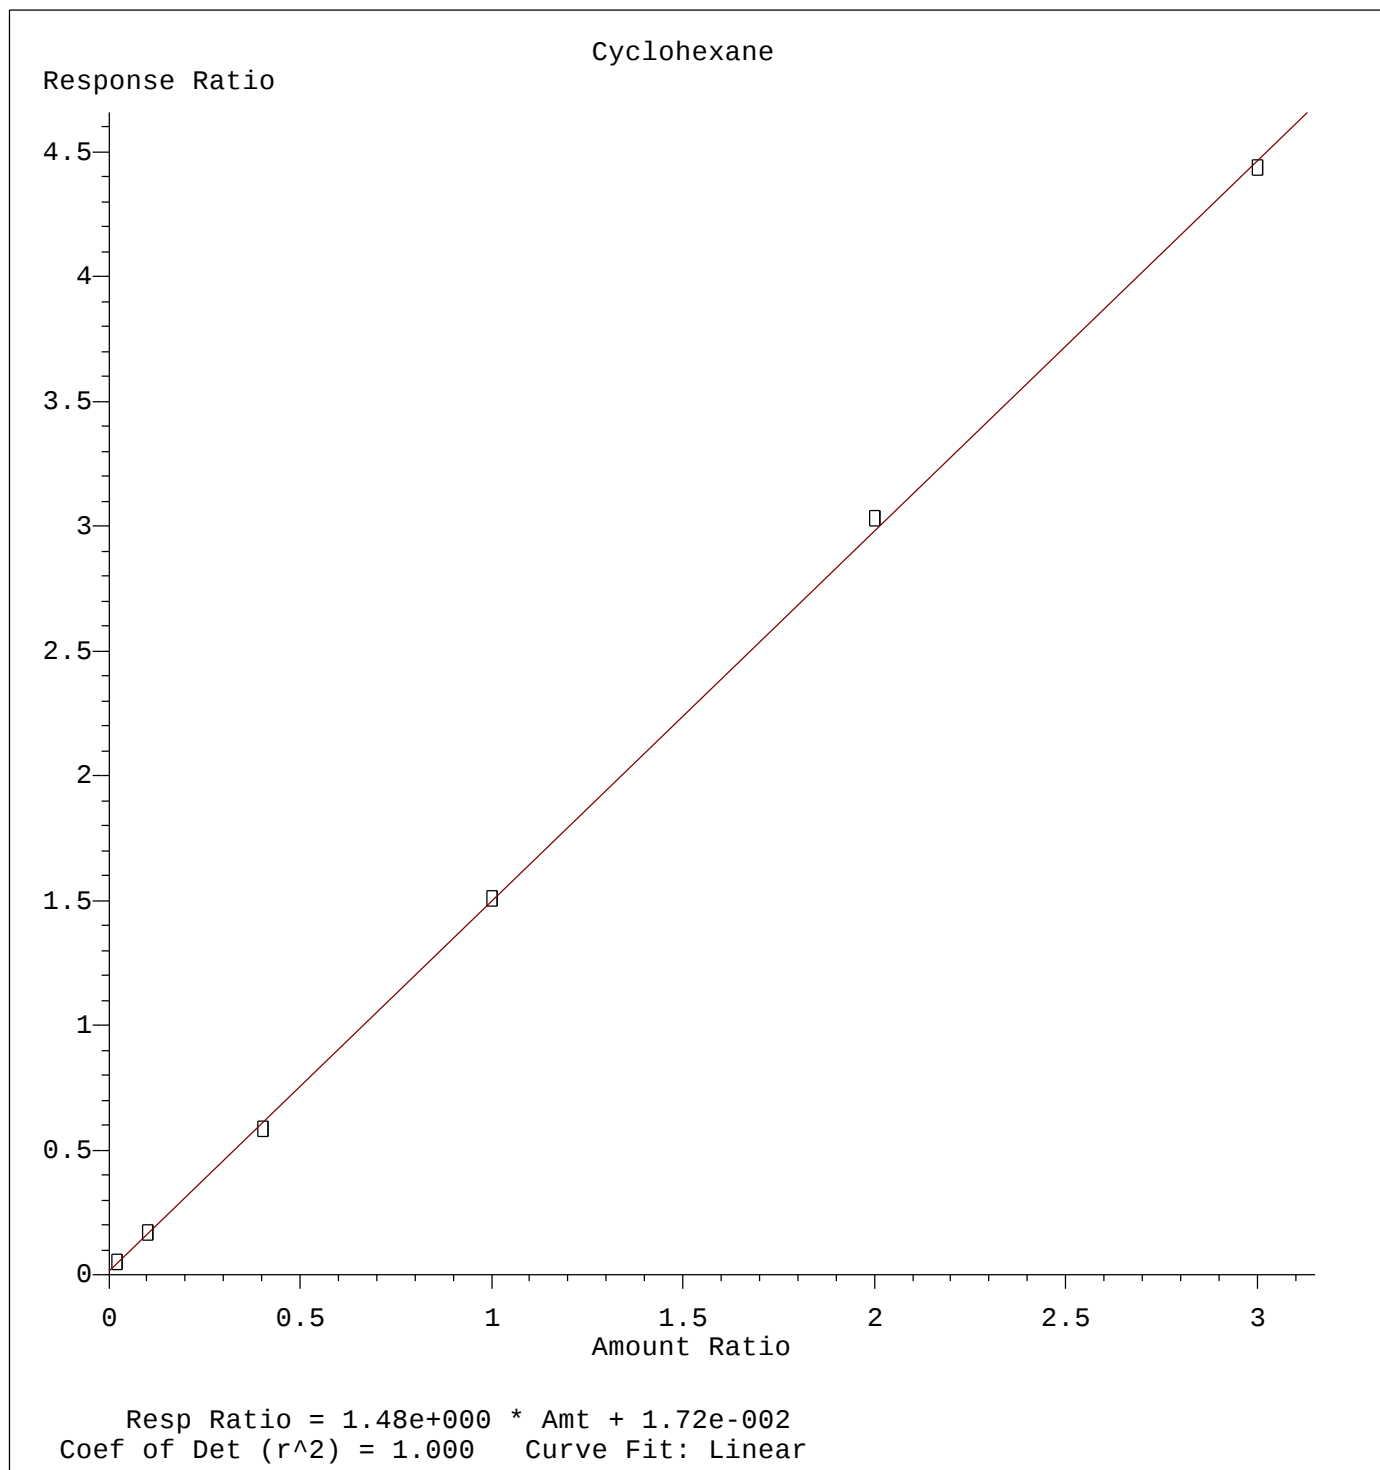

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Calibration Table Last Updated: Mon Sep 24 16:46:49 2018