


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092218\
Data File : VU026965.D
Acq On : 21 Sep 2018 12:59
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Title : SW846 8260
Last Update : Sat Sep 22 01:31:57 2018

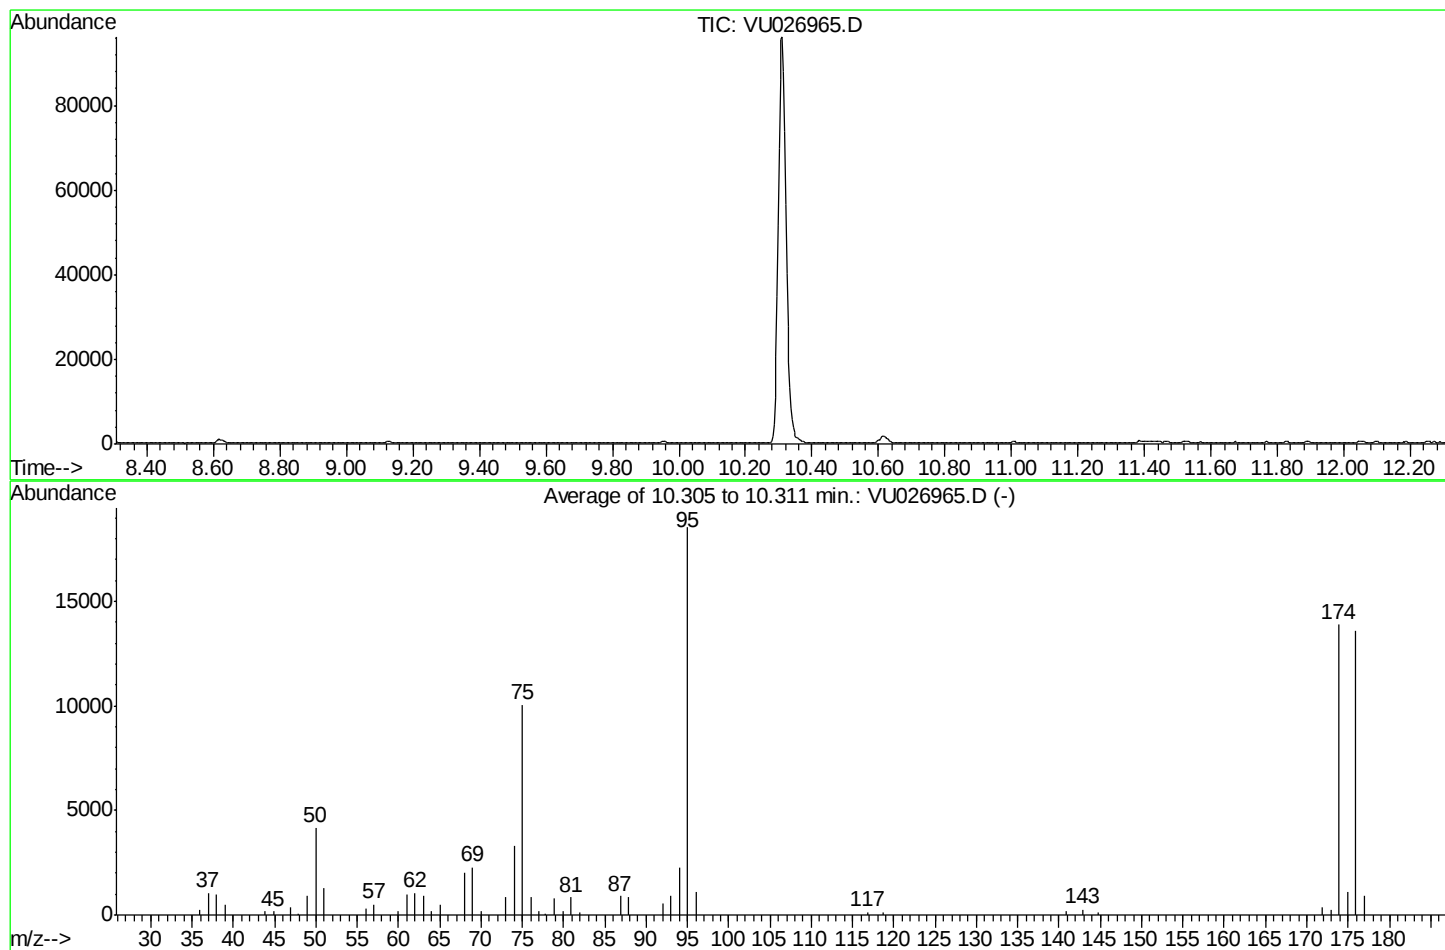

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	4174	PASS
75	95	30	60	54.2	10042	PASS
95	95	100	100	100.0	18541	PASS
96	95	5	9	6.0	1120	PASS
173	174	0.00	2	1.6	225	PASS
174	95	50	100	74.9	13884	PASS
175	174	5	9	7.9	1098	PASS
176	174	95	101	98.0	13612	PASS
177	176	5	9	6.8	932	PASS