


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092218\
Data File : VU026992.D
Acq On : 22 Sep 2018 02:46
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Title : SW846 8260
Last Update : Sat Sep 22 01:31:57 2018

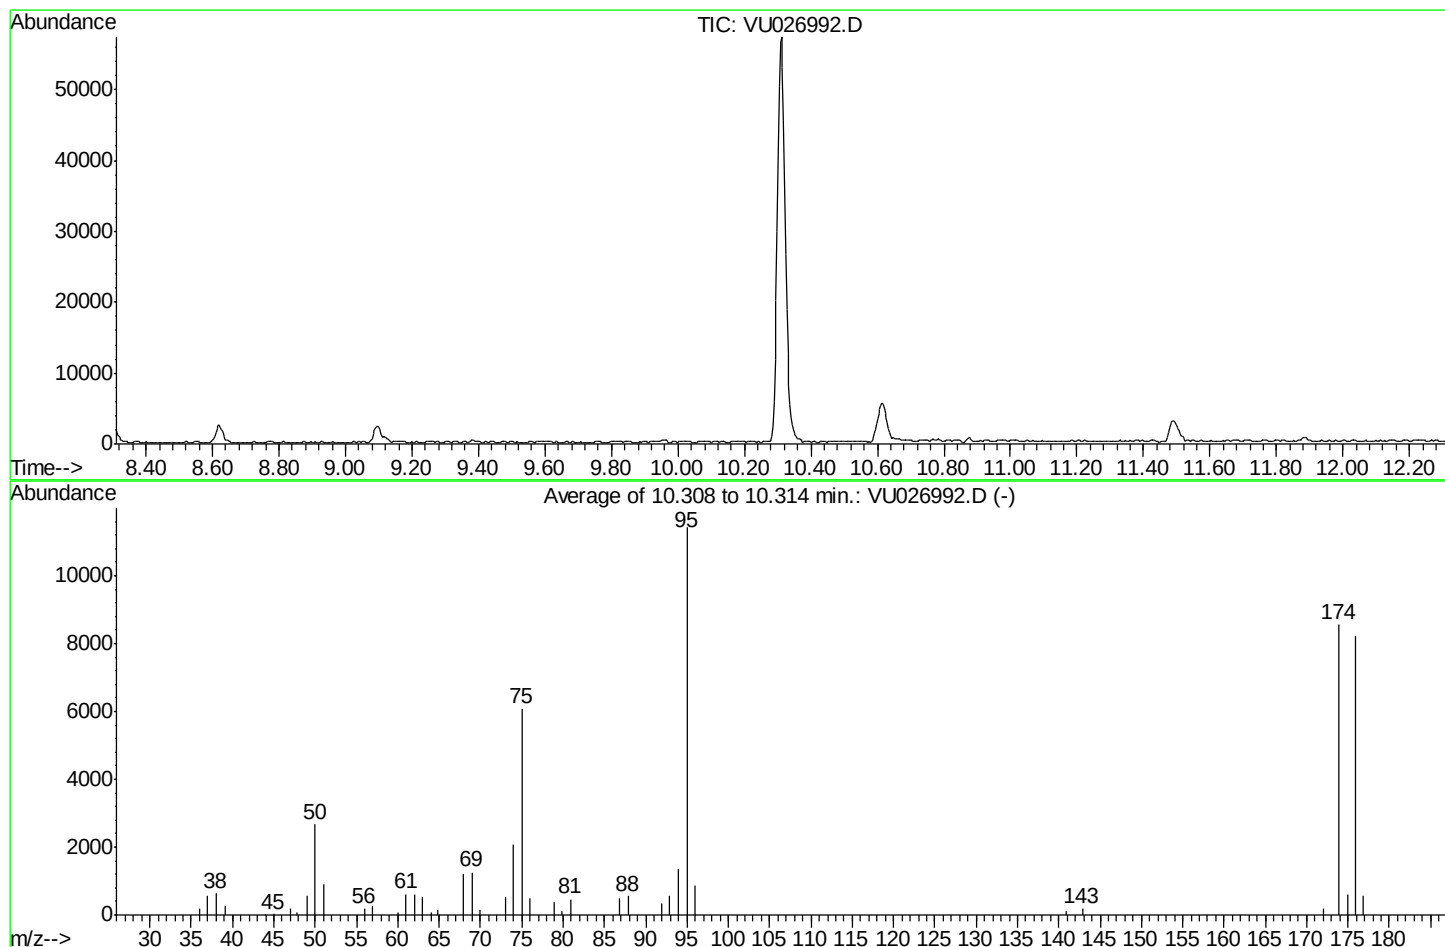

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	2668	PASS
75	95	30	60	53.3	6094	PASS
95	95	100	100	100.0	11429	PASS
96	95	5	9	7.5	853	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.8	8551	PASS
175	174	5	9	7.2	616	PASS
176	174	95	101	96.0	8211	PASS
177	176	5	9	6.9	567	PASS