


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092220\
 Data File : VU040246.D
 Acq On : 22 Sep 2020 10:35
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U091120DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Fri Sep 11 13:27:06 2020

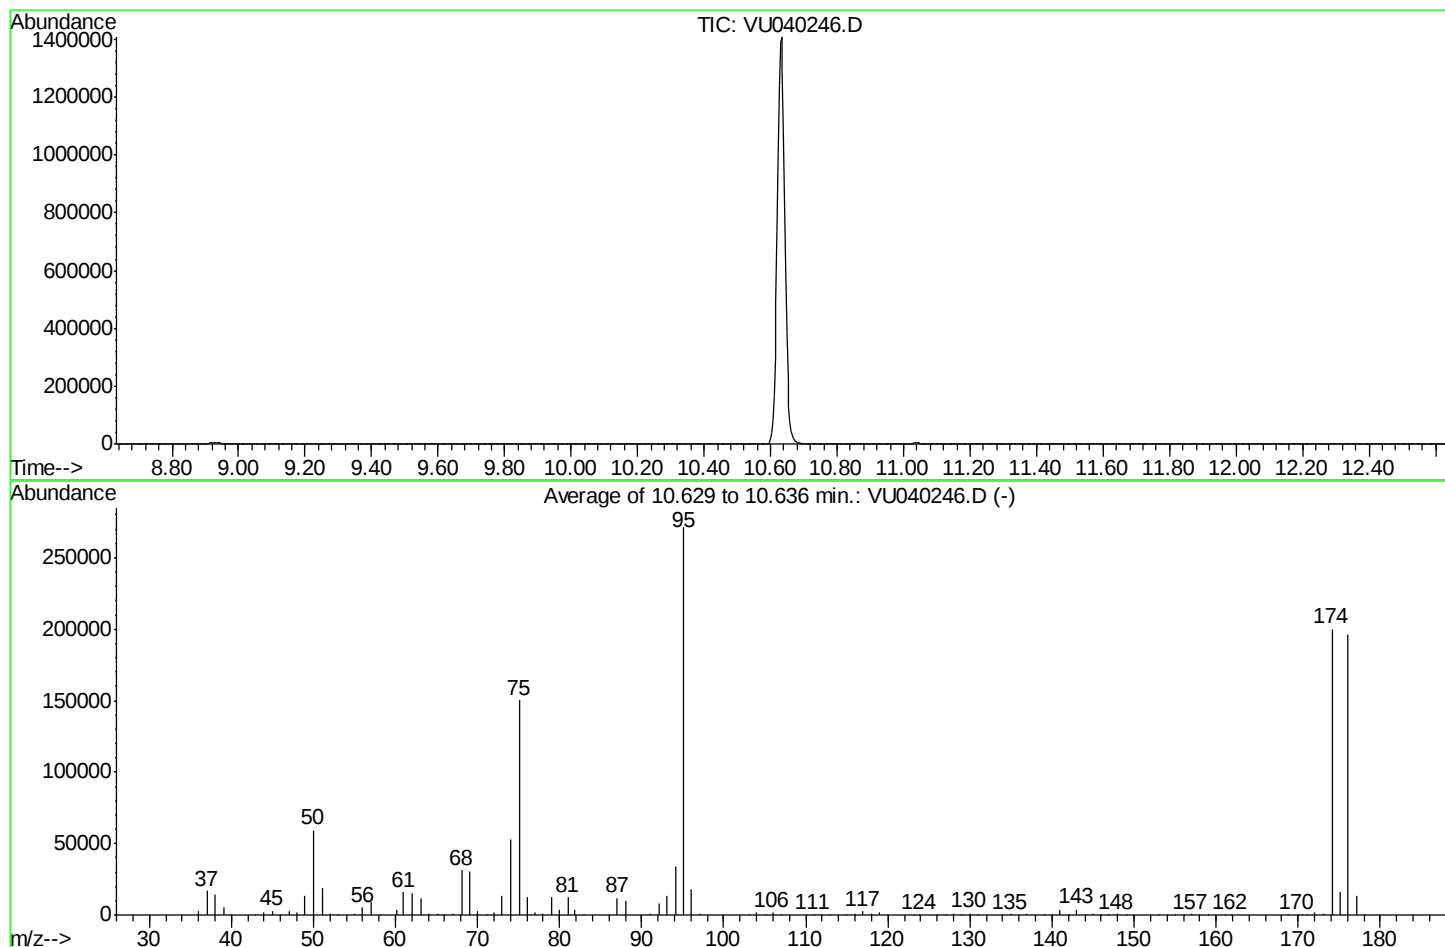

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	59344	PASS
75	95	30	60	55.4	150208	PASS
95	95	100	100	100.0	271338	PASS
96	95	5	9	6.5	17586	PASS
173	174	0.00	2	0.5	1003	PASS
174	95	50	100	73.8	200256	PASS
175	174	5	9	8.1	16290	PASS
176	174	95	101	98.0	196330	PASS
177	176	5	9	6.8	13318	PASS