

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
 Data File : VU044753.D
 Acq On : 22 Sep 2021 12:49
 Operator : SY/MD
 Sample : M3814-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6Y1

Manual Integrations
 APPROVED

MMDadoda
 9/24/2021 1:35:29 PM

Quant Time: Sep 23 03:02:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 23 02:59:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	133195	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	133173	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	65557	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	32202	4.097	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.000%
7) Chloroethane-d5	1.916	69	31566	3.936	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.800%
11) 1,1-Dichloroethene-d2	2.572	65	14594	3.677	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.600%
20) 2-Butanone-d5	4.642	46	137571m	41.758	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.520%
24) Chloroform-d	5.070	84	70868	4.287	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.800%
26) 1,2-Dichloroethane-d4	5.710	65	41755	4.236	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.800%
32) Benzene-d6	5.732	84	135623	3.994	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.800%
36) 1,2-Dichloropropane-d6	6.697	67	46124	4.136	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.800%
41) Toluene-d8	7.903	98	107941	3.651	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.000%
43) trans-1,3-Dichloroprop...	8.186	79	16026	4.077	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.600%
46) 2-Hexanone-d5	8.645	63	103237	40.862	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.720%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	41749	4.222	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.400%
66) 1,2-Dichlorobenzene-d4	12.198	152	45000	4.160	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.200%
Target Compounds						
					Qvalue	
3) Chloromethane	1.520	50	50748	3.974	ug/L	98
6) Bromomethane	1.861	94	22465	3.366	ug/L	97
9) Trichlorofluoromethane	2.141	101	120679	8.228	ug/L	99
12) 1,1-Dichloroethene	2.584	96	33337	3.896	ug/L	95
13) Acetone	2.646	43	213000m	99.267	ug/L	
14) Carbon disulfide	2.797	76	153930	5.682	ug/L	98
16) Methylene chloride	3.054	84	37994	2.792	ug/L	99
17) Methyl tert-butyl Ether	3.372	73	204500	8.646	ug/L	99
19) 1,1-Dichloroethane	3.877	63	180044	9.790	ug/L	100
21) 2-Butanone	4.719	43	447247	124.834	ug/L	84
27) 1,2-Dichloroethane	5.803	62	98839	7.703	ug/L	97
29) 1,1,1-Trichloroethane	5.324	97	133550	9.203	ug/L	99
30) Cyclohexane	5.395	56	196666	11.834	ug/L	99
34) Trichloroethene	6.549	95	53358	5.453	ug/L	95
35) Methylcyclohexane	6.768	83	106104	6.599	ug/L	99
37) 1,2-Dichloropropane	6.797	63	24692	2.331	ug/L	99
42) Toluene	7.977	91	367533	8.904	ug/L	98
47) Tetrachloroethene	8.559	164	62530	9.203	ug/L	99
48) 2-Hexanone	8.697	43	344719	56.180	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
 Data File : VU044753.D
 Acq On : 22 Sep 2021 12:49
 Operator : SY/MD
 Sample : M3814-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6Y1

Manual Integrations
 APPROVED

MMDadoda
 9/24/2021 1:35:29 PM

Quant Time: Sep 23 03:02:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 23 02:59:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

50) 1,2-Dibromoethane	8.928	107	114197	16.108	ug/L	99
51) Chlorobenzene	9.452	112	282101	11.023	ug/L	99
52) Ethylbenzene	9.575	91	302605	6.768	ug/L	100
53) m,p-Xylene	9.703	106	238230	14.012	ug/L	100
54) o-Xylene	10.105	106	92182	5.676	ug/L	99
55) Styrene	10.118	104	157850	5.552	ug/L	99
59) Bromoform	10.295	173	22322	5.478	ug/L	97
60) Isopropylbenzene	10.488	105	144627	3.524	ug/L	99
65) 1,4-Dichlorobenzene	11.841	146	82911	4.200	ug/L	98
67) 1,2-Dichlorobenzene	12.218	146	228967	12.607	ug/L	99
68) 1,2-Dibromo-3-chloropr...	13.002	75	5992	3.761	ug/L	94
72) 1,2,3-Trichlorobenzene	14.333	180	107422	9.511	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
 Data File : VU044753.D
 Acq On : 22 Sep 2021 12:49
 Operator : SY/MD
 Sample : M3814-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1


Instrument :
 MSVOA_U
 ClientSampleId :
 GB6Y1

Manual Integrations
 APPROVED


MMDadoda
 9/24/2021 1:35:29 PM

Quant Time: Sep 23 03:02:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 23 02:59:45 2021
 Response via : Initial Calibration

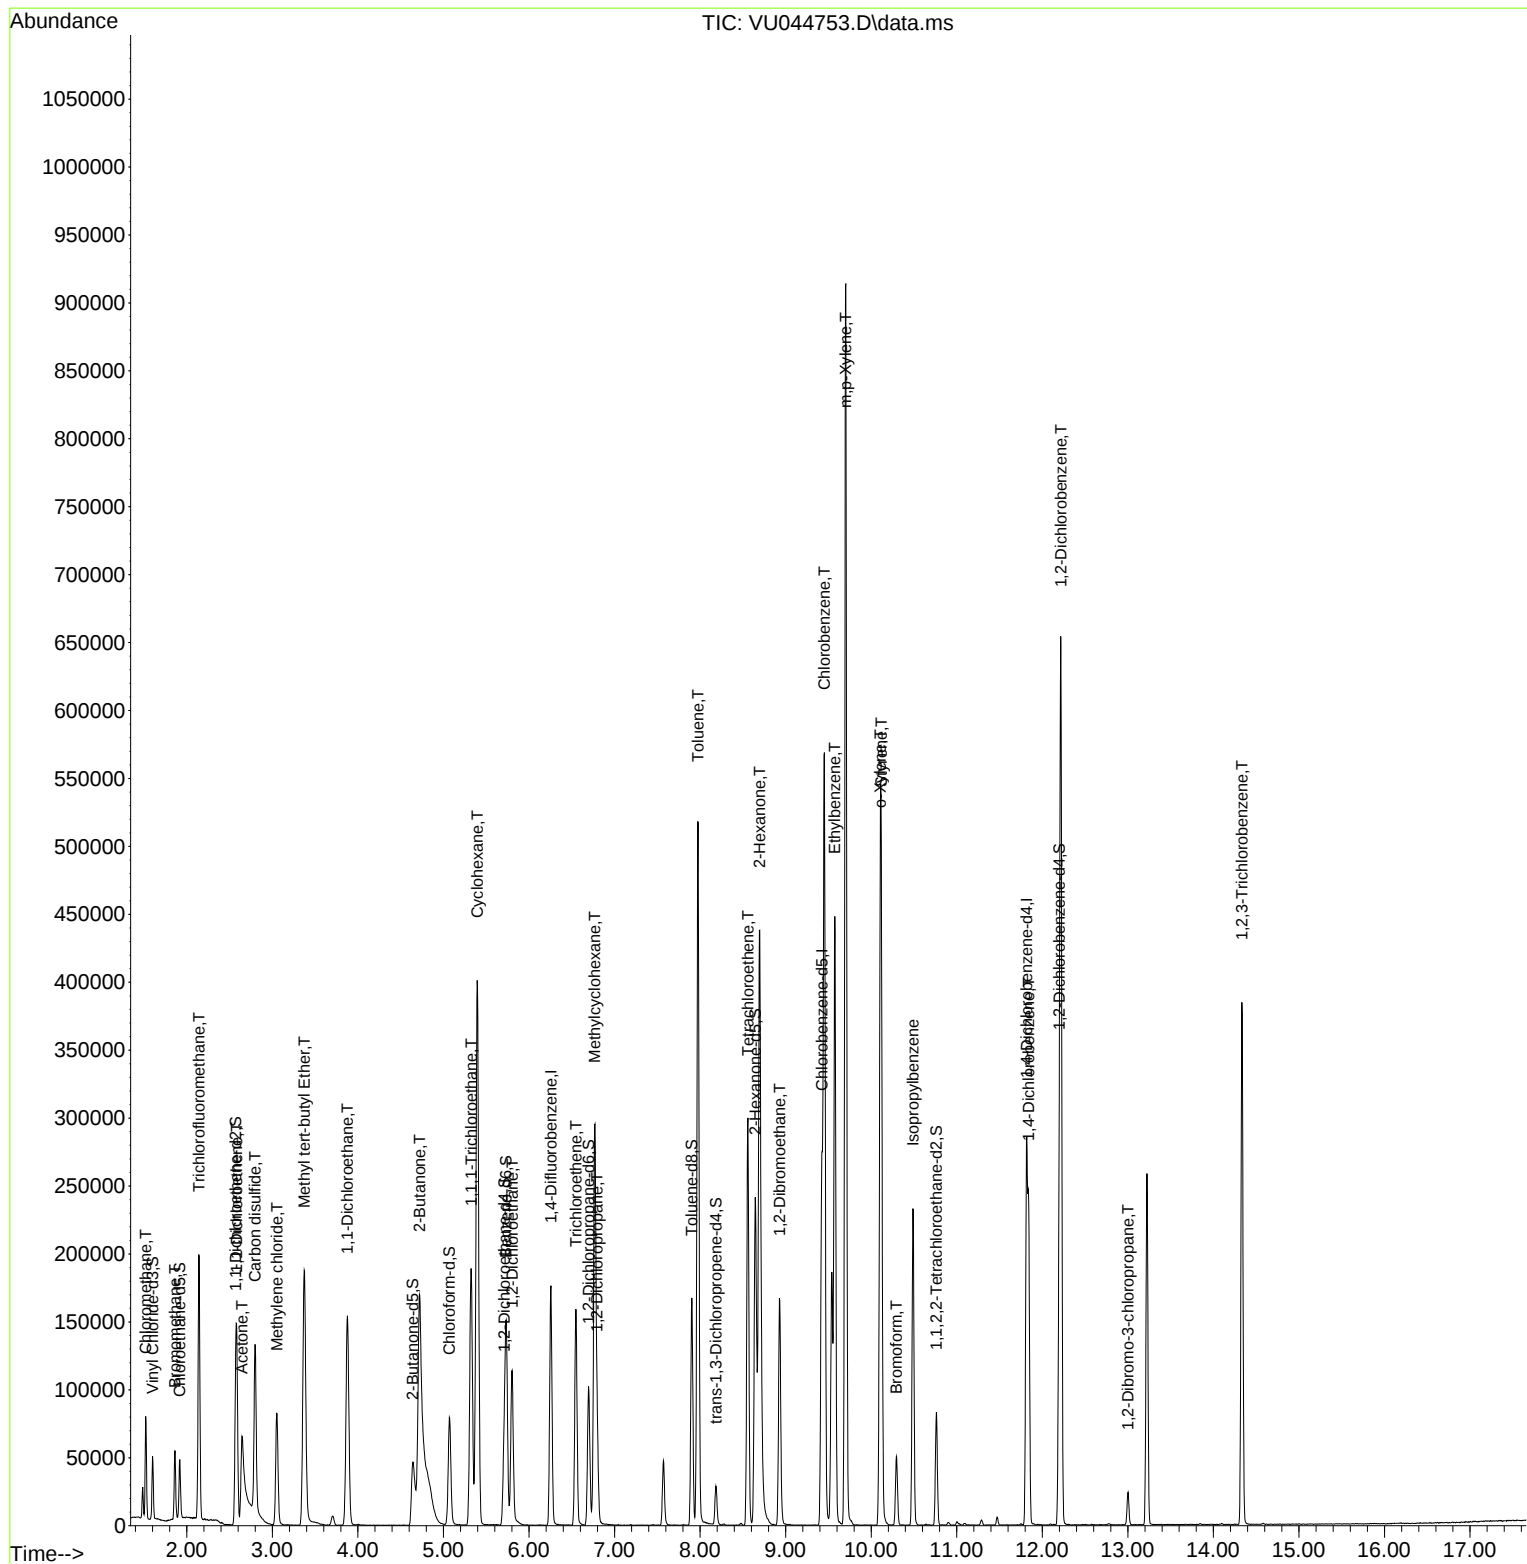


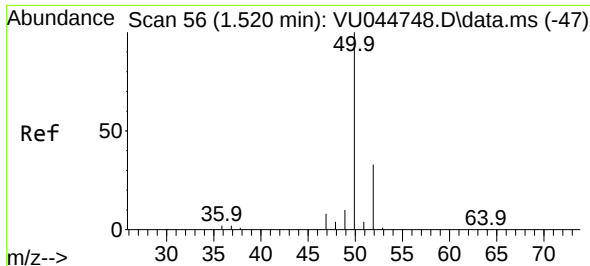

#3
Chloromethane
Concen: 3.974 ug/L
RT: 1.520 min Scan# 56
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

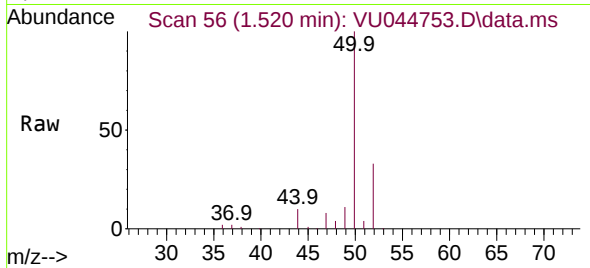


Tgt Ion: 50 Resp: 50748
Ion Ratio Lower Upper
50 100
52 33.5 22.6 42.0

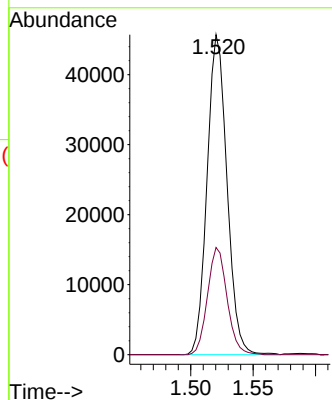


Instrument :
MSVOA_U
ClientSampleId :
GB6Y1

Manual Integrations
APPROVED



MMDadoda
9/24/2021 1:35:29 PM

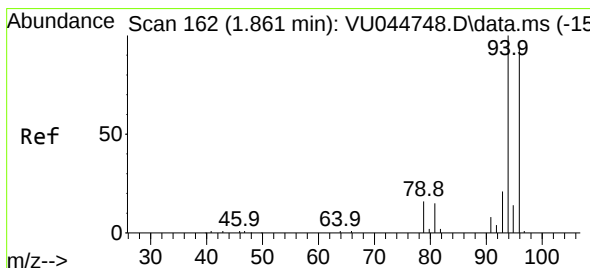


#6
Bromomethane
Concen: 3.366 ug/L
RT: 1.861 min Scan# 162
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

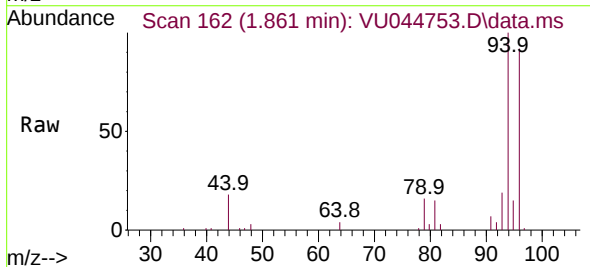

Tgt Ion: 94 Resp: 22465
Ion Ratio Lower Upper
94 100
96 92.3 66.4 123.4

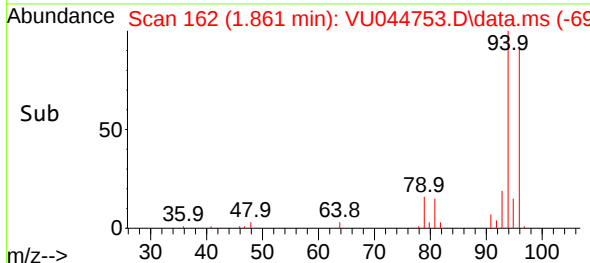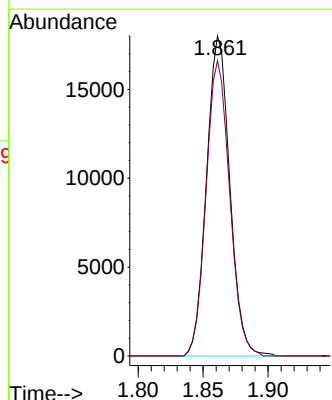







#9
Trichlorofluoromethane
Concen: 8.228 ug/L
RT: 2.141 min Scan# 249
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Instrument :
MSVOA_U
ClientSampled :
GB6Y1

Tgt Ion:101 Resp: 120679
Ion Ratio Lower Upper
101 100
103 64.7 51.2 76.8




Manual Integrations
APPROVED


MMDadoda
9/24/2021 1:35:29 PM

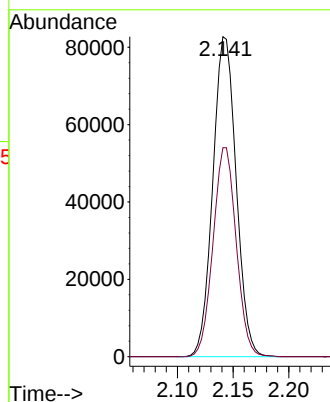

#12
1,1-Dichloroethene
Concen: 3.896 ug/L
RT: 2.584 min Scan# 387
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Tgt Ion: 96 Resp: 33337
Ion Ratio Lower Upper
96 100
61 187.1 129.3 240.1
63 120.0 91.3 169.5

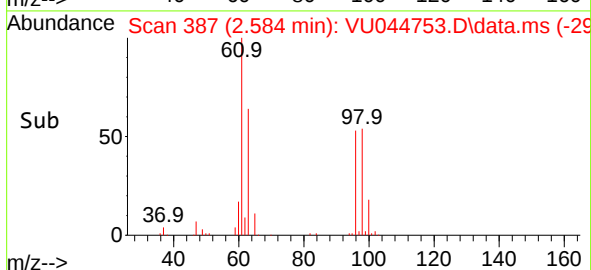







#13
Acetone
Concen: 99.267 ug/L m
RT: 2.646 min Scan# 406
Delta R.T. -0.003 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Instrument :
MSVOA_U
ClientSampleId :
GB6Y1

Tgt Ion: 43 Resp: 213000
Ion Ratio Lower Upper
43 100
58 20.5 0.0 42.4




Manual Integrations
APPROVED


MMDadoda
9/24/2021 1:35:29 PM

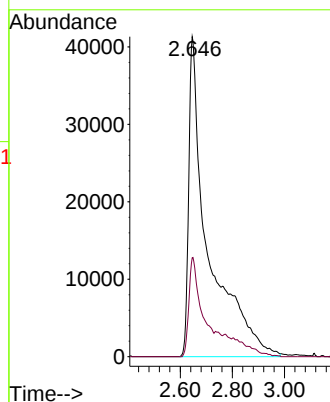

#14
Carbon disulfide
Concen: 5.682 ug/L
RT: 2.797 min Scan# 453
Delta R.T. -0.003 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49


Tgt Ion: 76 Resp: 153930
Ion Ratio Lower Upper
76 100
78 8.4 7.4 11.0

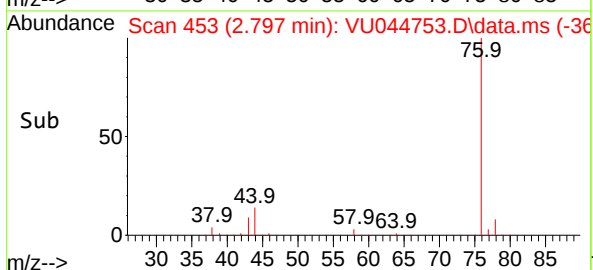



#16
Methylene chloride
Concen: 2.792 ug/L
RT: 3.054 min Scan# 533
Delta R.T. 0.003 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Instrument :
MSVOA_U
ClientSampled :
GB6Y1






Tgt Ion: 84 Resp: 37994


Ion	Ratio	Lower	Upper
84	100		
86	62.9	45.8	85.2
49	132.6	92.9	172.5

Manual Integrations
APPROVED

MMDadoda
9/24/2021 1:35:29 PM

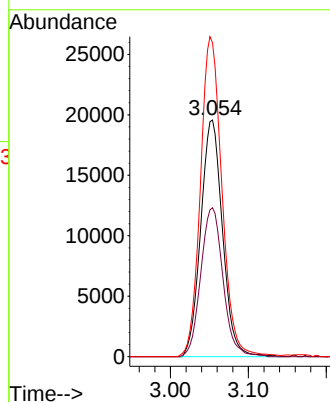




#17
Methyl tert-butyl Ether
Concen: 8.646 ug/L
RT: 3.372 min Scan# 632
Delta R.T. -0.003 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49



Tgt Ion: 73 Resp: 204500

Ion	Ratio	Lower	Upper
73	100		
43	22.6	17.8	26.6
57	23.1	18.6	27.8

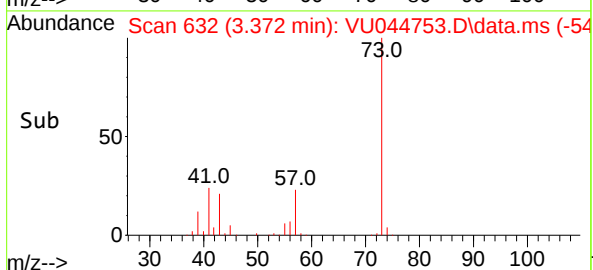



#19

1,1-Dichloroethane

Concen: 9.790 ug/L

RT: 3.877 min Scan# 789

Delta R.T. 0.000 min

Lab File: VU044753.D

Acq: 22 Sep 2021 12:49

Tgt Ion:	63	Resp:	180044
Ion Ratio	Lower	Upper	
63	100		
65	31.3	21.8	40.6
83	12.8	8.8	16.3

Instrument :





MSVOA_U

ClientSampleId :

GB6Y1

Manual Integrations
APPROVED

MMDadoda
9/24/2021 1:35:29 PM



#21

2-Butanone

Concen: 124.834 ug/L




RT: 4.719 min Scan# 1051


Delta R.T. -0.003 min

Lab File: VU044753.D

Acq: 22 Sep 2021 12:49

Tgt Ion:	43	Resp:	447247
Ion Ratio	Lower	Upper	
43	100		
72	25.3	9.2	27.4

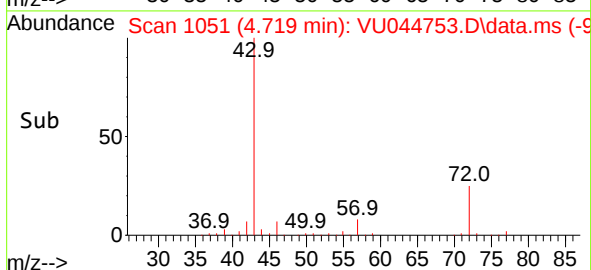



#27

1,2-Dichloroethane

Concen: 7.703 ug/L

RT: 5.803 min Scan# 1388

Delta R.T. 0.000 min

Lab File: VU044753.D

Acq: 22 Sep 2021 12:49

Tgt Ion: 62 Resp: 98839

Ion Ratio Lower Upper

62 100

98 9.3 6.6 10.0

Instrument :

MSVOA_U

ClientSampled :





GB6Y1

Manual Integrations

APPROVED

MMDadoda

9/24/2021 1:35:29 PM

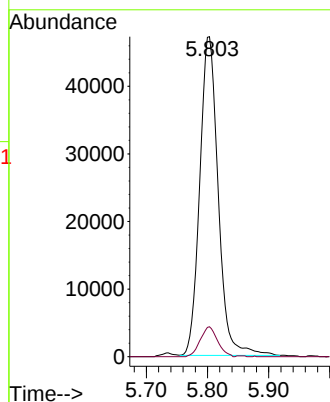

#29

1,1,1-Trichloroethane

Concen: 9.203 ug/L

RT: 5.324 min Scan# 1239

Delta R.T. 0.000 min

Lab File: VU044753.D

Acq: 22 Sep 2021 12:49




Tgt Ion: 97 Resp: 133550


Ion Ratio Lower Upper

97 100

99 63.4 50.7 76.1


61 52.0 40.6 60.8

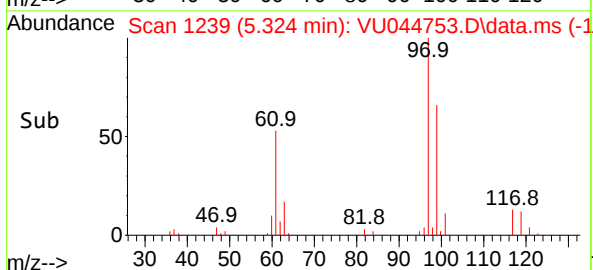



#30
Cyclohexane
Concen: 11.834 ug/L
RT: 5.395 min Scan# 1261
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49




Instrument :
MSVOA_U
ClientSampled :
GB6Y1




Tgt Ion: 56 Resp: 196666
Ion Ratio Lower Upper
56 100
69 29.6 23.4 35.2
84 83.3 65.5 98.3

Manual Integrations
APPROVED



MMDadoda
9/24/2021 1:35:29 PM

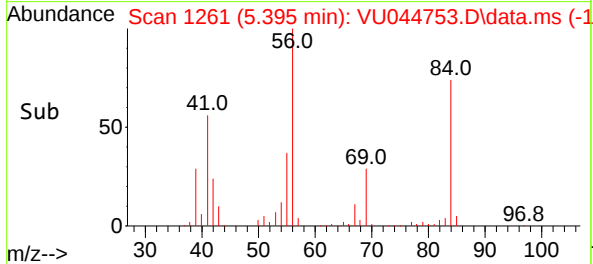


#34
Trichloroethene
Concen: 5.453 ug/L
RT: 6.549 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

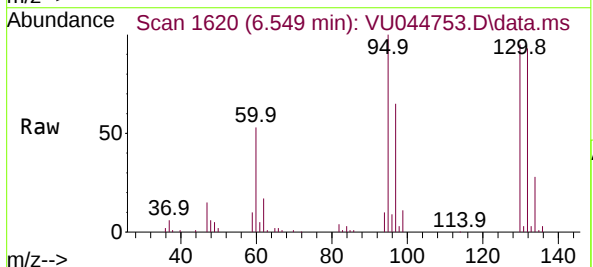

Tgt Ion: 95 Resp: 53358
Ion Ratio Lower Upper
95 100
97 65.3 44.7 82.9
132 93.1 60.3 111.9
130 95.0 63.7 118.3

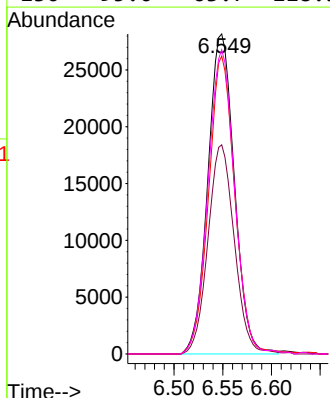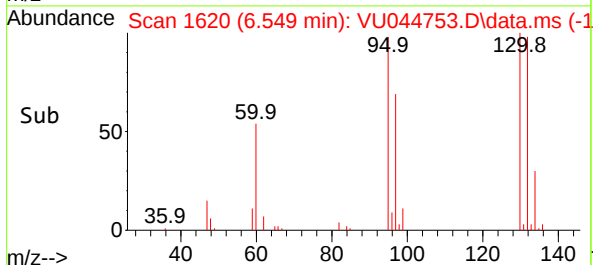



#35

Methylcyclohexane

Concen: 6.599 ug/L

RT: 6.768 min Scan# 1688

Delta R.T. -0.003 min

Lab File: VU044753.D





Acq: 22 Sep 2021 12:49

Tgt Ion:	83	Resp:	106104
Ion Ratio	Lower	Upper	
83	100		
55	85.8	68.3	102.5
98	47.8	37.3	55.9

Instrument :
MSVOA_U
ClientSampled :
GB6Y1

Manual Integrations
APPROVED

MMDadoda
9/24/2021 1:35:29 PM

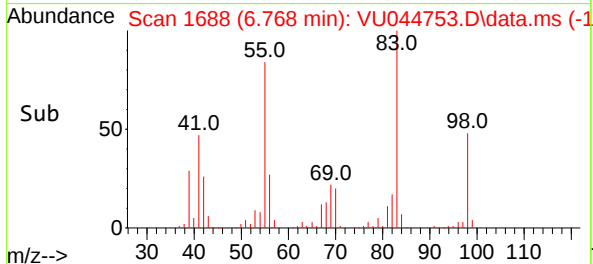

#37

1,2-Dichloropropane

Concen: 2.331 ug/L




RT: 6.797 min Scan# 1697


Delta R.T. -0.003 min

Lab File: VU044753.D

Acq: 22 Sep 2021 12:49


Tgt Ion:	63	Resp:	24692
Ion Ratio	Lower	Upper	
63	100		
112	3.7	3.1	4.7

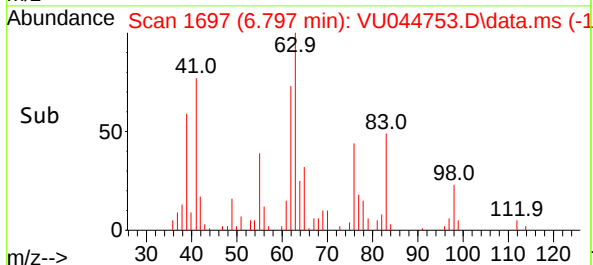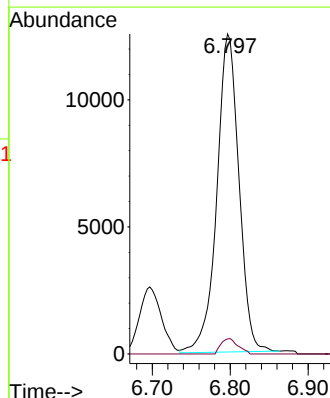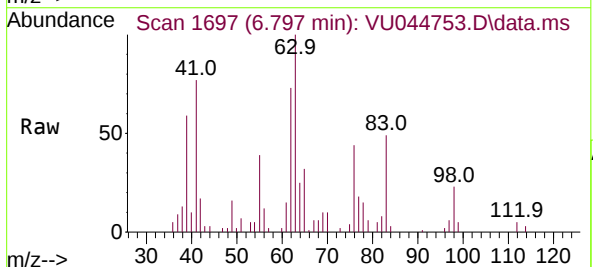



#42
Toluene
Concen: 8.904 ug/L
RT: 7.977 min Scan# 2064
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49




Instrument :
MSVOA_U
ClientSampled :
GB6Y1




Tgt Ion: 91 Resp: 367533
Ion Ratio Lower Upper
91 100
92 56.9 41.1 76.3

Manual Integrations
APPROVED



MMDadoda
9/24/2021 1:35:29 PM

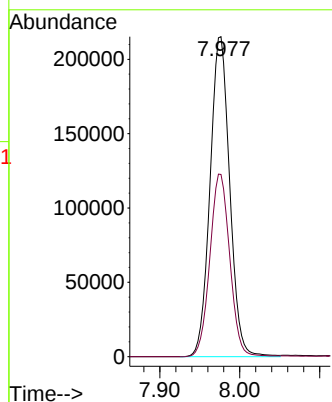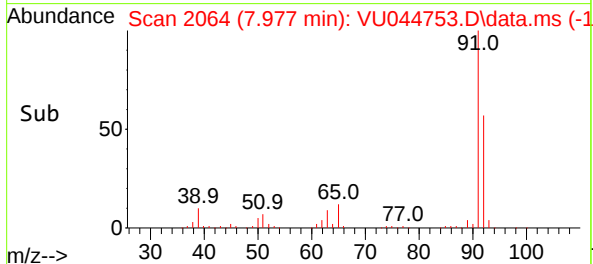


#47
Tetrachloroethene
Concen: 9.203 ug/L
RT: 8.559 min Scan# 2245
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49




Tgt Ion: 164 Resp: 62530
Ion Ratio Lower Upper
164 100
129 96.6 67.0 124.4
131 93.4 65.2 121.0
166 128.0 87.6 162.8

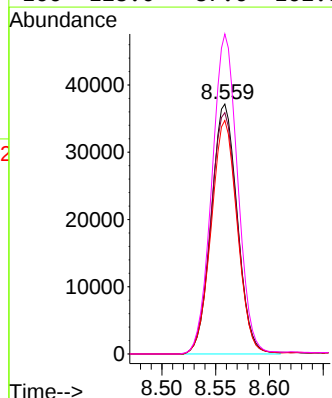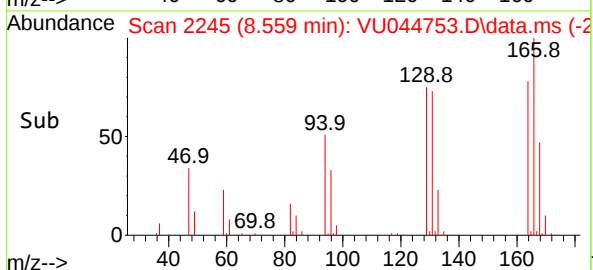



#48
2-Hexanone
Concen: 56.180 ug/L
RT: 8.697 min Scan# 2288
Delta R.T. 0.003 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49




Instrument :
MSVOA_U
ClientSampleId :
GB6Y1




Tgt Ion: 43 Resp: 344719
Ion Ratio Lower Upper
43 100
58 56.0 44.6 66.8
57 19.0 14.8 22.2
100 11.3 9.0 13.4

Manual Integrations
APPROVED



MMDadoda
9/24/2021 1:35:29 PM

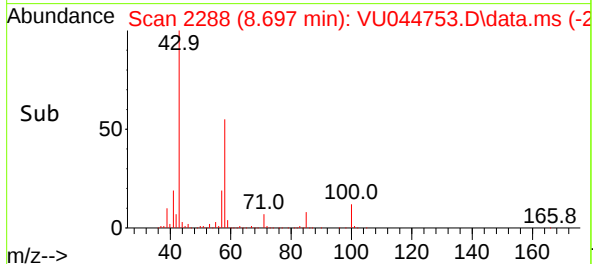


#50
1,2-Dibromoethane
Concen: 16.108 ug/L
RT: 8.928 min Scan# 2360
Delta R.T. -0.003 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

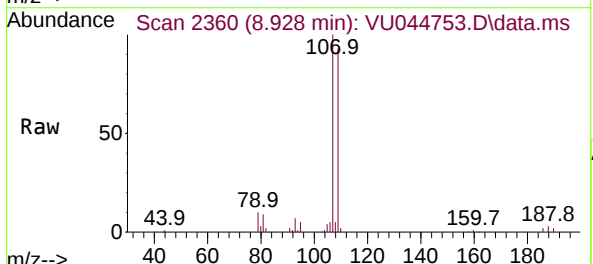

Tgt Ion: 107 Resp: 114197
Ion Ratio Lower Upper
107 100
109 93.1 65.5 121.7
188 3.5 3.0 4.4

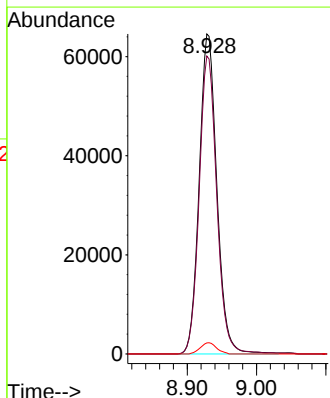







#51
Chlorobenzene
Concen: 11.023 ug/L
RT: 9.452 min Scan# 2523
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Instrument :
MSVOA_U
ClientSampled :
GB6Y1

Tgt Ion:112 Resp: 282101
Ion Ratio Lower Upper
112 100
114 32.5 22.8 42.4
77 62.7 51.4 77.0




Manual Integrations
APPROVED


MMDadoda
9/24/2021 1:35:29 PM

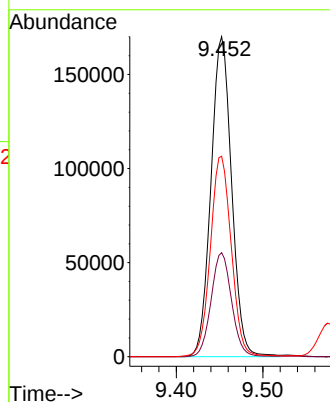

#52
Ethylbenzene
Concen: 6.768 ug/L
RT: 9.575 min Scan# 2561
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Tgt Ion: 91 Resp: 302605
Ion Ratio Lower Upper
91 100
106 30.3 21.1 39.1

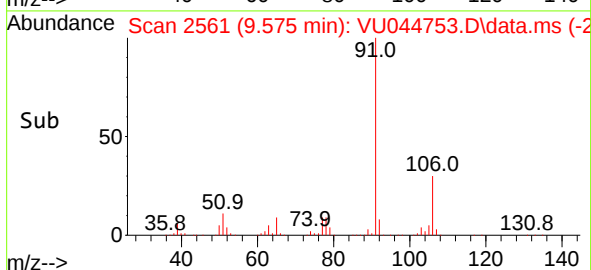







#53
m,p-Xylene
Concen: 14.012 ug/L
RT: 9.703 min Scan# 2601
Delta R.T. 0.003 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Tgt Ion:106 Resp: 238230
Ion Ratio Lower Upper
106 100
91 206.0 144.6 268.6

Instrument :
MSVOA_U
ClientSampleId :
GB6Y1




Manual Integrations
APPROVED


MMDadoda
9/24/2021 1:35:29 PM

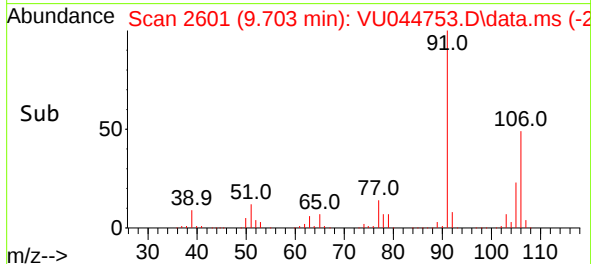

#54
o-Xylene
Concen: 5.676 ug/L
RT: 10.105 min Scan# 2726
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Tgt Ion:106 Resp: 92182
Ion Ratio Lower Upper
106 100
91 221.0 156.2 290.0

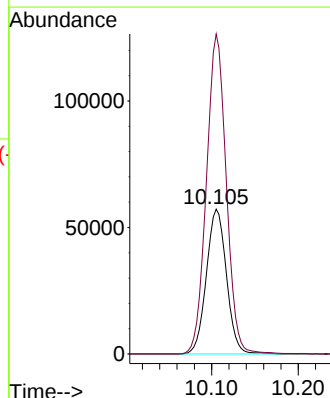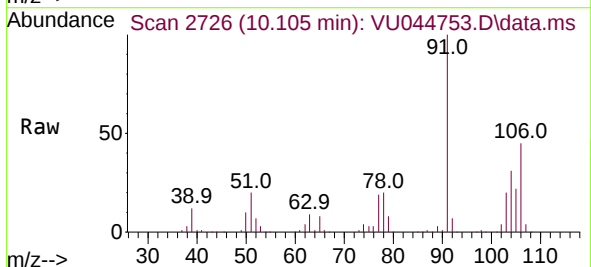







#55
Styrene
Concen: 5.552 ug/L
RT: 10.118 min Scan# 2730
Delta R.T. -0.003 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Instrument :
MSVOA_U
ClientSampled :
GB6Y1

Tgt Ion:104 Resp: 157850
Ion Ratio Lower Upper
104 100
78 48.7 33.6 62.4




Manual Integrations
APPROVED


MMDadoda
9/24/2021 1:35:29 PM

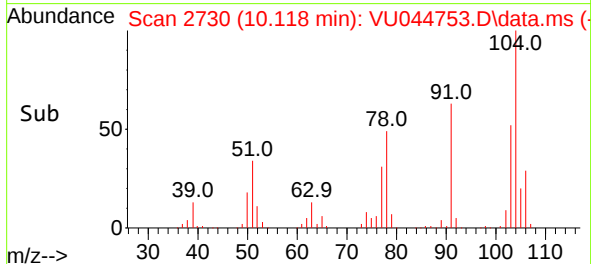

#59
Bromoform
Concen: 5.478 ug/L
RT: 10.295 min Scan# 2785
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Tgt Ion:173 Resp: 22322
Ion Ratio Lower Upper
173 100
175 46.3 38.8 58.2
254 5.9 4.9 7.3

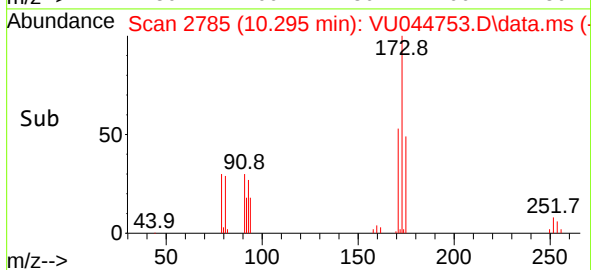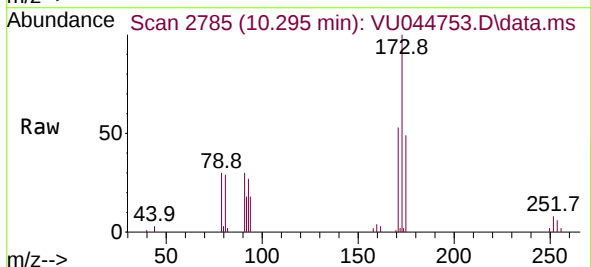

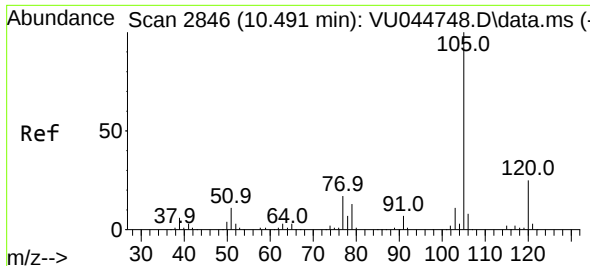





#60
Isopropylbenzene
Concen: 3.524 ug/L
RT: 10.488 min Scan# 2845
Delta R.T. -0.003 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

Tgt Ion:105 Resp: 144627
Ion Ratio Lower Upper
105 100
120 25.9 20.2 30.2
77 17.1 13.6 20.4

Instrument :
MSVOA_U
ClientSampled :
GB6Y1




Manual Integrations
APPROVED


MMDadoda
9/24/2021 1:35:29 PM

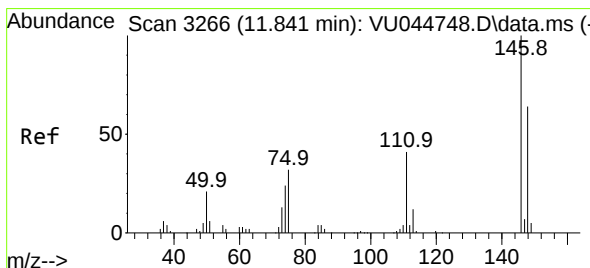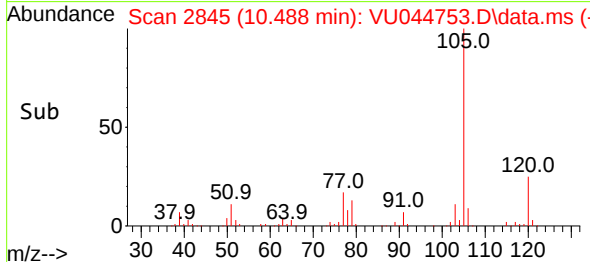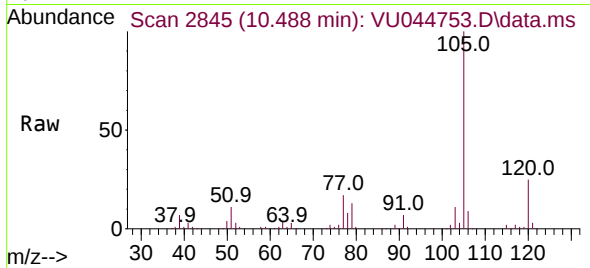

#65
1,4-Dichlorobenzene
Concen: 4.200 ug/L
RT: 11.841 min Scan# 3266
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49


Tgt Ion:146 Resp: 82911
Ion Ratio Lower Upper
146 100
111 39.7 28.7 53.3
148 63.2 45.4 84.4

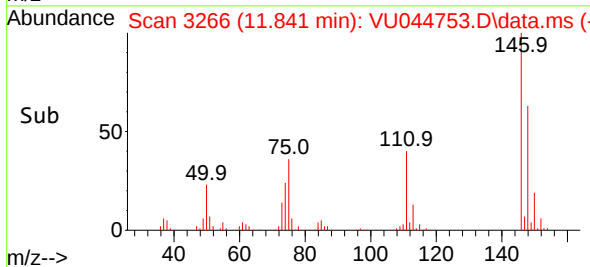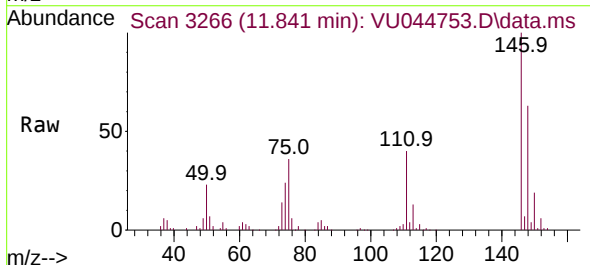

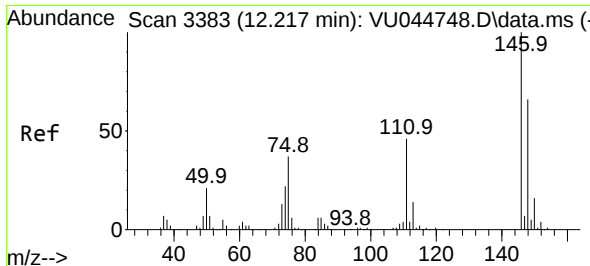

#67
1,2-Dichlorobenzene
Concen: 12.607 ug/L
RT: 12.218 min Scan# 3383
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49




Instrument :
MSVOA_U
ClientSampled :
GB6Y1

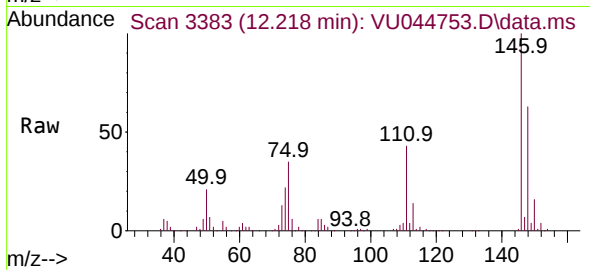


Tgt Ion:146 Resp: 228967
Ion Ratio Lower Upper
146 100
111 43.0 34.6 51.8
148 63.4 51.3 76.9

Manual Integrations
APPROVED



MMDadoda
9/24/2021 1:35:29 PM

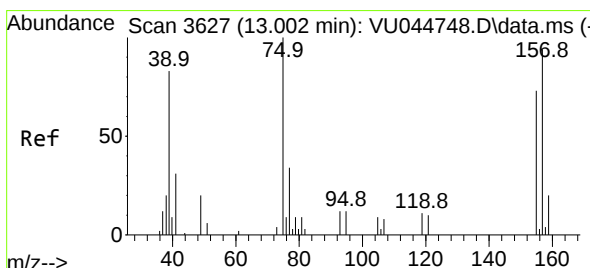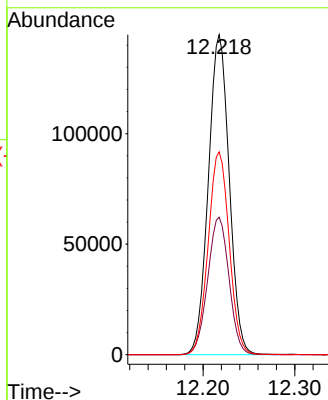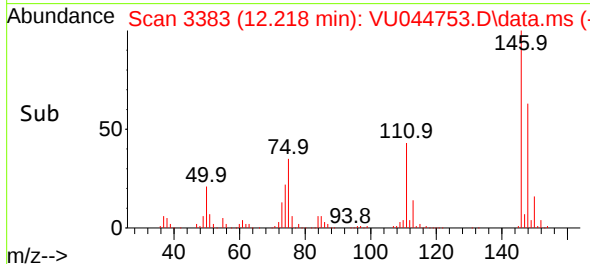


#68
1,2-Dibromo-3-chloropropane
Concen: 3.761 ug/L
RT: 13.002 min Scan# 3627
Delta R.T. 0.000 min
Lab File: VU044753.D
Acq: 22 Sep 2021 12:49

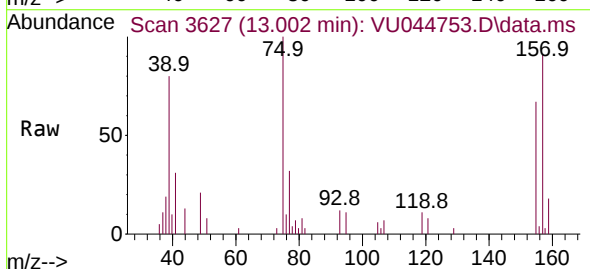


Tgt Ion: 75 Resp: 5992
Ion Ratio Lower Upper
75 100
155 66.7 54.0 81.0
157 91.3 65.4 98.2

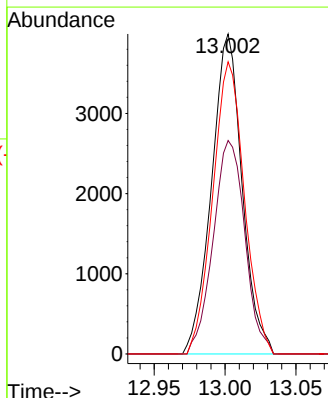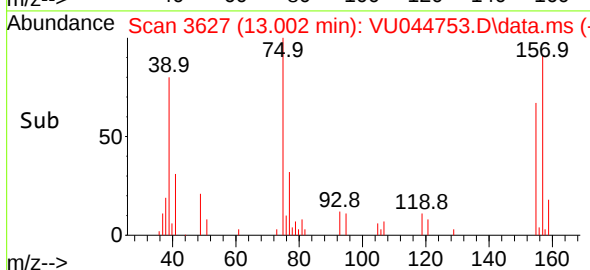



#72
 1,2,3-Trichlorobenzene
 Concen: 9.511 ug/L
 RT: 14.333 min Scan# 4041
 Delta R.T. 0.000 min
 Lab File: VU044753.D
 Acq: 22 Sep 2021 12:49

Instrument :
 MSVOA_U
 ClientSampled :
 GB6Y1

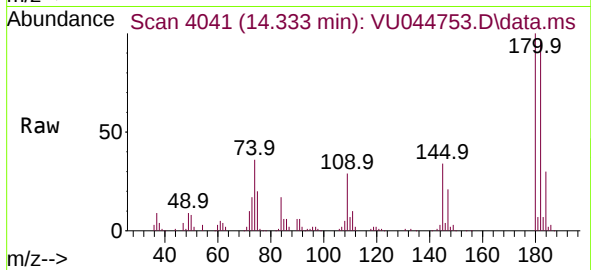

Tgt Ion:180 Resp: 107422
 Ion Ratio Lower Upper
 180 100
 182 95.1 75.9 113.9
 145 33.3 27.0 40.6

Manual Integrations
 APPROVED

MMDadoda
 9/24/2021 1:35:29 PM

