

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
 Data File : VU044757.D
 Acq On : 22 Sep 2021 14:39
 Operator : SY/MD
 Sample : M3814-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6W5

Quant Time: Sep 23 03:03:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 23 02:59:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	124302	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	126931	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	56452	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	31142	4.246	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.000%
7) Chloroethane-d5	1.916	69	30952	4.135	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.800%
11) 1,1-Dichloroethene-d2	2.571	65	14216	3.838	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.800%
20) 2-Butanone-d5	4.642	46	132741	43.175	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	86.340%
24) Chloroform-d	5.070	84	69730	4.520	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%
26) 1,2-Dichloroethane-d4	5.710	65	41624	4.525	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.400%
32) Benzene-d6	5.735	84	129788	4.010	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.200%
36) 1,2-Dichloropropane-d6	6.697	67	45996	4.327	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.600%
41) Toluene-d8	7.902	98	105251	3.736	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.800%
43) trans-1,3-Dichloroprop...	8.185	79	14883	3.972	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.400%
46) 2-Hexanone-d5	8.645	63	99246	41.215	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.420%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	40729	4.322	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	12.198	152	42020	4.511	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.200%
Target Compounds					Qvalue	
13) Acetone	2.649	43	4604	2.299	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044757.D
Acq On : 22 Sep 2021 14:39
Operator : SY/MD
Sample : M3814-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB6W5

Quant Time: Sep 23 03:03:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 23 02:59:45 2021
Response via : Initial Calibration

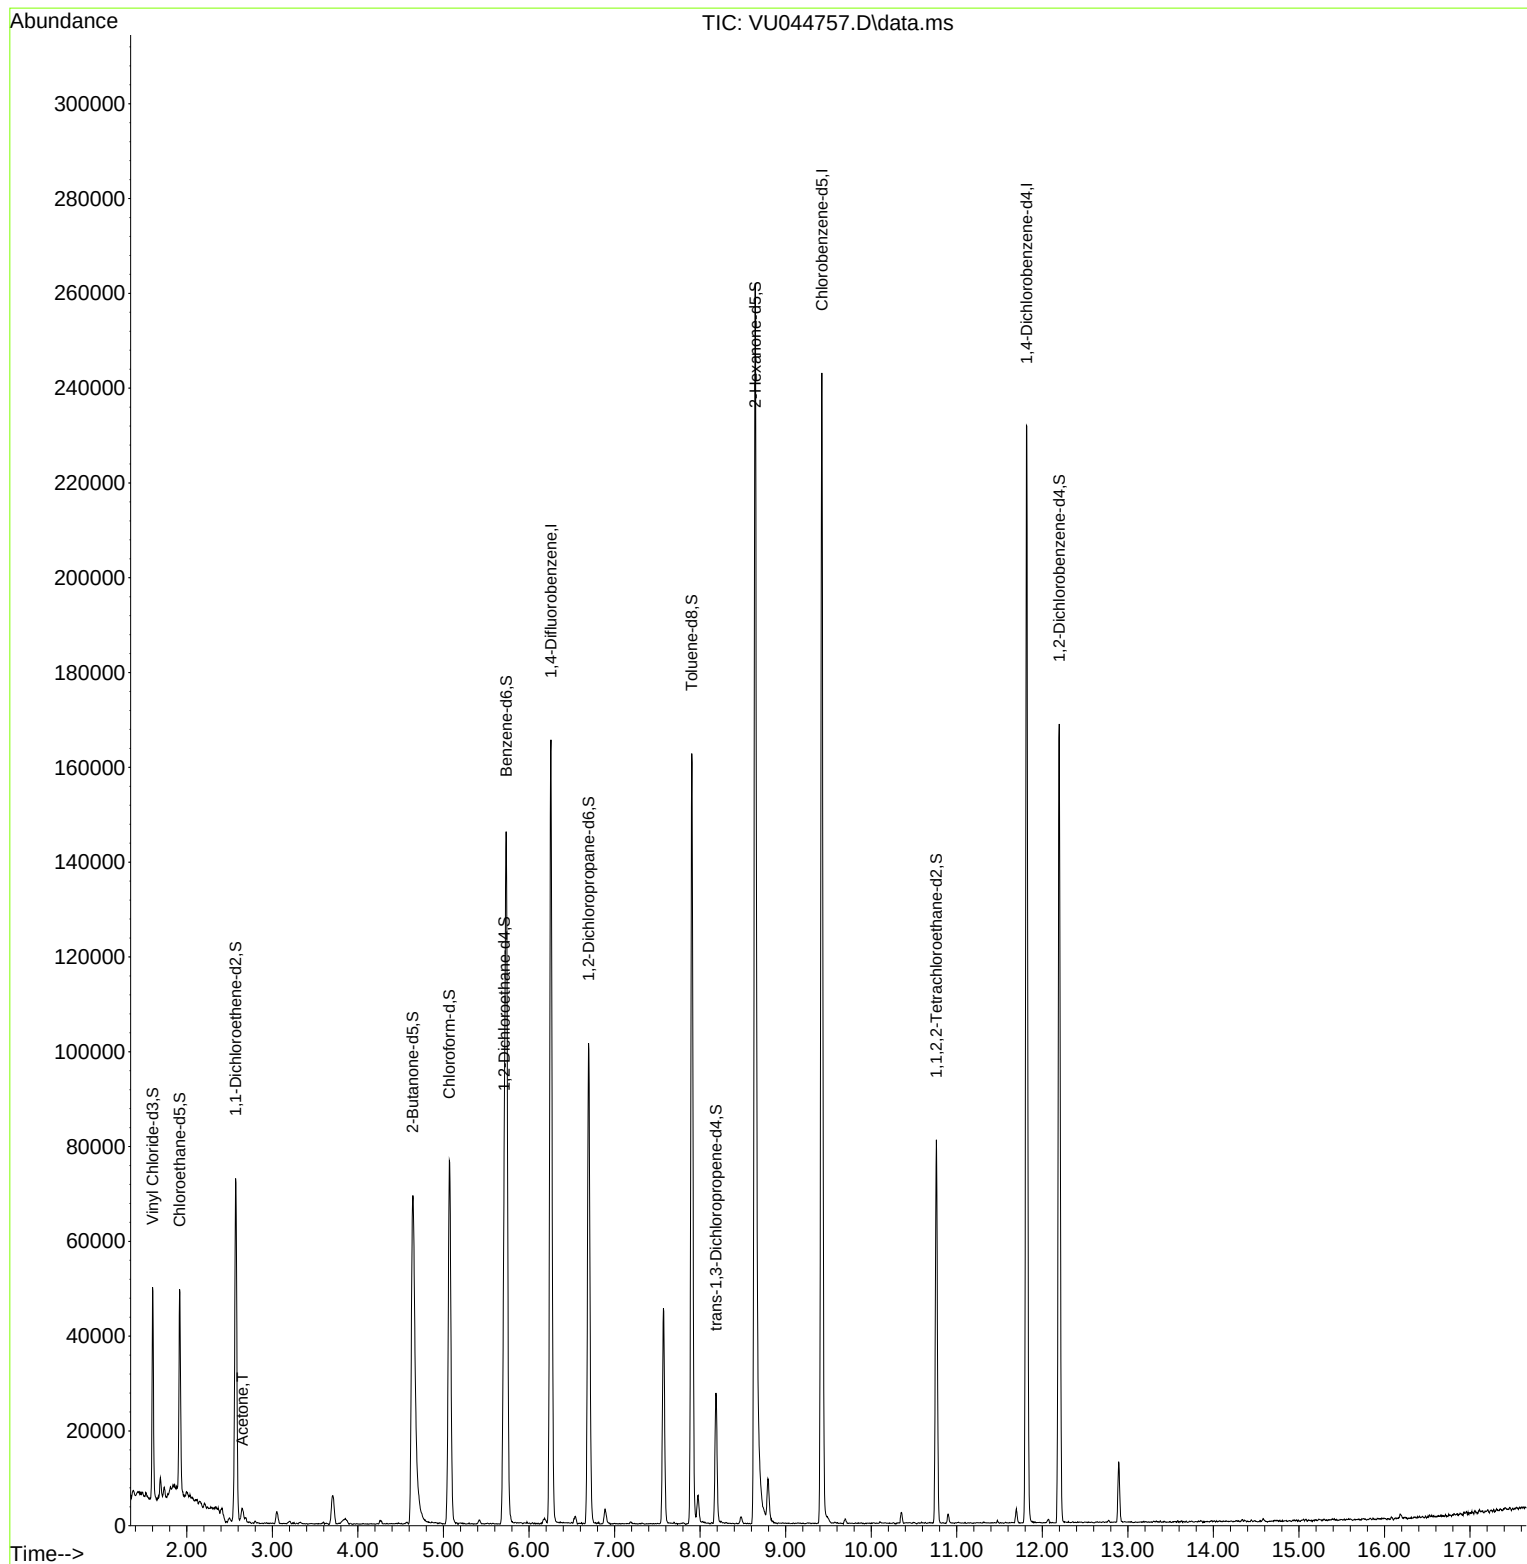

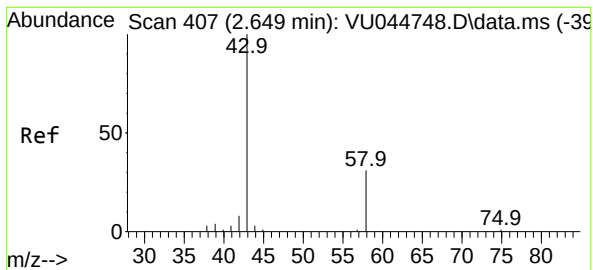

#13
 Acetone
 Concen: 2.299 ug/L
 RT: 2.649 min Scan# 407
 Delta R.T. -0.000 min
 Lab File: VU044757.D
 Acq: 22 Sep 2021 14:39

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6W5

Tgt Ion: 43 Resp: 4604
 Ion Ratio Lower Upper
 43 100
 58 27.8 0.0 42.4

