

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
 Data File : VU044767.D
 Acq On : 22 Sep 2021 18:39
 Operator : SY/MD
 Sample : M3814-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6X3

Quant Time: Sep 23 03:05:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 23 02:59:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	125947	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	126872	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	56870	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	30294	4.076	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.600%
7) Chloroethane-d5	1.916	69	29889	3.941	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.800%
11) 1,1-Dichloroethene-d2	2.571	65	13196	3.516	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.400%
20) 2-Butanone-d5	4.642	46	136174	43.713	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.420%
24) Chloroform-d	5.070	84	69770	4.463	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
26) 1,2-Dichloroethane-d4	5.710	65	41805	4.485	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.800%
32) Benzene-d6	5.732	84	127281	3.935	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.600%
36) 1,2-Dichloropropane-d6	6.697	67	46149	4.344	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.800%
41) Toluene-d8	7.902	98	100957	3.585	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.600%
43) trans-1,3-Dichloroprop...	8.185	79	15174	4.052	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.000%
46) 2-Hexanone-d5	8.642	63	100807	41.882	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.760%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	41354	4.390	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.800%
66) 1,2-Dichlorobenzene-d4	12.198	152	40104	4.274	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.400%
Target Compounds						
					Qvalue	
13) Acetone	2.649	43	6602	3.254	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044767.D
Acq On : 22 Sep 2021 18:39
Operator : SY/MD
Sample : M3814-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB6X3

Quant Time: Sep 23 03:05:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 23 02:59:45 2021
Response via : Initial Calibration

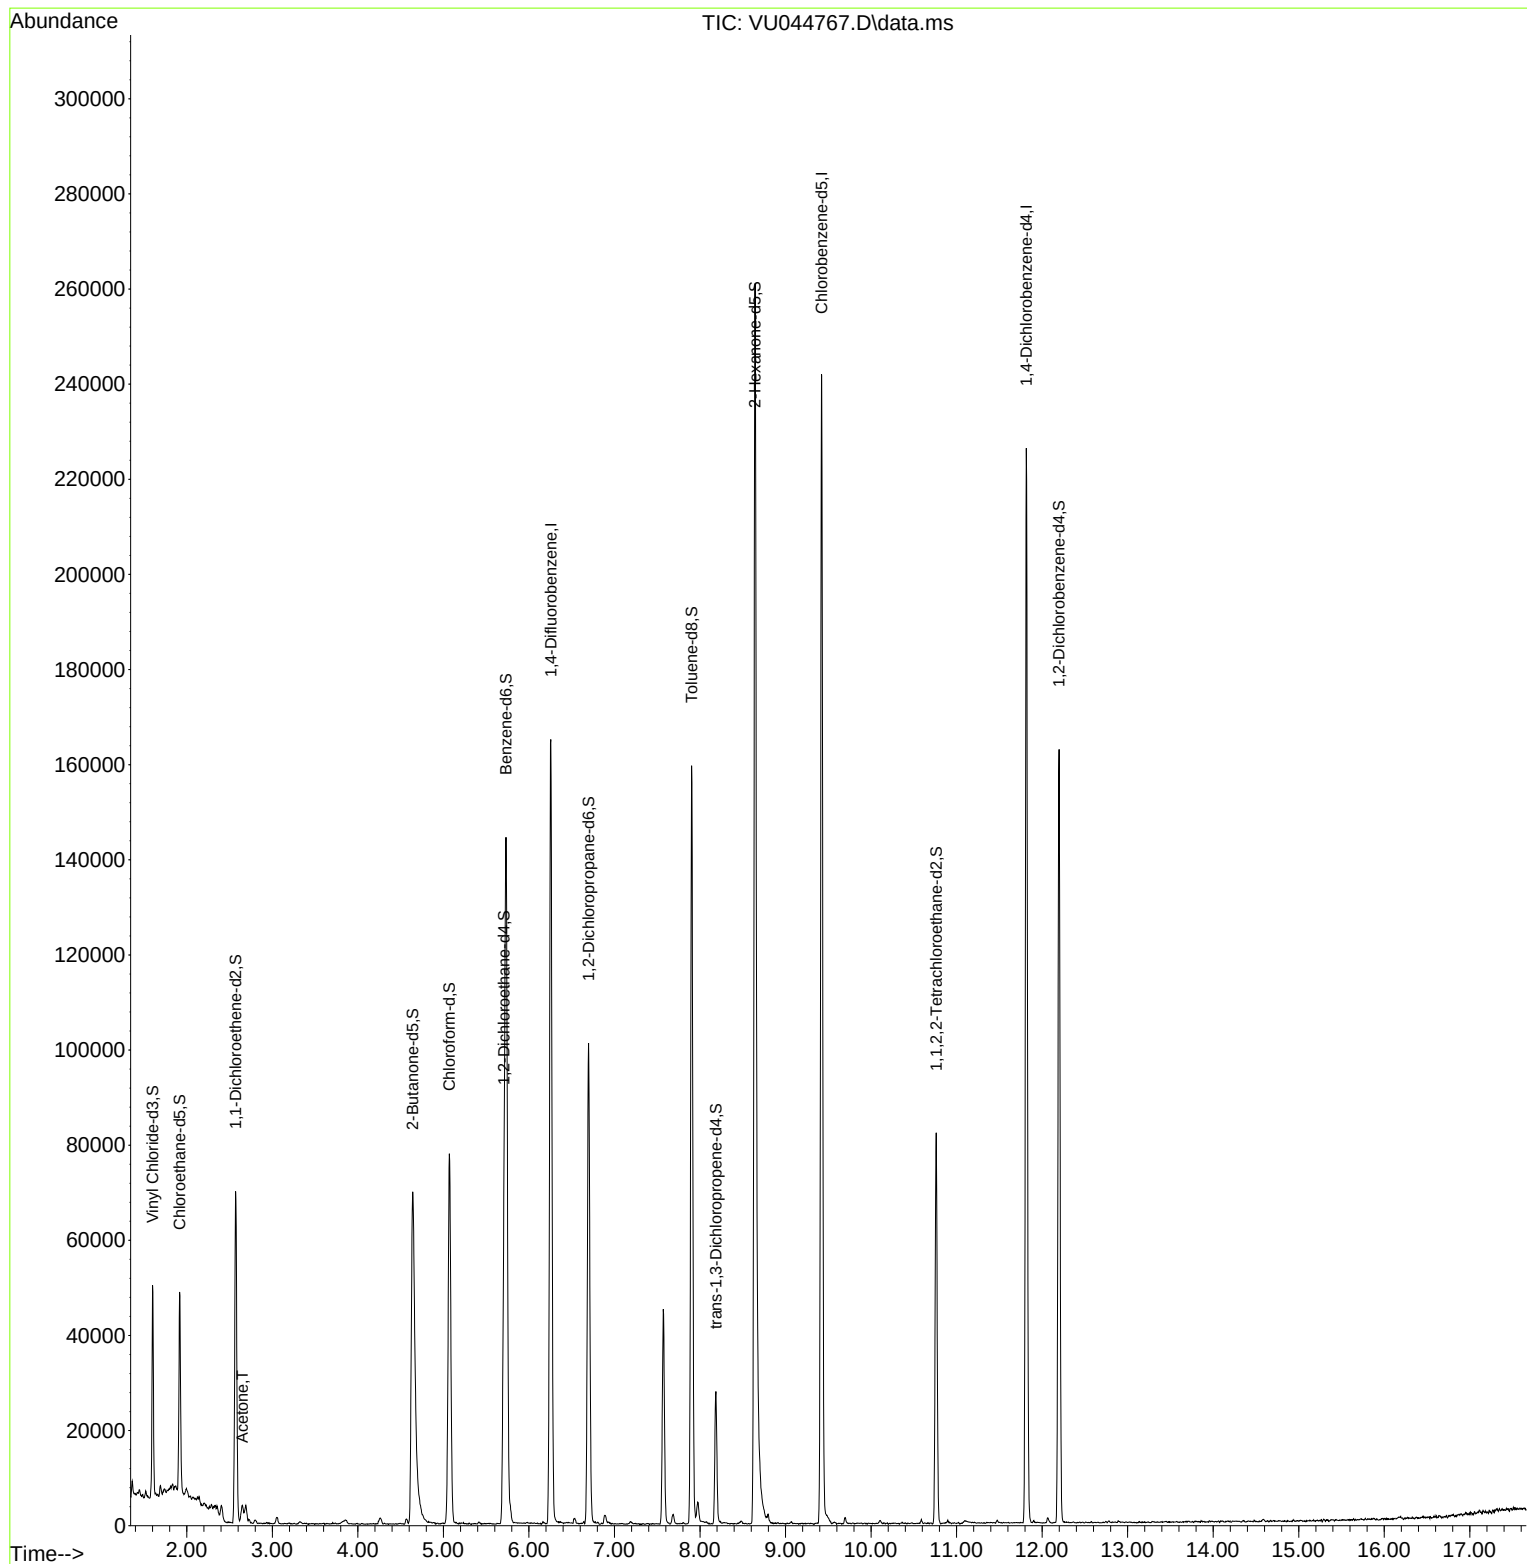

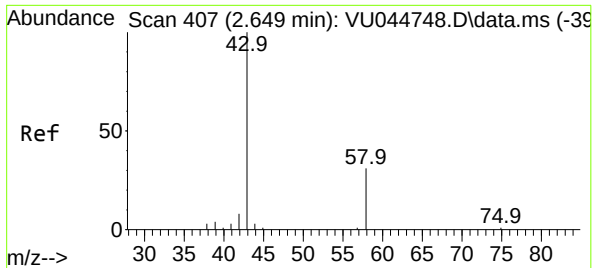

#13
 Acetone
 Concen: 3.254 ug/L
 RT: 2.649 min Scan# 407
 Delta R.T. -0.000 min
 Lab File: VU044767.D
 Acq: 22 Sep 2021 18:39

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6X3

Tgt Ion: 43	Resp: 6602
Ion Ratio	Lower Upper
43 100	
58 31.5	0.0 42.4

