

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
 Data File : VU044768.D
 Acq On : 22 Sep 2021 19:04
 Operator : SY/MD
 Sample : M3814-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6X4

Quant Time: Sep 23 03:06:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 23 02:59:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	121452	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	125960	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	54868	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	29385	4.101	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.000%
7) Chloroethane-d5	1.916	69	29123	3.982	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.600%
11) 1,1-Dichloroethene-d2	2.572	65	13203	3.648	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.000%
20) 2-Butanone-d5	4.642	46	132093	43.972	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.940%
24) Chloroform-d	5.073	84	67638	4.487	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%
26) 1,2-Dichloroethane-d4	5.710	65	41144	4.578	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
32) Benzene-d6	5.735	84	122330	3.809	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.200%
36) 1,2-Dichloropropane-d6	6.697	67	44059	4.177	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.600%
41) Toluene-d8	7.903	98	96830	3.463	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.200%#
43) trans-1,3-Dichloroprop...	8.186	79	14661	3.943	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.800%
46) 2-Hexanone-d5	8.645	63	99774	41.753	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.500%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	40232	4.302	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.000%
66) 1,2-Dichlorobenzene-d4	12.198	152	39456	4.358	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.200%
Target Compounds						Qvalue
13) Acetone	2.649	43	9036	4.618	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044768.D
Acq On : 22 Sep 2021 19:04
Operator : SY/MD
Sample : M3814-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB6X4

Quant Time: Sep 23 03:06:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 23 02:59:45 2021
Response via : Initial Calibration

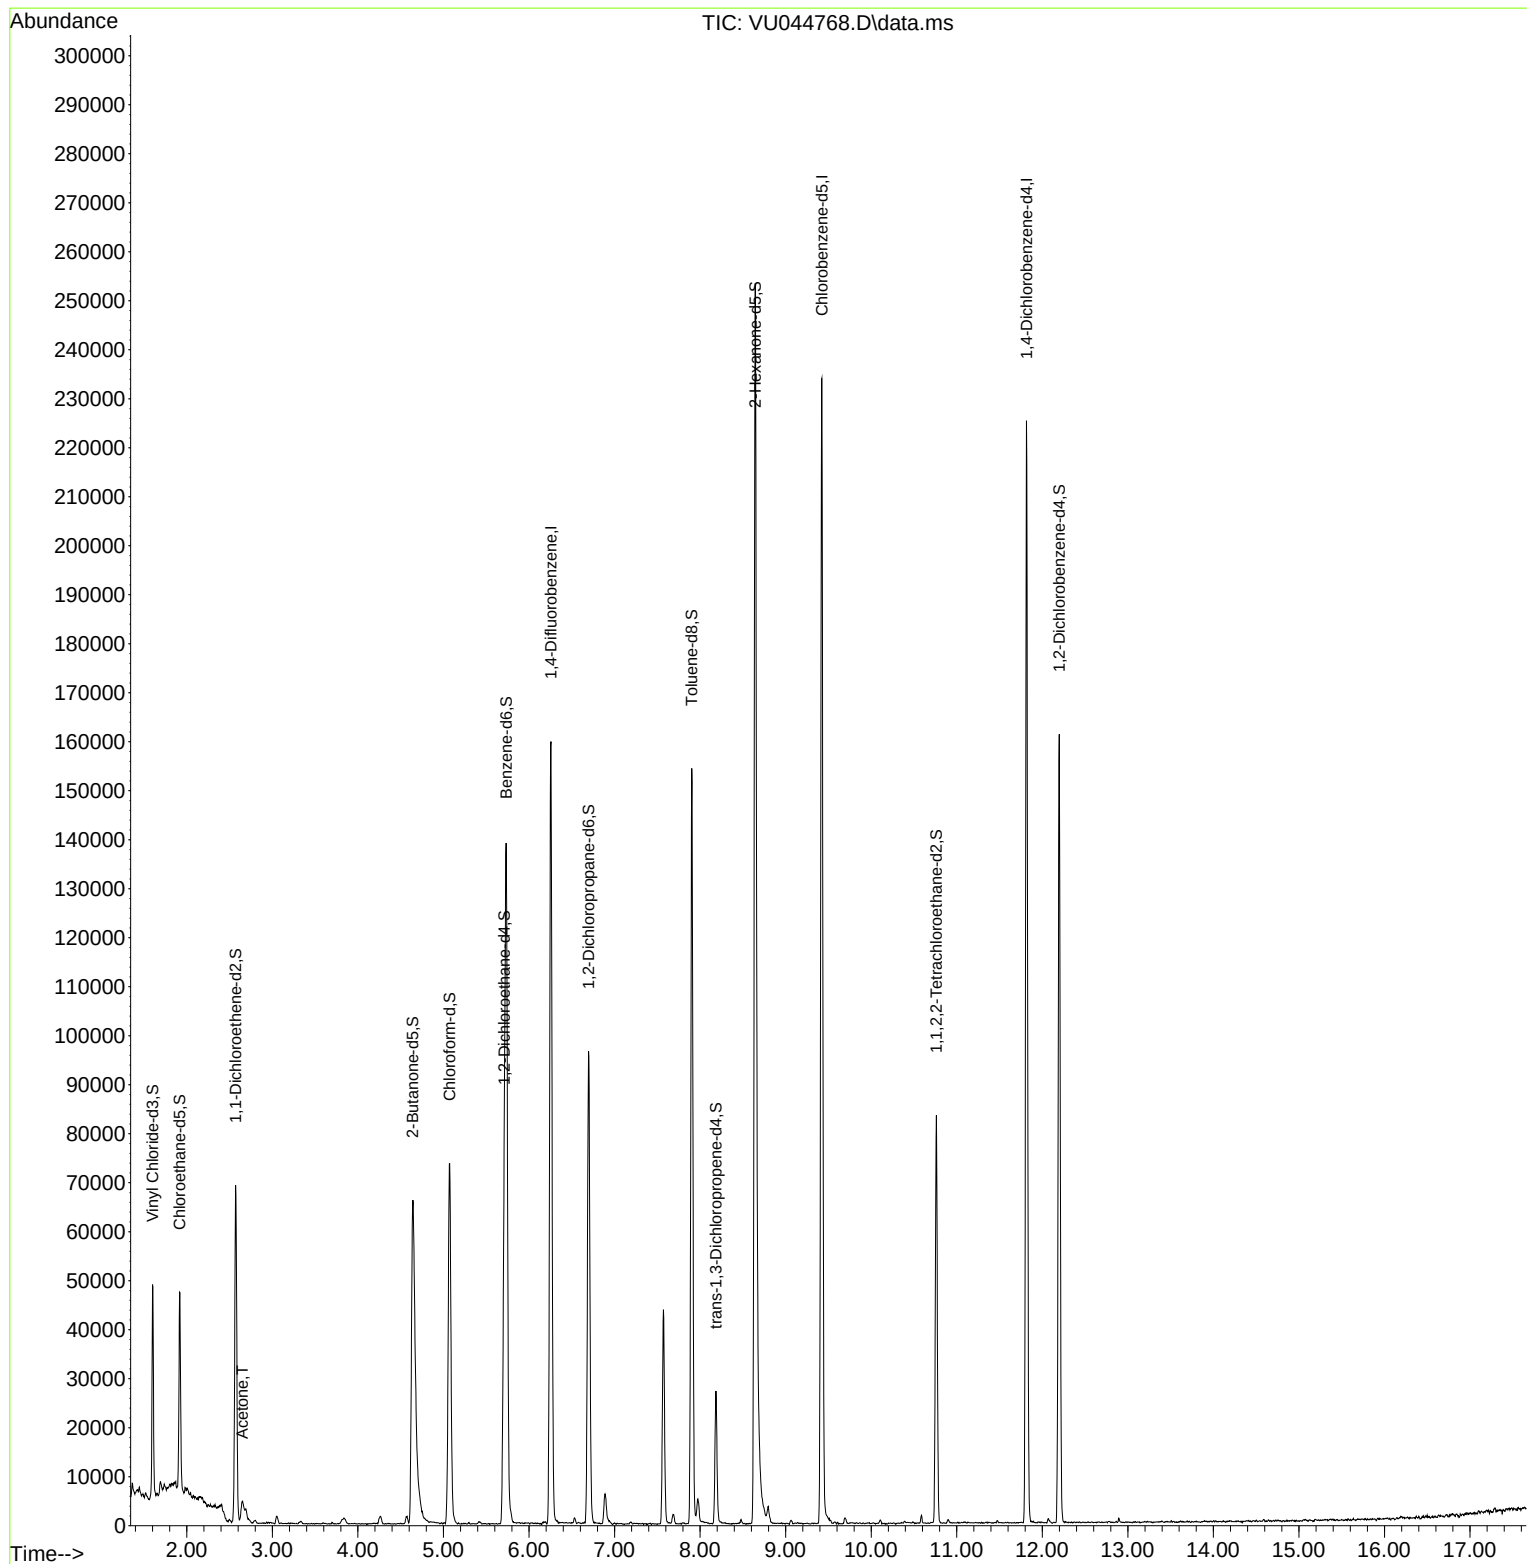

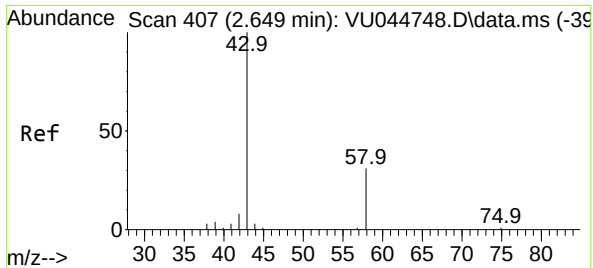

#13
 Acetone
 Concen: 4.618 ug/L
 RT: 2.649 min Scan# 407
 Delta R.T. 0.000 min
 Lab File: VU044768.D
 Acq: 22 Sep 2021 19:04

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6X4

Tgt Ion: 43 Resp: 9036
 Ion Ratio Lower Upper
 43 100
 58 27.6 0.0 42.4

