

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
 Data File : VU044761.D
 Acq On : 22 Sep 2021 16:16
 Operator : SY/MD
 Sample : M3814-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6W7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	92	rBV	45134	50426	9.36%	1.384%
2	1.691	103	109	118	rBV2	5682	8629	1.60%	0.237%
3	1.916	172	179	193	rVB	41659	54496	10.12%	1.496%
4	2.572	368	383	396	rBV	73110	121246	22.51%	3.329%
5	4.639	1011	1026	1064	rBV	69073	220630	40.95%	6.058%
6	5.070	1145	1160	1187	rVB	76084	168553	31.29%	4.628%
7	5.732	1344	1366	1387	rBV2	145399	382434	70.99%	10.500%
8	6.256	1515	1529	1548	rBV	162222	306596	56.91%	8.418%
9	6.697	1653	1666	1686	rBV	99533	195289	36.25%	5.362%
10	7.571	1926	1938	1954	rBV	45065	78984	14.66%	2.169%
11	7.903	2025	2041	2056	rBV	158422	272220	50.53%	7.474%
12	7.973	2056	2063	2076	rVB	6042	10278	1.91%	0.282%
13	8.186	2115	2129	2144	rBV	28213	47006	8.73%	1.291%
14	8.642	2257	2271	2309	rBV	265967	538716	100.00%	14.791%
15	8.796	2310	2319	2328	rVB4	7382	13683	2.54%	0.376%
16	9.420	2501	2513	2532	rBV	236204	397437	73.77%	10.912%
17	10.761	2917	2930	2944	rBV	82492	131672	24.44%	3.615%
18	11.816	3246	3258	3273	rBV	228600	363912	67.55%	9.992%
19	12.198	3365	3377	3392	rVB	166367	269140	49.96%	7.389%
20	12.893	3585	3593	3602	rVB4	7871	10853	2.01%	0.298%




Sum of corrected areas: 3642200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044761.D
Acq On : 22 Sep 2021 16:16
Operator : SY/MD
Sample : M3814-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB6W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

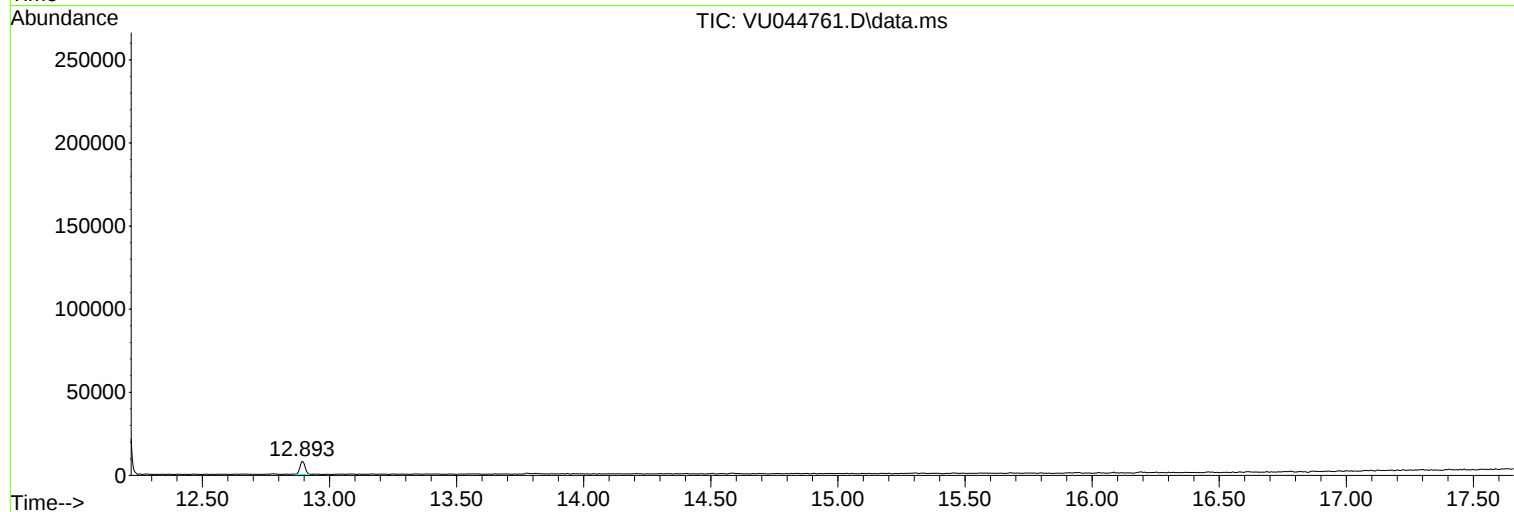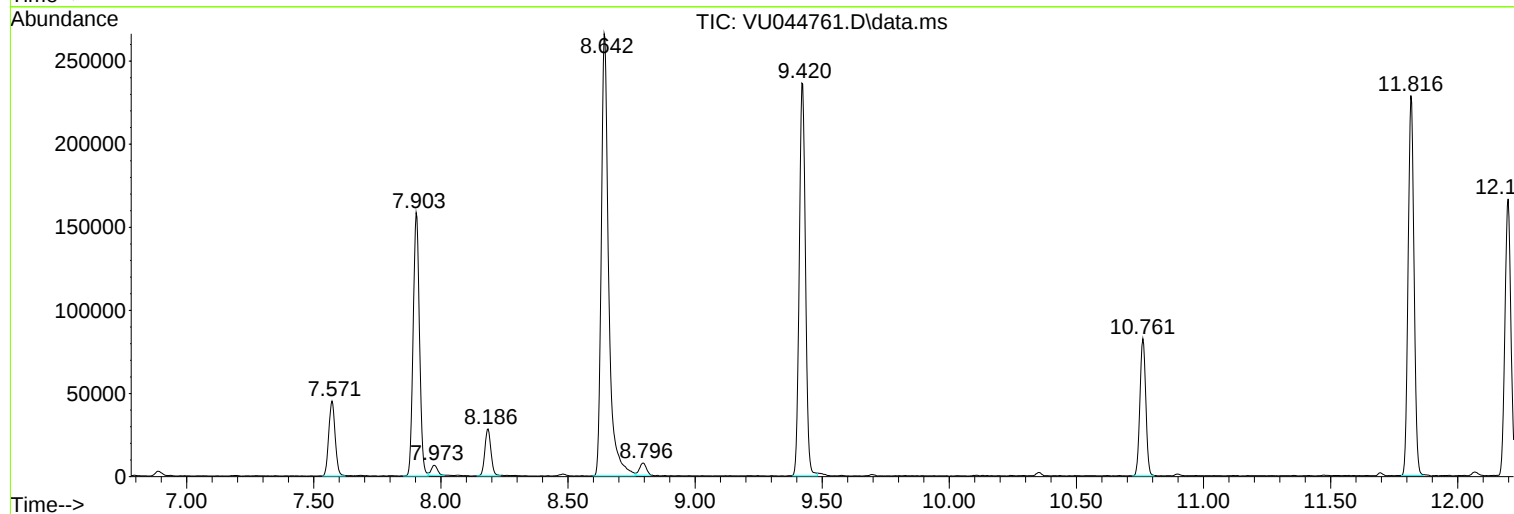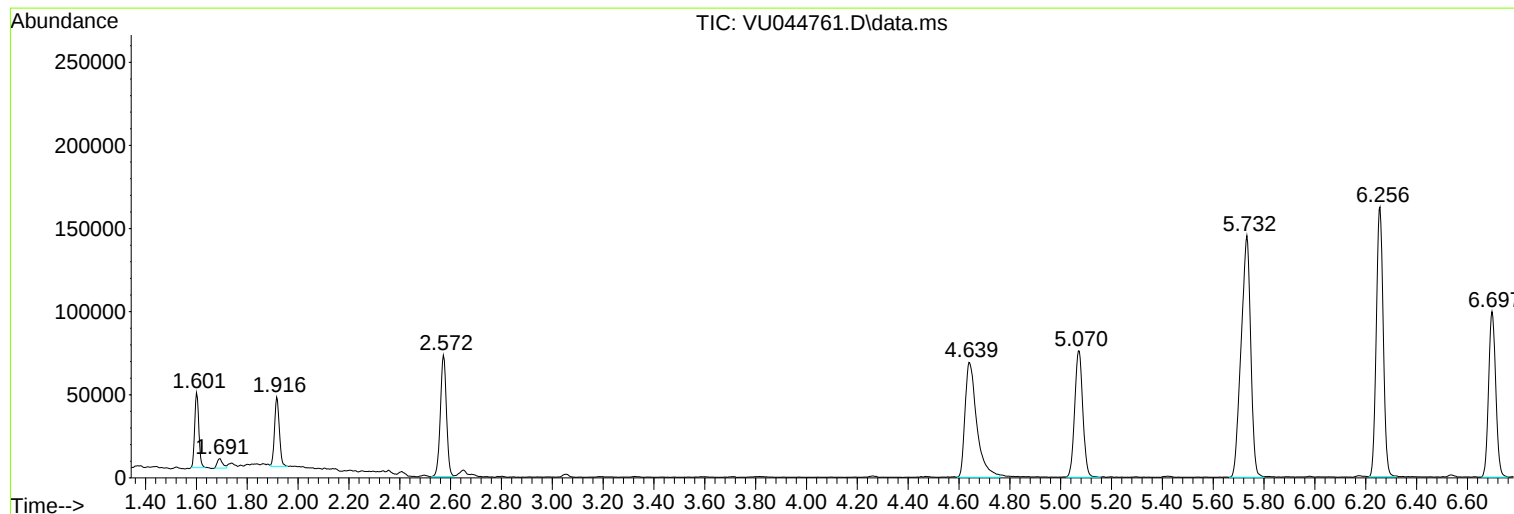

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044761.D
Acq On : 22 Sep 2021 16:16
Operator : SY/MD
Sample : M3814-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB6W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044761.D
Acq On : 22 Sep 2021 16:16
Operator : SY/MD
Sample : M3814-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB6W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
