

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
 Data File : VU044765.D
 Acq On : 22 Sep 2021 17:51
 Operator : SY/MD
 Sample : M3814-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB6X1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	92	rBV	43855	50643	9.42%	1.412%
2	1.919	172	180	191	rVB	40677	53721	9.99%	1.497%
3	2.571	370	383	398	rBV	69356	117191	21.79%	3.267%
4	2.645	398	406	414	rBV2	4183	8228	1.53%	0.229%
5	4.645	1012	1028	1078	rBV2	67822	224617	41.76%	6.261%
6	5.073	1143	1161	1182	rBV	74571	164319	30.55%	4.580%
7	5.732	1339	1366	1394	rBV3	140899	379091	70.48%	10.567%
8	6.256	1514	1529	1551	rBV	158791	300176	55.81%	8.367%
9	6.697	1652	1666	1687	rBV	99490	193617	36.00%	5.397%
10	6.890	1711	1726	1736	rBV3	3834	7741	1.44%	0.216%
11	7.571	1922	1938	1953	rBV	44231	77293	14.37%	2.154%
12	7.902	2027	2041	2055	rBV	155812	268465	49.91%	7.483%
13	7.976	2057	2064	2078	rVB2	5618	9422	1.75%	0.263%
14	8.185	2118	2129	2143	rBV	26556	45273	8.42%	1.262%
15	8.645	2258	2272	2309	rBV	256553	537873	100.00%	14.992%
16	8.796	2309	2319	2336	rVB4	7121	15191	2.82%	0.423%
17	9.420	2500	2513	2536	rBV	231223	390929	72.68%	10.897%
18	10.761	2916	2930	2948	rVB	82953	130707	24.30%	3.643%
19	11.815	3245	3258	3278	rBV	218468	349455	64.97%	9.741%
20	12.198	3365	3377	3398	rBV	162458	263697	49.03%	7.350%


Sum of corrected areas: 3587649

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044765.D
Acq On : 22 Sep 2021 17:51
Operator : SY/MD
Sample : M3814-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB6X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

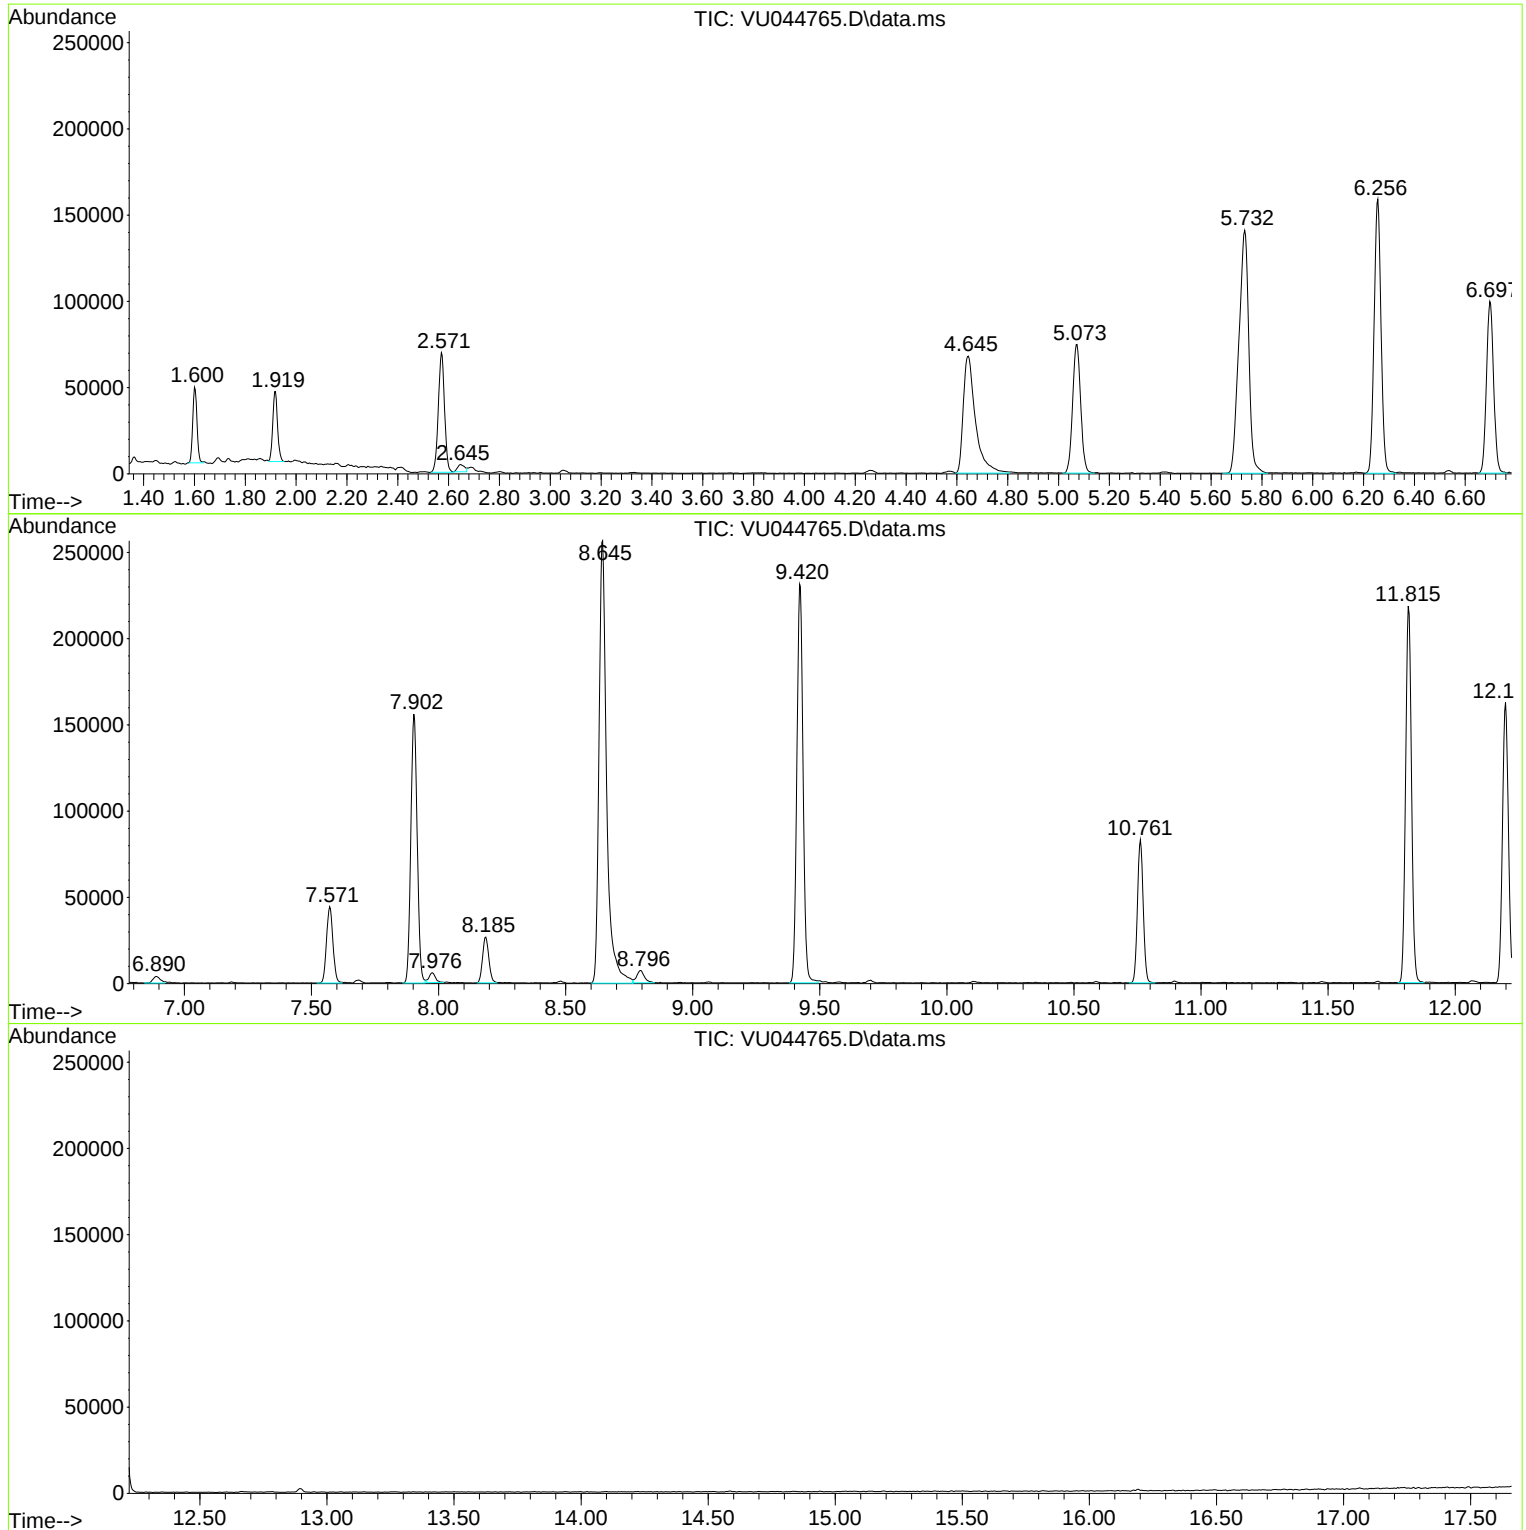

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044765.D
Acq On : 22 Sep 2021 17:51
Operator : SY/MD
Sample : M3814-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB6X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044765.D
Acq On : 22 Sep 2021 17:51
Operator : SY/MD
Sample : M3814-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB6X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
