
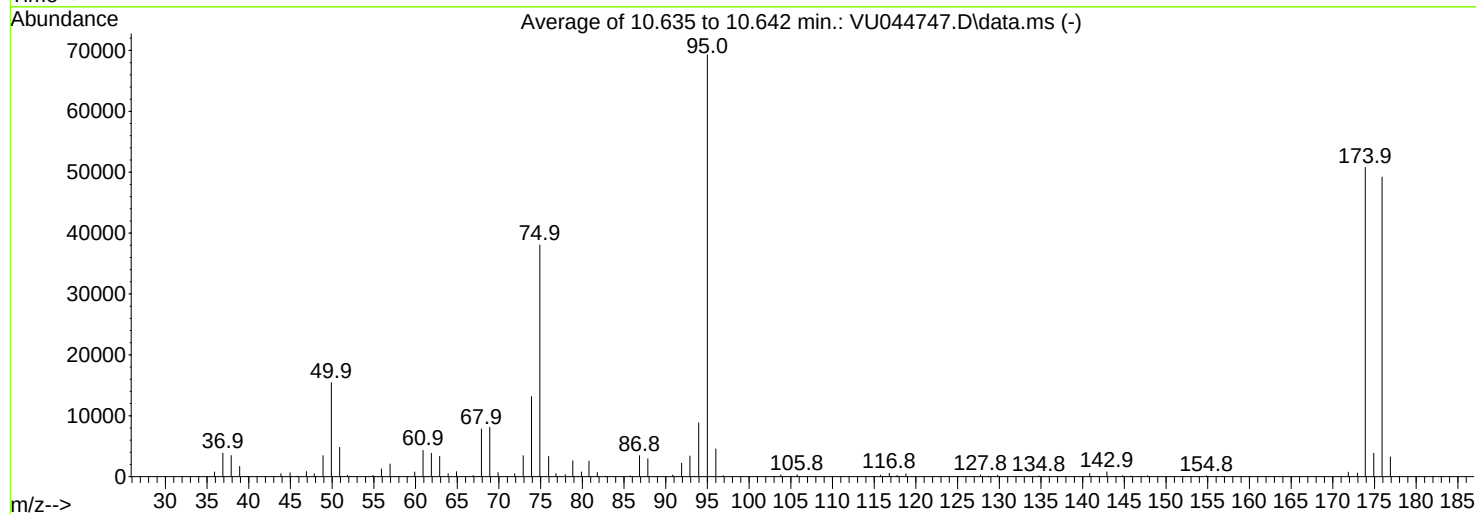


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092221\
Data File : VU044747.D
Acq On : 22 Sep 2021 09:10
Operator : SY/MD
Sample : BFB023
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB023

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Sep 23 02:59:45 2021

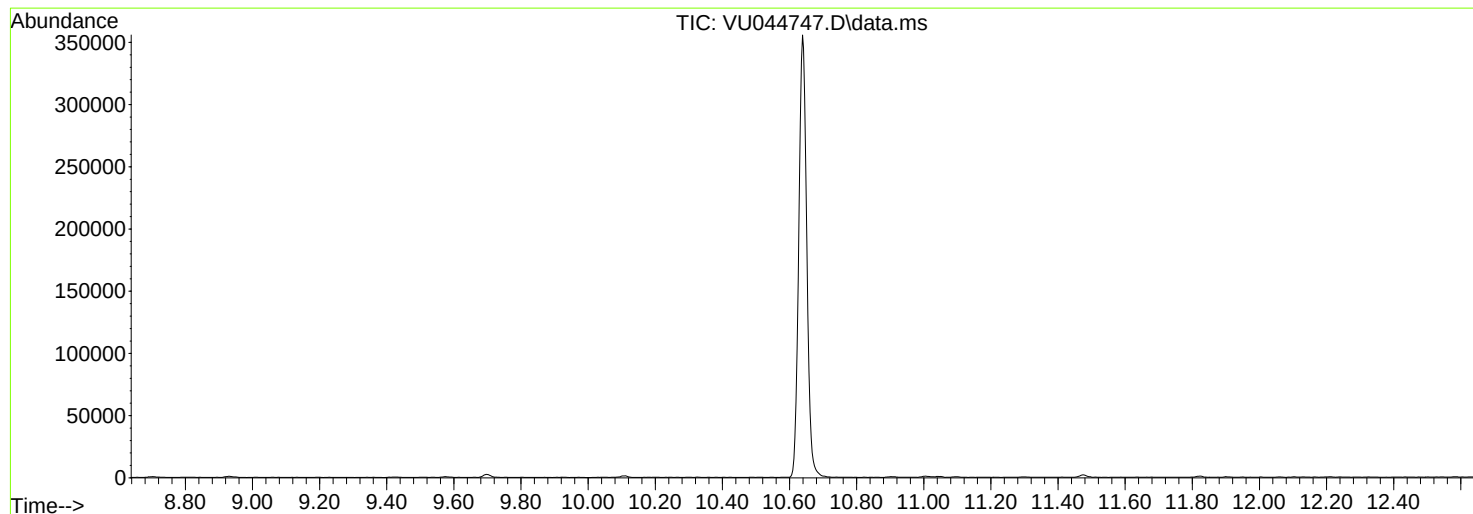

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	15436	PASS
75	95	30	80	54.9	38061	PASS
95	95	100	100	100.0	69280	PASS
96	95	5	9	6.6	4546	PASS
173	174	0.00	2	1.2	592	PASS
174	95	50	120	73.3	50797	PASS
175	174	5	9	7.6	3837	PASS
176	174	95	101	96.9	49197	PASS
177	176	5	9	6.6	3246	PASS

m/z	Abundance
39.80	178.0
43.80	344.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
35.90	737.0
36.90	3912.0
37.90	3454.0
38.90	1683.0
39.90	193.0
43.90	807.0
44.90	635.0
46.90	801.0
47.80	454.0
48.90	3455.0
49.90	15069.0
50.90	4667.0
51.90	234.0
52.90	103.0
54.90	227.0
55.90	1275.0
56.90	2132.0
59.90	730.0
60.90	4316.0
61.90	3706.0
62.90	3212.0
63.90	494.0
64.90	822.0
66.90	189.0
67.90	7569.0
68.90	7974.0
69.90	656.0
71.90	456.0
72.90	3375.0
73.90	12774.0
74.90	37152.0
75.90	3373.0
76.90	453.0
77.90	340.0
78.80	2636.0
79.90	747.0
80.80	2476.0
81.80	742.0
82.80	108.0
85.70	115.0
86.90	3245.0
87.80	2840.0
90.80	279.0
91.90	2186.0
92.90	3334.0
93.90	8709.0
95.00	67024.0
96.00	4486.0
96.90	161.0
103.80	290.0
105.70	307.0
115.70	204.0
116.80	578.0
117.80	206.0
118.80	379.0
127.70	260.0
128.70	128.0
129.80	224.0
134.70	133.0
140.80	544.0
142.90	761.0
144.80	197.0
145.80	114.0
147.80	148.0
154.90	156.0
171.90	678.0
173.00	588.0
173.90	48248.0
174.90	3724.0
175.90	47000.0
176.90	3225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
35.90	814.0
36.90	3966.0
37.90	3595.0
38.90	1754.0
39.80	198.0
43.90	861.0
45.00	660.0
45.80	112.0
46.90	876.0
47.80	481.0
48.90	3551.0
49.90	15777.0
50.90	4935.0
51.90	249.0
54.90	229.0
55.90	1315.0
56.90	2106.0
59.90	789.0
60.90	4495.0
61.90	3949.0
62.90	3483.0
63.90	526.0
64.90	834.0
66.90	168.0
67.90	8092.0
68.90	8377.0
69.90	717.0
71.90	492.0
72.90	3560.0
73.90	13591.0
74.90	39200.0
76.00	3381.0
76.90	507.0
77.90	328.0
78.80	2675.0
79.90	785.0
80.80	2611.0
81.80	720.0
82.80	111.0
85.80	125.0
86.90	3625.0
87.80	3039.0
90.80	284.0
91.90	2303.0
92.90	3496.0
94.00	9097.0
95.00	71256.0
96.00	4703.0
96.90	168.0
103.80	300.0
105.70	340.0
115.80	241.0
116.80	582.0
117.80	213.0
118.80	466.0
127.80	264.0
128.70	103.0
129.80	248.0
134.80	137.0
140.80	549.0
142.90	814.0
144.80	185.0
145.80	120.0
147.80	174.0
154.80	152.0
156.80	102.0
171.90	747.0
173.00	593.0
173.90	52368.0
174.90	3989.0
175.90	50856.0
176.90	3373.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
35.90	786.0
36.90	3709.0
37.90	3349.0
38.90	1622.0
39.80	206.0
43.90	890.0
45.00	645.0
45.80	134.0
46.90	881.0
47.90	469.0
48.90	3330.0
49.90	15461.0
50.90	4801.0
51.80	230.0
54.90	211.0
55.90	1196.0
57.00	2011.0
59.90	759.0
60.90	4126.0
61.90	3899.0
62.90	3324.0
63.90	502.0
64.90	797.0
66.90	180.0
67.90	7874.0
68.90	7963.0
69.90	693.0
71.90	474.0
72.90	3430.0
73.90	13088.0
74.90	37832.0
76.00	3158.0
76.80	549.0
78.00	333.0
78.90	2505.0
79.90	751.0
80.80	2538.0
81.80	594.0
85.80	168.0
86.80	3495.0
87.90	2944.0
90.90	254.0
91.90	2153.0
92.90	3334.0
94.00	8707.0
95.00	69560.0
96.00	4448.0
96.90	147.0
103.80	307.0
104.80	117.0
105.80	338.0
115.80	258.0
116.80	535.0
117.70	219.0
118.80	526.0
127.80	254.0
129.80	254.0
134.80	120.0
136.90	107.0
140.90	525.0
142.90	775.0
144.80	179.0
145.80	106.0
147.80	168.0
154.80	121.0
156.80	108.0
171.80	805.0
172.90	594.0
173.90	51776.0
174.90	3798.0
175.90	49736.0
176.90	3139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023