

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050891.D
 Acq On : 22 Sep 2022 12:09
 Operator : JC/MD
 Sample : N4650-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ06

Quant Time: Sep 23 01:09:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 23 01:08:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	402847	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	388107	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	141929	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	155877	37.347	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.700%		
7) Chloroethane-d5	1.903	69	136138	45.799	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.600%		
11) 1,1-Dichloroethene-d2	2.562	63	207405	31.936	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.880%		
21) 2-Butanone-d5	4.620	46	315574	117.115	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	117.110%		
24) Chloroform-d	5.060	84	309949	47.387	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.780%		
26) 1,2-Dichloroethane-d4	5.700	65	200085	49.637	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.280%		
32) Benzene-d6	5.726	84	596041	46.626	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.260%		
36) 1,2-Dichloropropane-d6	6.690	67	210579	48.802	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.600%		
41) Toluene-d8	7.896	98	474643	42.476	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.960%		
43) trans-1,3-Dichloroprop...	8.179	79	81850	43.604	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.200%		
47) 2-Hexanone-d5	8.632	63	184263	103.623	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	103.620%		
56) 1,1,2,2-Tetrachloroeth...	10.755	84	316766	48.151	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.300%		
66) 1,2-Dichlorobenzene-d4	12.192	152	158124	53.211	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.420%		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.575	96	15794	5.100	ug/L	# 1
19) 1,1-Dichloroethane	3.867	63	47454	7.399	ug/L	98
20) cis-1,2-Dichloroethene	4.665	96	12440	3.535	ug/L	92
30) 1,1,1-Trichloroethane	5.317	97	90676	17.562	ug/L	99
46) Tetrachloroethene	8.555	164	8246	3.459	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050891.D
Acq On : 22 Sep 2022 12:09
Operator : JC/MD
Sample : N4650-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ06

Quant Time: Sep 23 01:09:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 23 01:08:30 2022
Response via : Initial Calibration




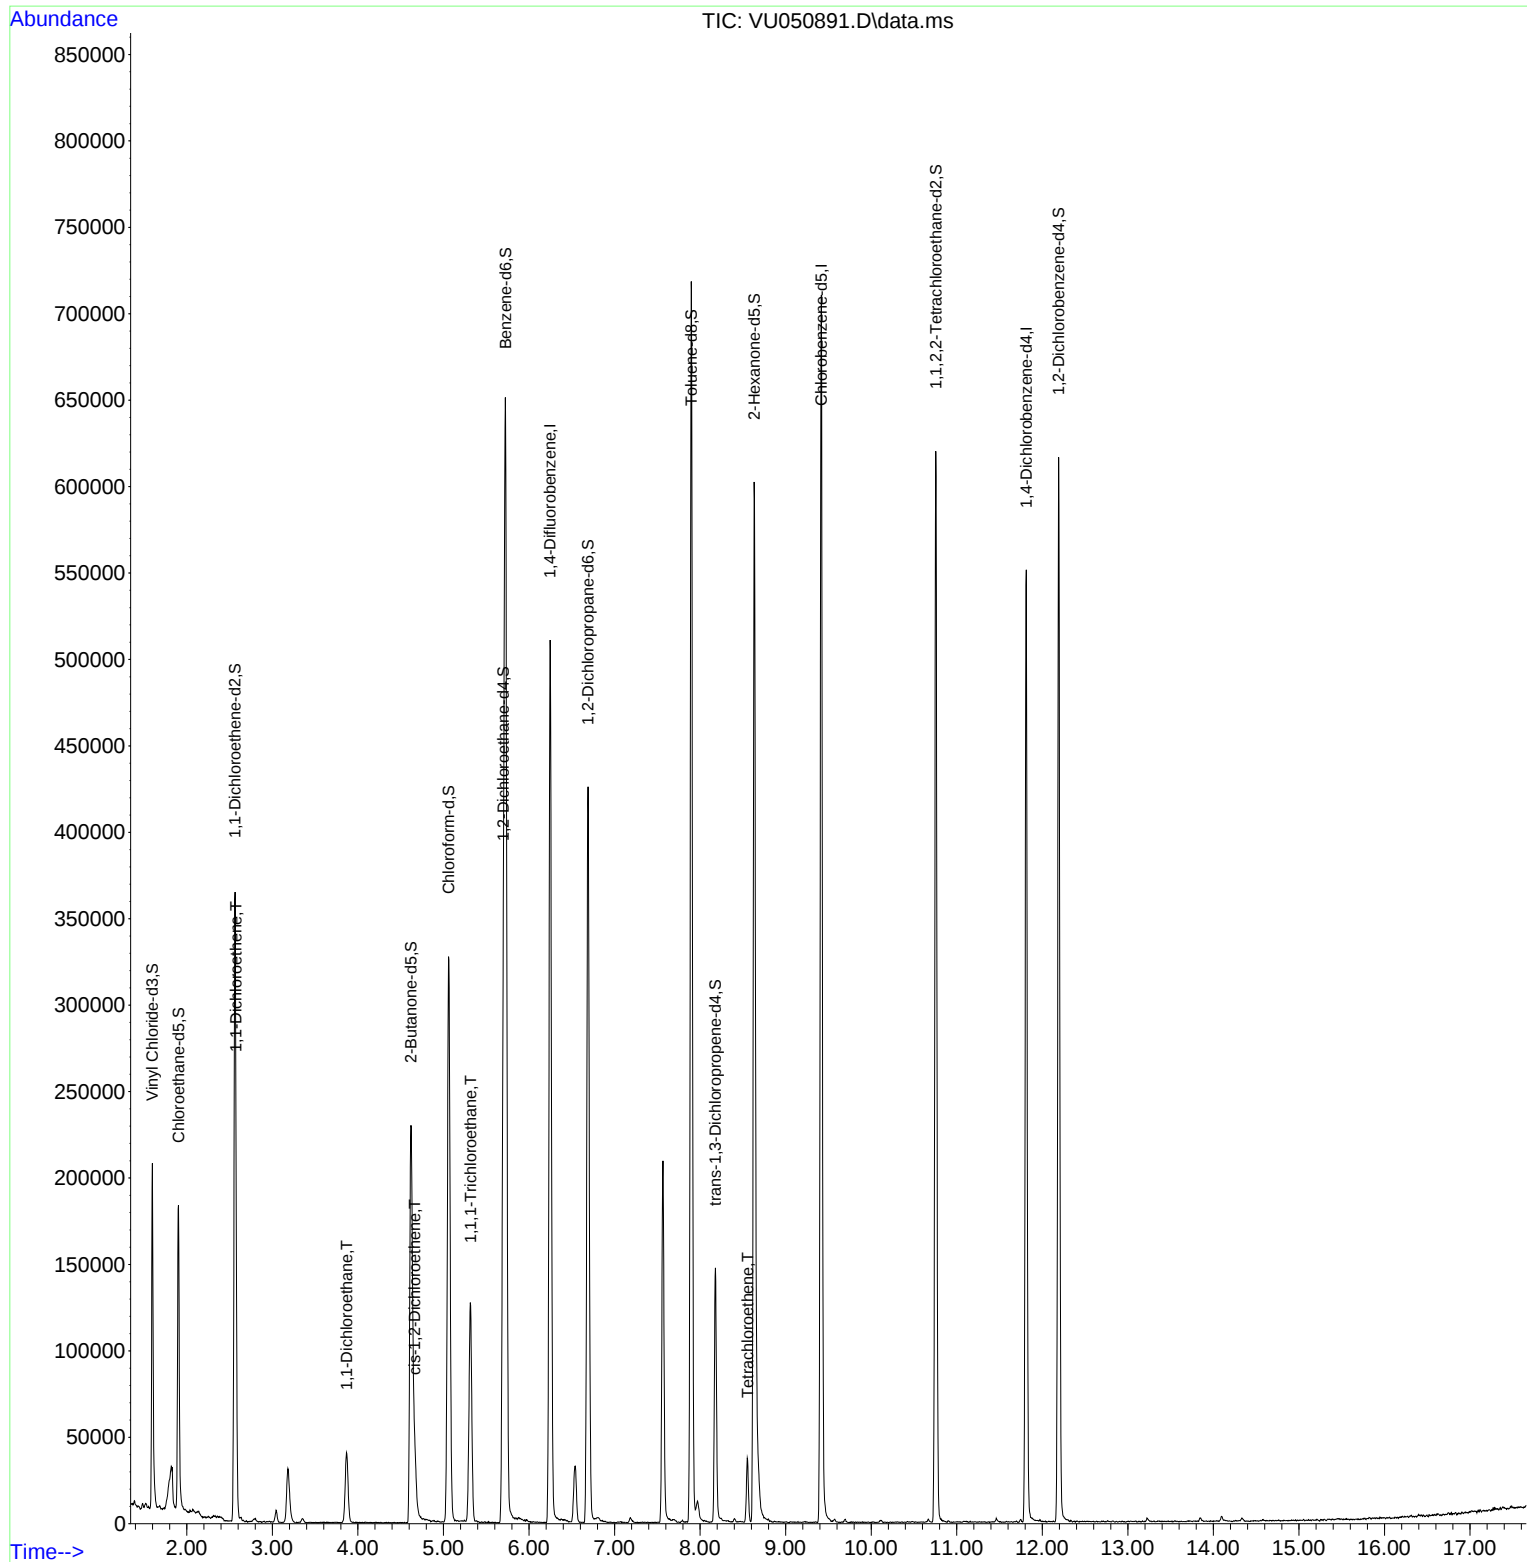


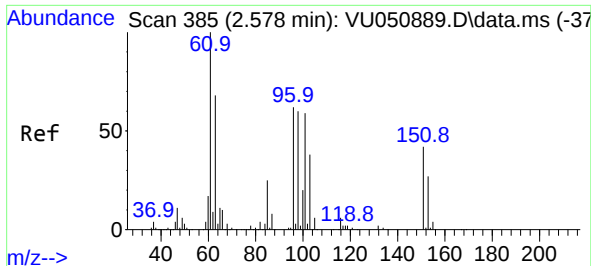

#12
1,1-Dichloroethene
Concen: 5.100 ug/L
RT: 2.575 min Scan# 385
Delta R.T. -0.003 min
Lab File: VU050891.D
Acq: 22 Sep 2022 12:09




Instrument :
MSVOA_U
ClientSampleId :
EXZ06


Tgt Ion: 96 Resp: 15794
Ion Ratio Lower Upper
96 100
61 242.6 118.6 220.2#
63 749.2 90.4 168.0#

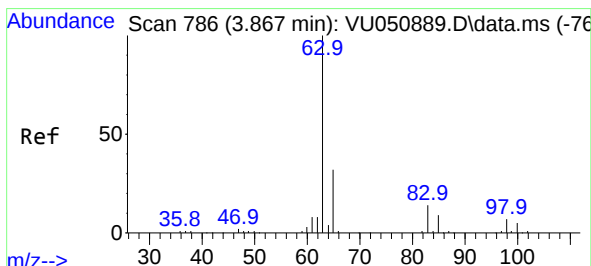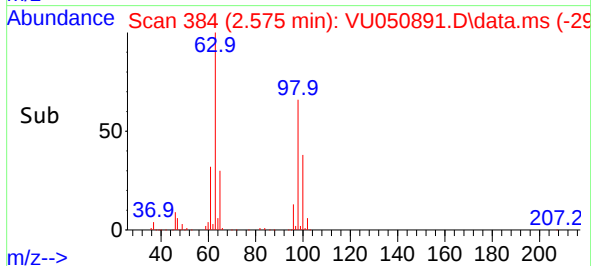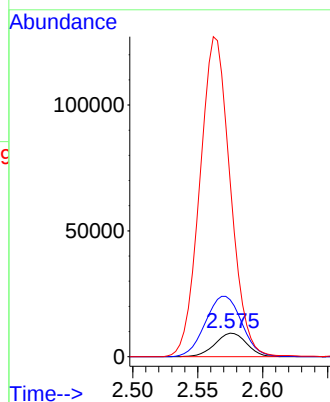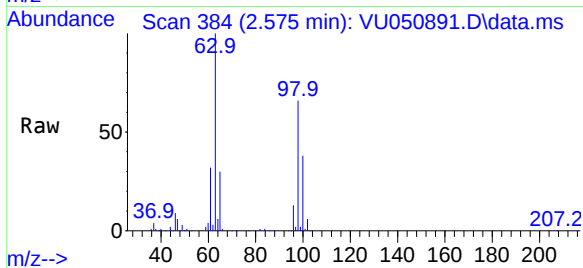

#19
1,1-Dichloroethane
Concen: 7.399 ug/L
RT: 3.867 min Scan# 786
Delta R.T. 0.000 min
Lab File: VU050891.D
Acq: 22 Sep 2022 12:09

Tgt Ion: 63 Resp: 47454
Ion Ratio Lower Upper
63 100
65 31.0 21.5 39.9
83 11.8 9.3 17.3


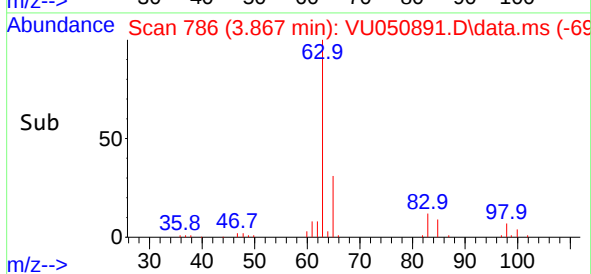
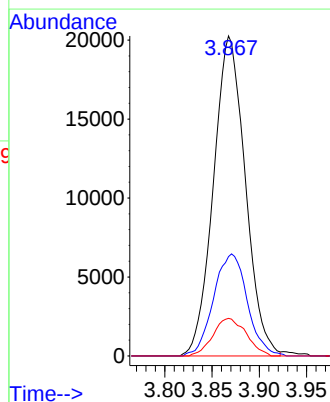
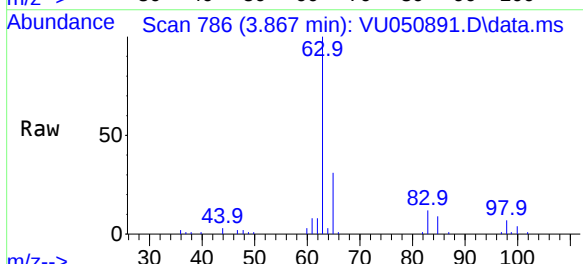


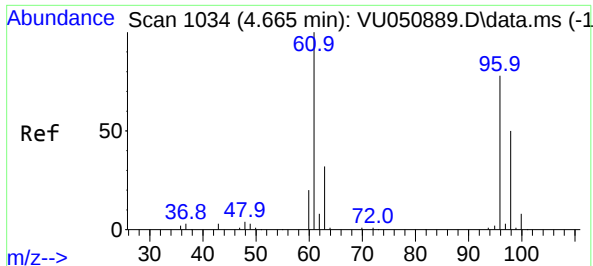

#20
 cis-1,2-Dichloroethene
 Concen: 3.535 ug/L
 RT: 4.665 min Scan# 1034
 Delta R.T. 0.000 min
 Lab File: VU050891.D
 Acq: 22 Sep 2022 12:09




Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ06


Tgt Ion: 96 Resp: 12440
 Ion Ratio Lower Upper
 96 100
 61 137.8 90.1 167.3
 68 0.0 0.0 0.0

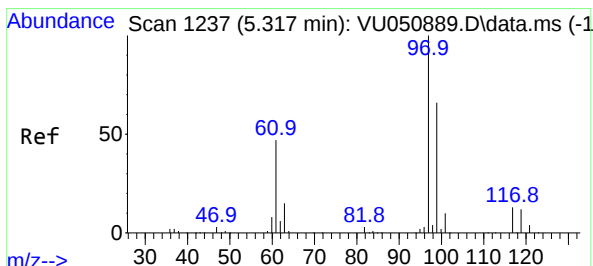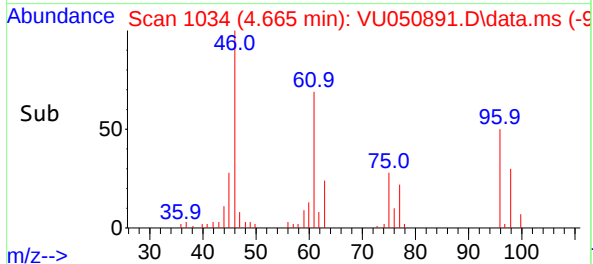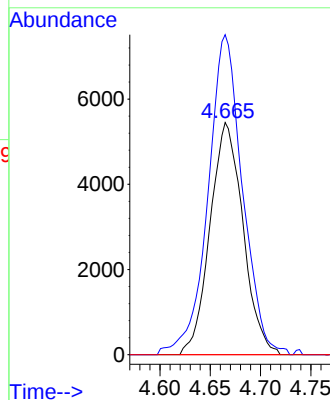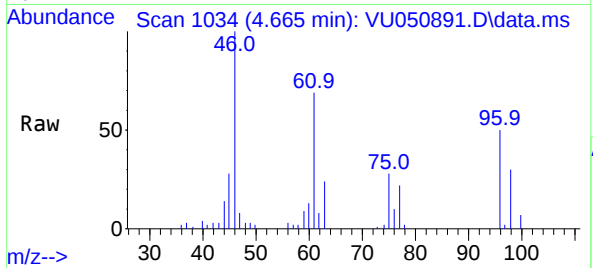

#30
 1,1,1-Trichloroethane
 Concen: 17.562 ug/L
 RT: 5.317 min Scan# 1237
 Delta R.T. 0.000 min
 Lab File: VU050891.D
 Acq: 22 Sep 2022 12:09

Tgt Ion: 97 Resp: 90676
 Ion Ratio Lower Upper
 97 100
 99 64.7 52.2 78.2
 61 45.7 37.1 55.7

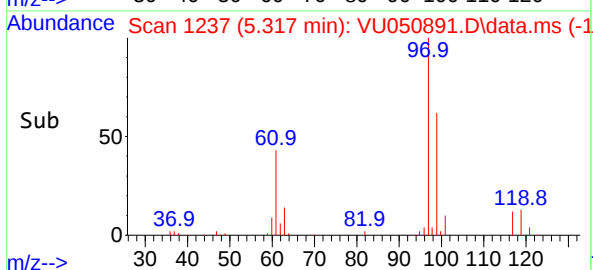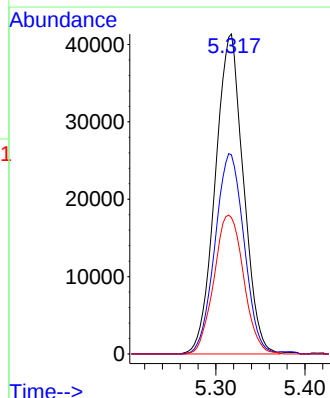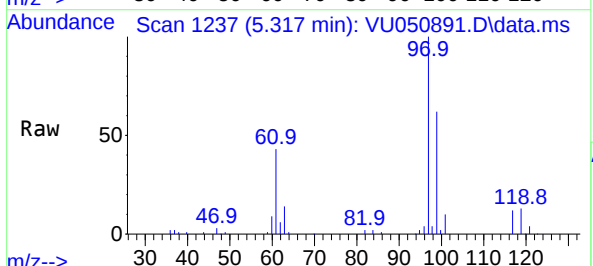

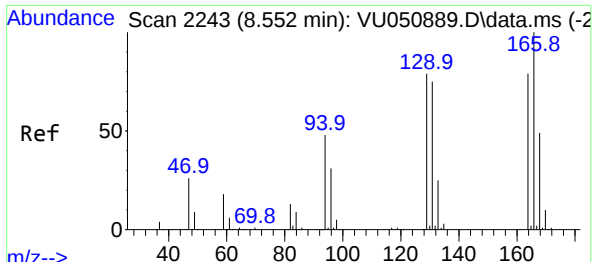

#46
Tetrachloroethene
Concen: 3.459 ug/L
RT: 8.555 min Scan# 21
Delta R.T. 0.003 min
Lab File: VU050891.D
Acq: 22 Sep 2022 12:09

Instrument :
MSVOA_U
ClientSampleId :
EXZ06

Tgt Ion:164 Resp: 8246

Ion	Ratio	Lower	Upper
164	100		
129	90.6	68.5	127.3
131	87.0	66.1	122.7
166	124.3	88.8	164.8

