

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050894.D
 Acq On : 22 Sep 2022 13:41
 Operator : JC/MD
 Sample : VIBLK136
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	199136	229893	12.55%	1.685%
2	1.909	170	177	193	rVB	176451	233556	12.75%	1.712%
3	2.565	370	381	396	rBV	321476	523989	28.60%	3.841%
4	3.044	521	530	543	rVB4	8107	14771	0.81%	0.108%
5	3.182	560	573	589	rVB	12446	26427	1.44%	0.194%
6	3.276	600	602	604	rBV	201	135	0.01%	0.001%
7	3.465	659	661	663	rBV2	229	109	0.01%	0.001%
8	3.555	683	689	692	rBV2	378	468	0.03%	0.003%
9	3.684	724	729	732	rBV3	426	394	0.02%	0.003%
10	3.793	758	763	765	rBV2	378	379	0.02%	0.003%
11	3.867	782	786	794	rVB3	722	763	0.04%	0.006%
12	4.002	825	828	831	rVB3	341	199	0.01%	0.001%
13	4.022	831	834	836	rBV	297	188	0.01%	0.001%
14	4.080	848	852	858	rBV3	436	628	0.03%	0.005%
15	4.115	861	863	865	rBV2	160	98	0.01%	0.001%
16	4.160	874	877	878	rBV	169	92	0.01%	0.001%
17	4.266	908	910	920	rVB3	455	496	0.03%	0.004%
18	4.308	920	923	926	rBV2	299	233	0.01%	0.002%
19	4.337	926	932	935	rVV4	589	657	0.04%	0.005%
20	4.356	935	938	943	rVB2	498	346	0.02%	0.003%
21	4.414	954	956	965	rVB2	337	352	0.02%	0.003%
22	4.526	989	991	994	rVB	259	114	0.01%	0.001%
23	4.549	994	998	1003	rBV	313	363	0.02%	0.003%
24	4.616	1005	1019	1052	rBV	241877	594816	32.46%	4.360%
25	4.986	1132	1134	1137	rBV2	470	270	0.01%	0.002%
26	5.063	1141	1158	1185	rVV	337716	742118	40.50%	5.440%
27	5.446	1271	1277	1287	rBV4	411	595	0.03%	0.004%
28	5.530	1298	1303	1308	rVB2	417	475	0.03%	0.003%
29	5.565	1312	1314	1315	rBV2	213	94	0.01%	0.001%
30	5.620	1326	1331	1335	rBV3	376	434	0.02%	0.003%
31	5.639	1335	1337	1342	rVB2	287	181	0.01%	0.001%
32	5.726	1342	1364	1393	rBV2	656531	1832242	100.00%	13.430%
33	6.028	1456	1458	1460	rBV2	494	290	0.02%	0.002%
34	6.176	1499	1504	1511	rBV4	410	569	0.03%	0.004%
35	6.250	1511	1527	1548	rBV	514880	984957	53.76%	7.220%
36	6.530	1603	1614	1631	rVB3	16756	34169	1.86%	0.250%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050894.D
 Acq On : 22 Sep 2022 13:41
 Operator : JC/MD
 Sample : VIBLK136
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.591	1631	1633	1635	rBV	235	94	0.01%	0.001%
38	6.620	1640	1642	1647	rVB2	331	219	0.01%	0.002%
39	6.690	1647	1664	1683	rBV	448932	872833	47.64%	6.398%
40	6.906	1728	1731	1734	rBV4	495	298	0.02%	0.002%
41	6.951	1742	1745	1746	rBV2	162	90	0.00%	0.001%
42	6.960	1746	1748	1753	rVB2	479	363	0.02%	0.003%
43	6.983	1753	1755	1756	rBV	430	178	0.01%	0.001%
44	7.031	1768	1770	1771	rBV	469	162	0.01%	0.001%
45	7.105	1788	1793	1796	rBV3	446	354	0.02%	0.003%
46	7.185	1810	1818	1820	rBV4	1968	2293	0.13%	0.017%
47	7.234	1831	1833	1836	rVB	173	96	0.01%	0.001%
48	7.263	1839	1842	1845	rBV2	270	142	0.01%	0.001%
49	7.292	1848	1851	1852	rBV	259	153	0.01%	0.001%
50	7.398	1882	1884	1885	rBV	283	129	0.01%	0.001%
51	7.497	1912	1915	1917	rVB2	252	153	0.01%	0.001%
52	7.513	1917	1920	1923	rBV2	210	149	0.01%	0.001%
53	7.565	1923	1936	1954	rBV	222963	397072	21.67%	2.911%
54	7.800	2000	2009	2017	rVB5	2838	4821	0.26%	0.035%
55	7.899	2026	2040	2056	rBV	740733	1258492	68.69%	9.225%
56	8.179	2116	2127	2145	rBV2	156057	267850	14.62%	1.963%
57	8.449	2208	2211	2212	rBV2	410	241	0.01%	0.002%
58	8.555	2238	2244	2255	rVB8	1650	2195	0.12%	0.016%
59	8.632	2255	2268	2305	rBV2	621956	1214618	66.29%	8.903%
60	8.999	2377	2382	2383	rBV3	649	533	0.03%	0.004%
61	9.066	2401	2403	2407	rBV3	203	147	0.01%	0.001%
62	9.128	2420	2422	2424	rBV	191	109	0.01%	0.001%
63	9.211	2445	2448	2450	rBV	340	165	0.01%	0.001%
64	9.234	2452	2455	2457	rBV2	332	249	0.01%	0.002%
65	9.279	2466	2469	2472	rBV2	380	278	0.02%	0.002%
66	9.333	2483	2486	2489	rBV2	361	202	0.01%	0.001%
67	9.372	2494	2498	2499	rBV	212	140	0.01%	0.001%
68	9.417	2499	2512	2542	rBV	735518	1214214	66.27%	8.900%
69	9.700	2589	2600	2608	rVB3	2569	3859	0.21%	0.028%
70	9.732	2608	2610	2612	rVB	260	122	0.01%	0.001%
71	9.783	2623	2626	2631	rVB2	608	412	0.02%	0.003%
72	9.845	2640	2645	2646	rBV	292	273	0.01%	0.002%
73	9.906	2662	2664	2670	rVV3	289	227	0.01%	0.002%
74	10.021	2695	2700	2706	rBV3	588	732	0.04%	0.005%
75	10.105	2719	2726	2728	rBV3	2914	2908	0.16%	0.021%
76	10.201	2753	2756	2758	rBV2	229	177	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050894.D
 Acq On : 22 Sep 2022 13:41
 Operator : JC/MD
 Sample : VIBLK136
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK136

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	10.221	2758	2762	2765	rVB	414	340	0.02%	0.002%
78	10.259	2772	2774	2776	rVB2	224	94	0.01%	0.001%
79	10.275	2776	2779	2782	rBV2	243	170	0.01%	0.001%
80	10.295	2782	2785	2788	rBV3	489	301	0.02%	0.002%
81	10.340	2798	2799	2804	rBV2	209	151	0.01%	0.001%
82	10.491	2838	2846	2852	rVB5	1791	2506	0.14%	0.018%
83	10.539	2859	2861	2867	rBV2	313	228	0.01%	0.002%
84	10.671	2894	2902	2908	rBV4	1695	2489	0.14%	0.018%
85	10.754	2916	2928	2946	rBV	659551	1060340	57.87%	7.772%
86	10.915	2976	2978	2983	rVB2	593	353	0.02%	0.003%
87	10.944	2985	2987	2991	rBV	358	298	0.02%	0.002%
88	11.214	3068	3071	3074	rBV3	566	357	0.02%	0.003%
89	11.471	3141	3151	3158	rBV5	3807	5558	0.30%	0.041%
90	11.581	3183	3185	3188	rBV3	432	293	0.02%	0.002%
91	11.748	3230	3237	3244	rVB5	4968	6912	0.38%	0.051%
92	11.812	3244	3257	3284	rBV	580007	933464	50.95%	6.842%
93	12.118	3349	3352	3355	rVB3	697	361	0.02%	0.003%
94	12.192	3362	3375	3399	rBV	639688	1062464	57.99%	7.788%
95	12.777	3555	3557	3560	rBV3	462	275	0.02%	0.002%
96	13.092	3652	3655	3658	rBV3	623	495	0.03%	0.004%
97	13.221	3689	3695	3707	rVB4	6549	10203	0.56%	0.075%
98	13.844	3882	3889	3899	rVB3	11706	18219	0.99%	0.134%
99	14.089	3957	3965	3976	rBV2	24362	38342	2.09%	0.281%
100	14.333	4033	4041	4054	rVB3	14899	24609	1.34%	0.180%




Sum of corrected areas: 13642424

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050894.D
Acq On : 22 Sep 2022 13:41
Operator : JC/MD
Sample : VIBLK136
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK136

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

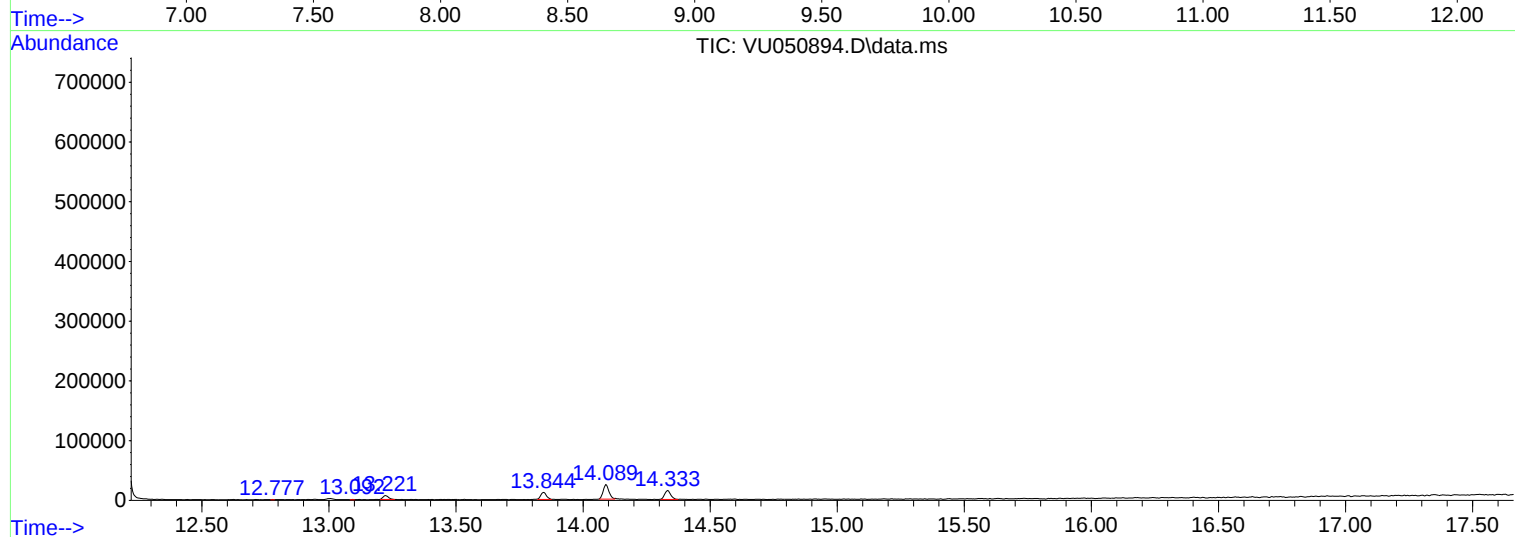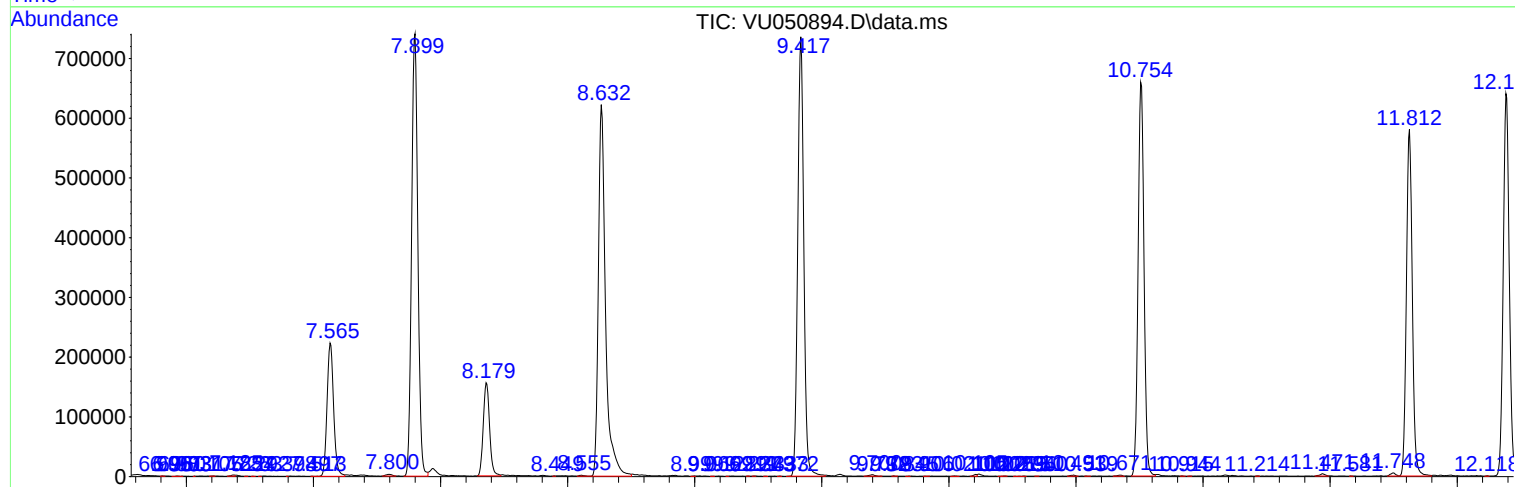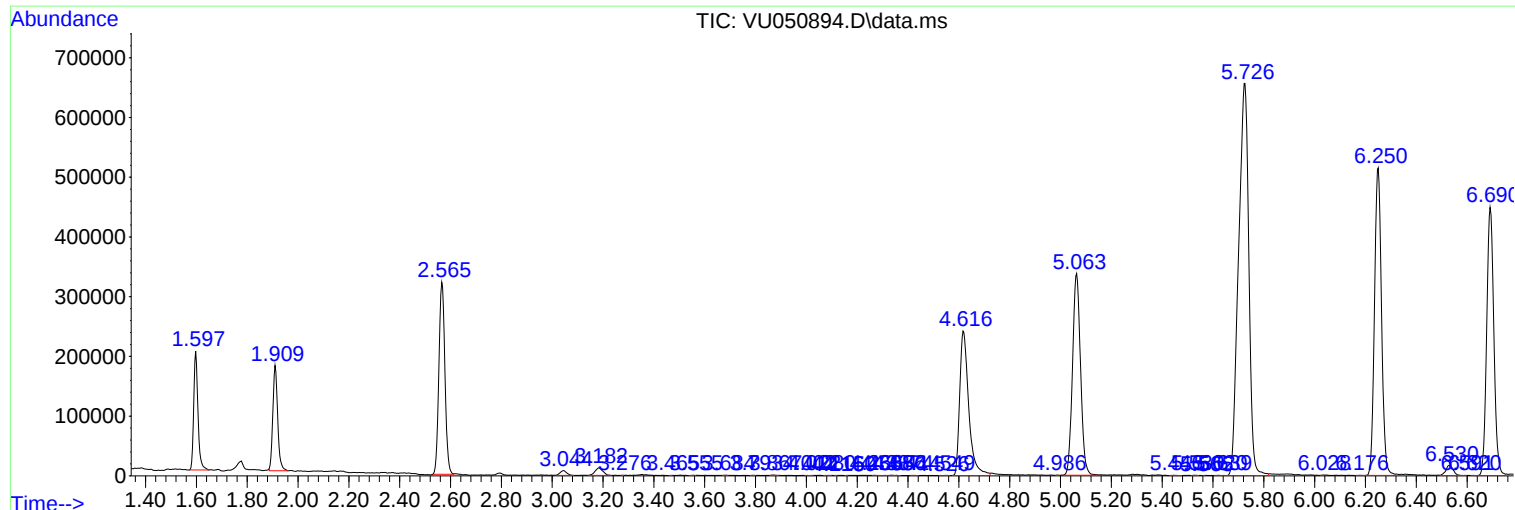

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050894.D
Acq On : 22 Sep 2022 13:41
Operator : JC/MD
Sample : VIBLK136
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK136

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050894.D
Acq On : 22 Sep 2022 13:41
Operator : JC/MD
Sample : VIBLK136
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK136

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------