

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050896.D
 Acq On : 22 Sep 2022 14:30
 Operator : JC/MD
 Sample : N4748-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050896.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	102	rVB	199884	250620	14.59%	1.949%
2	1.909	169	177	200	rVB	195298	262265	15.26%	2.040%
3	2.279	289	292	296	rBV5	1417	1395	0.08%	0.011%
4	2.565	368	381	397	rBV	332070	549148	31.96%	4.271%
5	2.777	442	447	448	rBV2	1057	782	0.05%	0.006%
6	2.890	480	482	487	rVB3	581	356	0.02%	0.003%
7	2.919	487	491	493	rBV2	470	301	0.02%	0.002%
8	2.951	497	501	504	rBV2	549	492	0.03%	0.004%
9	3.041	519	529	530	rBV3	1844	1925	0.11%	0.015%
10	3.160	563	566	569	rBV3	427	249	0.01%	0.002%
11	3.179	569	572	573	rBV	397	260	0.02%	0.002%
12	3.285	603	605	609	rVB	393	254	0.01%	0.002%
13	3.324	609	617	622	rBV3	582	937	0.05%	0.007%
14	3.353	622	626	627	rBV2	865	527	0.03%	0.004%
15	3.472	660	663	666	rVB2	510	359	0.02%	0.003%
16	3.497	666	671	675	rVB	532	471	0.03%	0.004%
17	3.530	675	681	684	rBV	504	578	0.03%	0.004%
18	3.584	694	698	700	rVV2	560	517	0.03%	0.004%
19	3.681	726	728	732	rVB2	442	334	0.02%	0.003%
20	3.706	732	736	740	rBV2	423	399	0.02%	0.003%
21	3.819	769	771	774	rBV	363	260	0.02%	0.002%
22	3.977	815	820	823	rBV	298	326	0.02%	0.003%
23	4.214	890	894	899	rVB3	314	321	0.02%	0.002%
24	4.456	964	969	971	rBV2	440	456	0.03%	0.004%
25	4.626	1008	1022	1060	rBV	206796	551841	32.12%	4.292%
26	5.063	1141	1158	1182	rBV	322424	707021	41.15%	5.499%
27	5.375	1249	1255	1260	rBV4	587	721	0.04%	0.006%
28	5.597	1319	1324	1329	rBV3	473	548	0.03%	0.004%
29	5.726	1341	1364	1392	rBV2	622113	1718100	100.00%	13.362%
30	6.102	1479	1481	1484	rBV	342	253	0.01%	0.002%
31	6.150	1492	1496	1502	rVB3	426	393	0.02%	0.003%
32	6.247	1511	1526	1549	rBV	521450	994491	57.88%	7.734%
33	6.472	1593	1596	1598	rBV2	346	256	0.01%	0.002%
34	6.529	1603	1614	1626	rVB3	13051	25002	1.46%	0.194%
35	6.578	1626	1629	1632	rBV3	635	393	0.02%	0.003%
36	6.610	1635	1639	1641	rVB2	543	359	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050896.D
 Acq On : 22 Sep 2022 14:30
 Operator : JC/MD
 Sample : N4748-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1682	rBV	423438	817032	47.55%	6.354%
38	6.902	1727	1730	1734	rVB3	991	635	0.04%	0.005%
39	6.960	1742	1748	1752	rVB2	461	393	0.02%	0.003%
40	7.009	1759	1763	1766	rBV	272	268	0.02%	0.002%
41	7.037	1769	1772	1780	rVV4	400	540	0.03%	0.004%
42	7.105	1788	1793	1796	rBV4	557	529	0.03%	0.004%
43	7.195	1811	1821	1829	rBV7	2219	4336	0.25%	0.034%
44	7.230	1830	1832	1837	rVV2	445	466	0.03%	0.004%
45	7.253	1837	1839	1843	rVB2	520	272	0.02%	0.002%
46	7.314	1855	1858	1862	rVB2	308	256	0.01%	0.002%
47	7.353	1867	1870	1876	rVB2	234	247	0.01%	0.002%
48	7.565	1921	1936	1956	rBV	199837	357816	20.83%	2.783%
49	7.735	1987	1989	1995	rVB3	632	438	0.03%	0.003%
50	7.790	1999	2006	2007	rBV2	769	574	0.03%	0.004%
51	7.803	2007	2010	2013	rVB3	987	650	0.04%	0.005%
52	7.896	2026	2039	2055	rBV	686469	1186412	69.05%	9.227%
53	8.179	2114	2127	2145	rBV2	141363	244653	14.24%	1.903%
54	8.513	2228	2231	2234	rBV2	467	297	0.02%	0.002%
55	8.555	2236	2244	2250	rVV5	2576	3245	0.19%	0.025%
56	8.635	2255	2269	2303	rBV2	582037	1158590	67.43%	9.011%
57	8.851	2333	2336	2338	rBV2	431	289	0.02%	0.002%
58	9.156	2429	2431	2439	rVB4	419	473	0.03%	0.004%
59	9.221	2447	2451	2453	rBV2	364	262	0.02%	0.002%
60	9.417	2498	2512	2546	rBV	722505	1198076	69.73%	9.318%
61	9.639	2578	2581	2584	rVB3	461	287	0.02%	0.002%
62	9.693	2592	2598	2600	rBV3	1481	1518	0.09%	0.012%
63	9.735	2609	2611	2617	rVB2	609	407	0.02%	0.003%
64	9.774	2621	2623	2628	rVV3	348	244	0.01%	0.002%
65	9.902	2658	2663	2667	rBV	258	265	0.02%	0.002%
66	10.037	2702	2705	2711	rVB2	445	361	0.02%	0.003%
67	10.108	2717	2727	2729	rBV3	1089	1304	0.08%	0.010%
68	10.259	2772	2774	2777	rBV2	300	259	0.02%	0.002%
69	10.481	2838	2843	2844	rBV2	759	521	0.03%	0.004%
70	10.664	2896	2900	2903	rVV	713	624	0.04%	0.005%
71	10.754	2916	2928	2949	rBV	624718	989037	57.57%	7.692%
72	10.889	2966	2970	2973	rVV2	858	598	0.03%	0.005%
73	10.970	2988	2995	3000	rBV2	384	434	0.03%	0.003%
74	10.999	3000	3004	3006	rBV2	477	358	0.02%	0.003%
75	11.086	3027	3031	3033	rBV3	561	449	0.03%	0.003%
76	11.102	3034	3036	3039	rVB3	667	443	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050896.D
 Acq On : 22 Sep 2022 14:30
 Operator : JC/MD
 Sample : N4748-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.375	3112	3121	3123	rBV3	689	906	0.05%	0.007%
78	11.465	3141	3149	3150	rBV5	1468	1385	0.08%	0.011%
79	11.513	3161	3164	3168	rBV2	497	396	0.02%	0.003%
80	11.648	3202	3206	3209	rBV2	294	267	0.02%	0.002%
81	11.693	3215	3220	3226	rVB3	692	839	0.05%	0.007%
82	11.745	3230	3236	3242	rBV5	1498	1909	0.11%	0.015%
83	11.812	3244	3257	3275	rBV	528228	850321	49.49%	6.613%
84	12.079	3333	3340	3346	rVB5	788	1115	0.06%	0.009%
85	12.192	3360	3375	3395	rBV	572194	935511	54.45%	7.276%
86	12.442	3449	3453	3457	rBV2	754	564	0.03%	0.004%
87	12.478	3461	3464	3468	rVB3	563	366	0.02%	0.003%
88	12.770	3552	3555	3559	rVB2	565	352	0.02%	0.003%
89	13.166	3672	3678	3683	rBV3	647	814	0.05%	0.006%
90	13.192	3683	3686	3690	rBV3	371	305	0.02%	0.002%
91	13.217	3690	3694	3695	rBV3	1072	749	0.04%	0.006%
92	13.532	3786	3792	3797	rBV3	619	763	0.04%	0.006%
93	13.674	3834	3836	3840	rVB	487	316	0.02%	0.002%
94	13.848	3884	3890	3900	rVB6	2157	2984	0.17%	0.023%
95	14.092	3964	3966	3981	rVB6	3422	5067	0.29%	0.039%
96	14.214	4001	4004	4007	rBV	616	467	0.03%	0.004%
97	14.339	4034	4043	4050	rBV8	2454	4282	0.25%	0.033%
98	14.638	4133	4136	4139	rBV4	704	661	0.04%	0.005%
99	14.979	4239	4242	4245	rBV2	579	416	0.02%	0.003%
100	15.124	4285	4287	4290	rBV3	731	353	0.02%	0.003%




Sum of corrected areas: 12857876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050896.D
Acq On : 22 Sep 2022 14:30
Operator : JC/MD
Sample : N4748-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

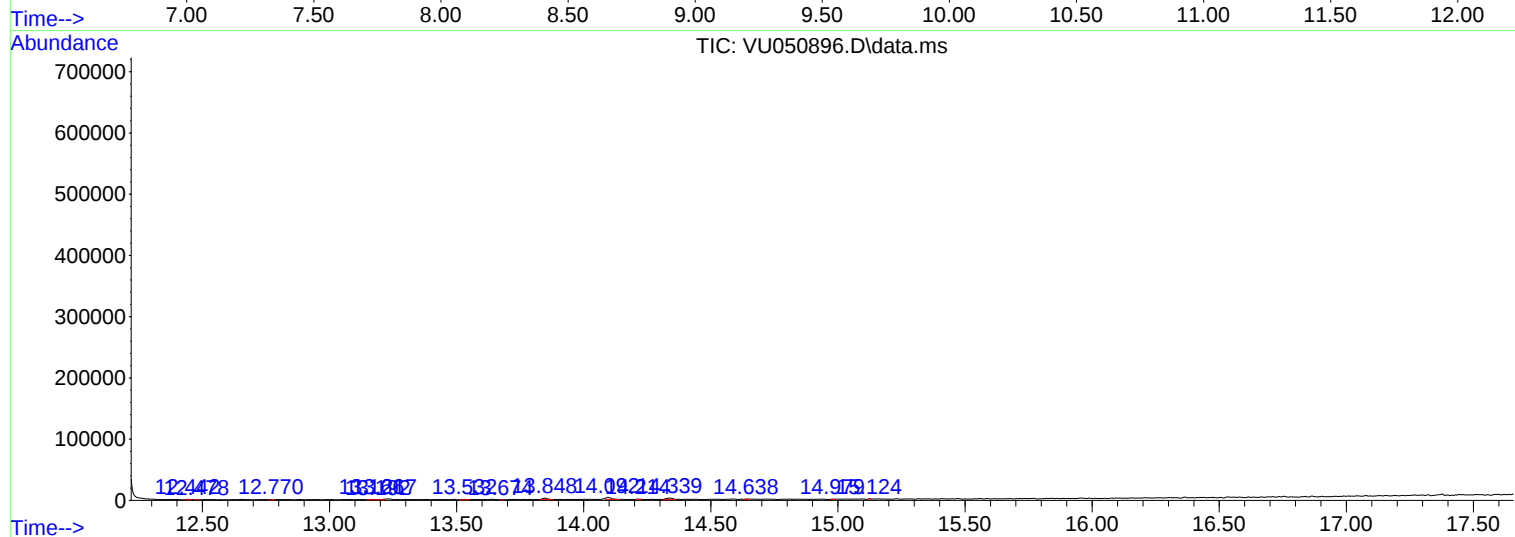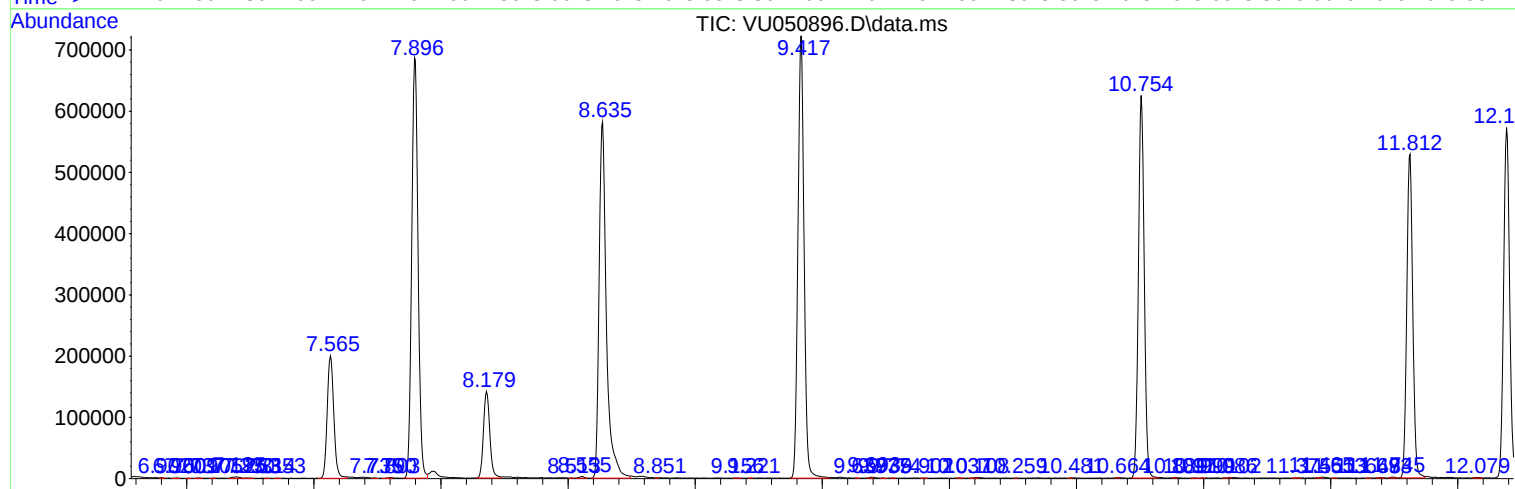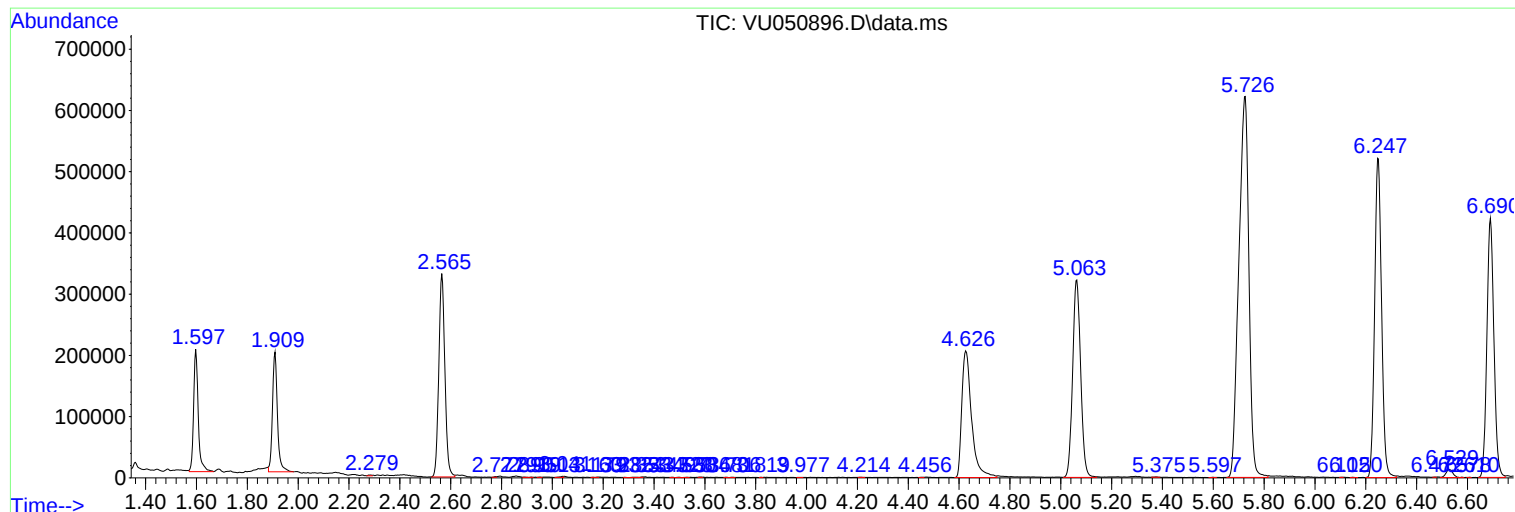

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050896.D
Acq On : 22 Sep 2022 14:30
Operator : JC/MD
Sample : N4748-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050896.D
Acq On : 22 Sep 2022 14:30
Operator : JC/MD
Sample : N4748-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------