

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050897.D
 Acq On : 22 Sep 2022 14:54
 Operator : JC/MD
 Sample : N4748-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	72	80	97	rVB	193996	229061	13.95%	1.862%
2	1.903	166	175	196	rVB	165914	225364	13.72%	1.832%
3	2.562	368	380	395	rBV	314957	517144	31.49%	4.204%
4	2.729	430	432	436	rVB2	465	359	0.02%	0.003%
5	2.758	436	441	443	rBV4	478	466	0.03%	0.004%
6	2.784	446	449	455	rVB4	1223	1257	0.08%	0.010%
7	2.842	464	467	469	rBV2	432	283	0.02%	0.002%
8	2.951	495	501	505	rBV2	747	808	0.05%	0.007%
9	3.044	522	530	539	rVV2	1379	2589	0.16%	0.021%
10	3.112	544	551	553	rBV3	312	405	0.02%	0.003%
11	3.144	556	561	564	rVV3	422	452	0.03%	0.004%
12	3.176	564	571	582	rVB4	1220	2353	0.14%	0.019%
13	3.253	591	595	600	rVB	379	348	0.02%	0.003%
14	3.327	613	618	622	rBV3	343	335	0.02%	0.003%
15	3.347	622	624	631	rVV4	450	407	0.02%	0.003%
16	4.138	866	870	874	rBV2	393	299	0.02%	0.002%
17	4.263	906	909	915	rVB	385	312	0.02%	0.003%
18	4.417	953	957	961	rVB	348	300	0.02%	0.002%
19	4.617	1005	1019	1046	rBV	218788	532079	32.40%	4.326%
20	4.948	1118	1122	1126	rBV4	380	288	0.02%	0.002%
21	4.993	1133	1136	1140	rBV3	421	376	0.02%	0.003%
22	5.060	1140	1157	1181	rVV	308668	676614	41.20%	5.501%
23	5.247	1212	1215	1218	rBV2	669	449	0.03%	0.004%
24	5.289	1222	1228	1231	rBV5	1157	1103	0.07%	0.009%
25	5.379	1252	1256	1258	rBV4	840	646	0.04%	0.005%
26	5.723	1341	1363	1387	rBV2	598932	1642221	100.00%	13.351%
27	5.983	1441	1444	1448	rVB3	1248	776	0.05%	0.006%
28	6.035	1456	1460	1463	rBV2	825	728	0.04%	0.006%
29	6.247	1511	1526	1552	rBV	500920	952117	57.98%	7.741%
30	6.369	1561	1564	1568	rVB3	855	521	0.03%	0.004%
31	6.527	1603	1613	1624	rBV3	10937	21175	1.29%	0.172%
32	6.568	1624	1626	1635	rVB3	1057	925	0.06%	0.008%
33	6.607	1636	1638	1646	rVB2	290	274	0.02%	0.002%
34	6.687	1646	1663	1682	rBV	397259	778073	47.38%	6.326%
35	6.909	1729	1732	1734	rBV2	476	324	0.02%	0.003%
36	6.977	1750	1753	1756	rBV	427	366	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050897.D
 Acq On : 22 Sep 2022 14:54
 Operator : JC/MD
 Sample : N4748-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.067	1778	1781	1785	rVB2	381	274	0.02%	0.002%
38	7.109	1790	1794	1799	rBV	442	343	0.02%	0.003%
39	7.183	1807	1817	1828	rBV5	2615	4784	0.29%	0.039%
40	7.565	1923	1936	1956	rBV2	195004	345527	21.04%	2.809%
41	7.691	1972	1975	1978	rBV4	1330	905	0.06%	0.007%
42	7.771	1996	2000	2004	rBV3	566	486	0.03%	0.004%
43	7.896	2025	2039	2054	rBV	660979	1124374	68.47%	9.141%
44	8.179	2114	2127	2148	rBV	137408	236660	14.41%	1.924%
45	8.549	2236	2242	2250	rBV6	2054	2844	0.17%	0.023%
46	8.633	2255	2268	2301	rBV2	573888	1114850	67.89%	9.064%
47	8.980	2372	2376	2381	rBV2	384	446	0.03%	0.004%
48	9.128	2419	2422	2428	rVB2	605	508	0.03%	0.004%
49	9.163	2428	2433	2436	rBV	419	410	0.02%	0.003%
50	9.414	2498	2511	2543	rBV	682810	1147220	69.86%	9.327%
51	9.575	2559	2561	2564	rVB3	772	416	0.03%	0.003%
52	9.636	2576	2580	2583	rVB3	329	294	0.02%	0.002%
53	9.671	2587	2591	2593	rBV3	465	388	0.02%	0.003%
54	9.697	2595	2599	2603	rVB	864	826	0.05%	0.007%
55	9.896	2658	2661	2664	rVB	449	281	0.02%	0.002%
56	10.099	2720	2724	2725	rVV2	483	329	0.02%	0.003%
57	10.108	2725	2727	2732	rVB3	990	625	0.04%	0.005%
58	10.182	2745	2750	2753	rBV2	438	448	0.03%	0.004%
59	10.198	2753	2755	2759	rVB2	544	309	0.02%	0.003%
60	10.404	2816	2819	2825	rVB	365	313	0.02%	0.003%
61	10.517	2852	2854	2859	rBV	365	356	0.02%	0.003%
62	10.649	2889	2895	2896	rBV2	499	456	0.03%	0.004%
63	10.671	2896	2902	2909	rVB5	1461	2206	0.13%	0.018%
64	10.755	2914	2928	2949	rBV	596413	966350	58.84%	7.856%
65	10.832	2950	2952	2958	rVB4	541	392	0.02%	0.003%
66	10.858	2958	2960	2962	rBV	611	291	0.02%	0.002%
67	10.887	2967	2969	2972	rBV2	483	276	0.02%	0.002%
68	11.096	3028	3034	3037	rBV3	1132	1162	0.07%	0.009%
69	11.121	3037	3042	3047	rVB5	1217	1423	0.09%	0.012%
70	11.372	3117	3120	3123	rVB3	651	468	0.03%	0.004%
71	11.414	3129	3133	3136	rBV2	307	301	0.02%	0.002%
72	11.469	3146	3150	3157	rVB5	1392	1603	0.10%	0.013%
73	11.581	3183	3185	3189	rVB3	598	381	0.02%	0.003%
74	11.613	3189	3195	3199	rBV	355	375	0.02%	0.003%
75	11.694	3215	3220	3229	rBV5	974	1309	0.08%	0.011%
76	11.748	3232	3237	3241	rVB3	1153	1160	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050897.D
 Acq On : 22 Sep 2022 14:54
 Operator : JC/MD
 Sample : N4748-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ESQS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.809	3243	3256	3278	rBV	516481	830092	50.55%	6.748%
78	11.922	3289	3291	3293	rVB2	718	312	0.02%	0.003%
79	12.018	3318	3321	3326	rBV2	493	466	0.03%	0.004%
80	12.070	3332	3337	3339	rBV4	1527	1227	0.07%	0.010%
81	12.192	3362	3375	3401	rBV	557141	900441	54.83%	7.320%
82	12.706	3532	3535	3540	rVB2	508	325	0.02%	0.003%
83	12.935	3602	3606	3612	rVV3	653	507	0.03%	0.004%
84	12.967	3612	3616	3619	rBV3	568	425	0.03%	0.003%
85	13.012	3628	3630	3634	rBV	444	396	0.02%	0.003%
86	13.047	3638	3641	3642	rBV	716	396	0.02%	0.003%
87	13.227	3691	3697	3699	rVV2	549	632	0.04%	0.005%
88	13.259	3704	3707	3715	rBV3	375	547	0.03%	0.004%
89	13.362	3732	3739	3740	rBV3	630	643	0.04%	0.005%
90	13.517	3783	3787	3792	rBV3	388	509	0.03%	0.004%
91	13.722	3848	3851	3854	rBV	527	394	0.02%	0.003%
92	13.742	3854	3857	3864	rVB3	567	540	0.03%	0.004%
93	13.848	3884	3890	3900	rBV4	1502	2104	0.13%	0.017%
94	14.095	3961	3967	3970	rBV5	1669	1836	0.11%	0.015%
95	14.237	4008	4011	4016	rBV3	475	408	0.02%	0.003%
96	14.263	4016	4019	4022	rBV3	694	475	0.03%	0.004%
97	14.340	4036	4043	4052	rBV9	1570	1722	0.10%	0.014%
98	14.571	4110	4115	4116	rBV	788	615	0.04%	0.005%
99	14.600	4122	4124	4127	rBV3	498	367	0.02%	0.003%
100	15.780	4488	4491	4496	rBV4	1224	1057	0.06%	0.009%




Sum of corrected areas: 12300402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050897.D
Acq On : 22 Sep 2022 14:54
Operator : JC/MD
Sample : N4748-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

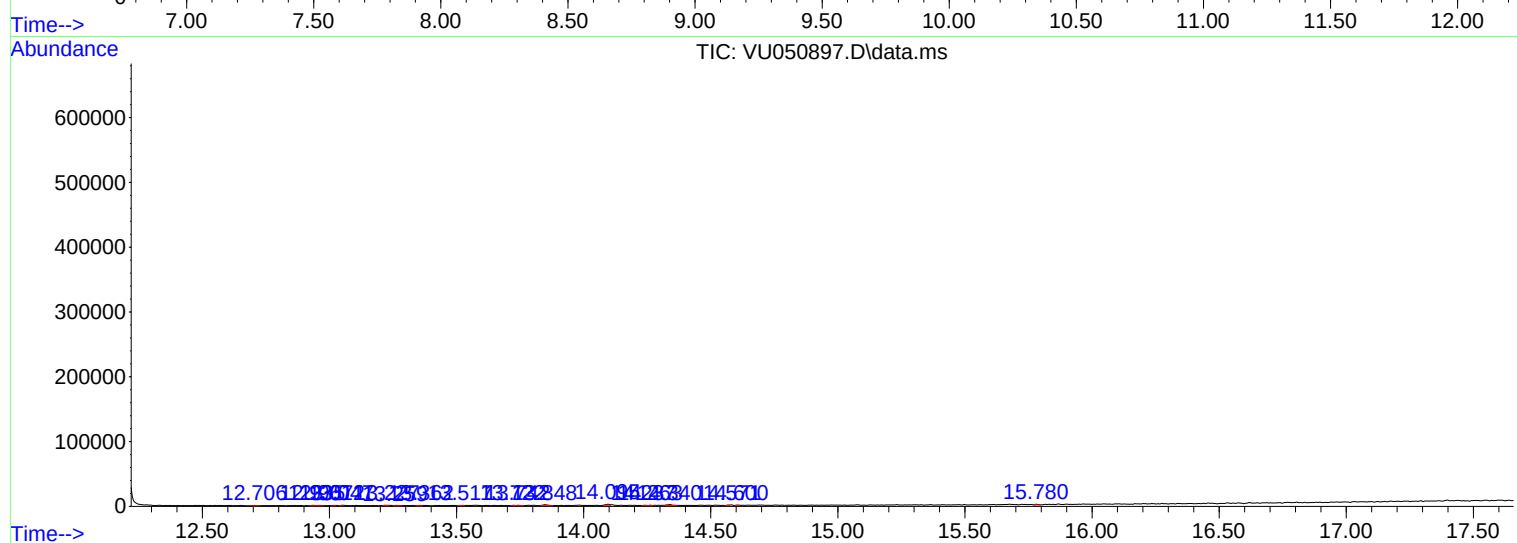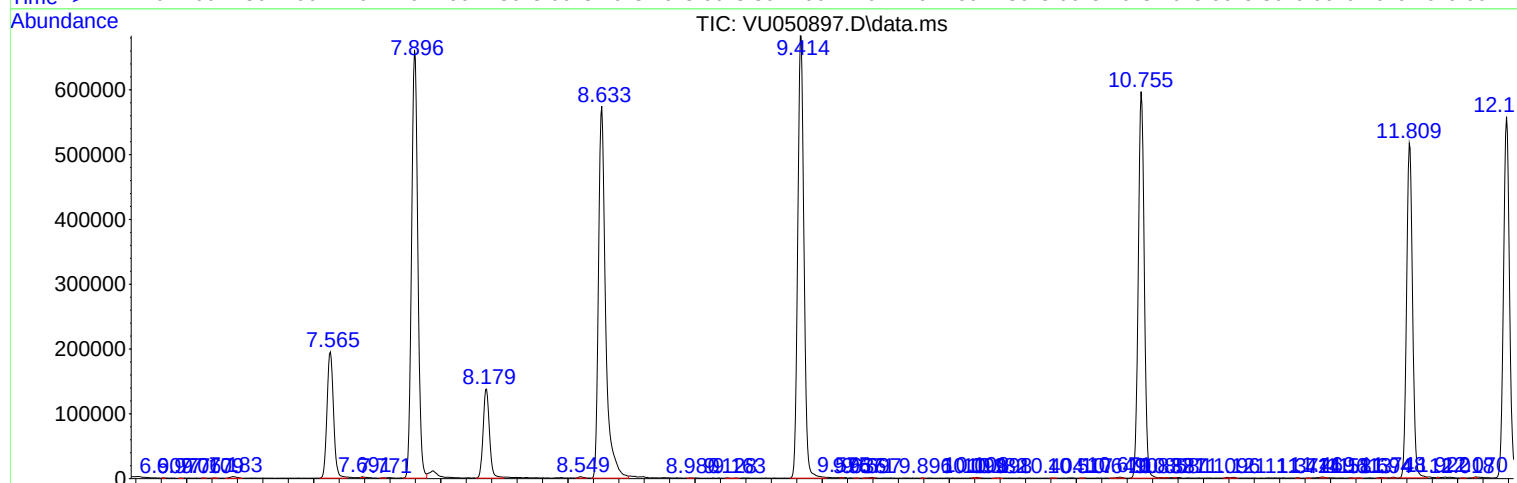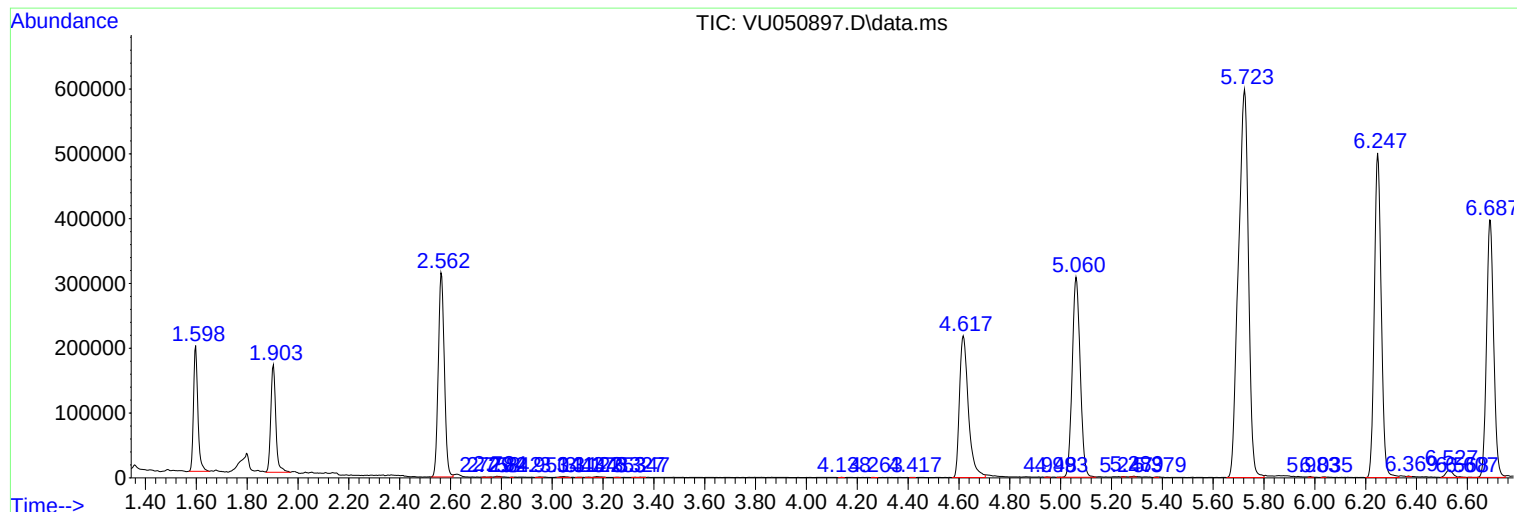

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050897.D
Acq On : 22 Sep 2022 14:54
Operator : JC/MD
Sample : N4748-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050897.D
Acq On : 22 Sep 2022 14:54
Operator : JC/MD
Sample : N4748-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ESQS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc