

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050899.D
 Acq On : 22 Sep 2022 15:40
 Operator : JC/MD
 Sample : N4650-05DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ01DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	214194	255342	14.47%	1.787%
2	1.903	167	175	195	rVB	172566	256252	14.52%	1.794%
3	2.565	368	381	396	rBV	335700	556580	31.54%	3.896%
4	2.710	421	426	430	rVB2	559	635	0.04%	0.004%
5	2.758	430	441	444	rBV4	1661	2600	0.15%	0.018%
6	2.819	458	460	464	rVB2	635	339	0.02%	0.002%
7	2.887	479	481	486	rVB3	439	335	0.02%	0.002%
8	2.974	505	508	512	rVB2	573	428	0.02%	0.003%
9	3.044	520	530	543	rVB2	6665	11100	0.63%	0.078%
10	3.183	556	573	593	rVB	34151	79033	4.48%	0.553%
11	3.356	616	627	631	rBV3	2151	3440	0.19%	0.024%
12	3.420	645	647	654	rVB2	395	338	0.02%	0.002%
13	3.465	654	661	664	rBV	343	284	0.02%	0.002%
14	3.771	752	756	762	rVB	539	398	0.02%	0.003%
15	3.867	766	786	806	rBV	81831	193209	10.95%	1.352%
16	4.543	990	996	999	rBV3	368	389	0.02%	0.003%
17	4.617	1003	1019	1027	rBV	244691	546105	30.94%	3.823%
18	4.903	1104	1108	1119	rVB4	887	1393	0.08%	0.010%
19	4.945	1119	1121	1124	rBV2	563	306	0.02%	0.002%
20	5.006	1137	1140	1141	rBV	639	342	0.02%	0.002%
21	5.060	1141	1157	1184	rVB	335024	727585	41.23%	5.093%
22	5.154	1184	1186	1191	rBV2	415	360	0.02%	0.003%
23	5.314	1219	1236	1254	rBV	250641	567699	32.17%	3.974%
24	5.462	1279	1282	1285	rBV2	350	271	0.02%	0.002%
25	5.488	1285	1290	1293	rBV3	931	1000	0.06%	0.007%
26	5.594	1319	1323	1325	rBV	324	272	0.02%	0.002%
27	5.723	1341	1363	1384	rBV2	652099	1764850	100.00%	12.354%
28	6.044	1461	1463	1474	rVB5	741	1040	0.06%	0.007%
29	6.247	1512	1526	1547	rBV	549490	1032976	58.53%	7.231%
30	6.533	1603	1615	1630	rVB6	15127	34451	1.95%	0.241%
31	6.687	1646	1663	1685	rBV	431236	842873	47.76%	5.900%
32	6.800	1695	1698	1701	rBV4	1574	1212	0.07%	0.008%
33	6.883	1721	1724	1730	rVB4	702	605	0.03%	0.004%
34	6.919	1730	1735	1738	rVV4	517	416	0.02%	0.003%
35	6.938	1738	1741	1746	rVB3	467	372	0.02%	0.003%
36	7.038	1765	1772	1777	rVV4	513	716	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050899.D
 Acq On : 22 Sep 2022 15:40
 Operator : JC/MD
 Sample : N4650-05DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ01DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.096	1786	1790	1792	rVV3	341	278	0.02%	0.002%
38	7.147	1801	1806	1809	rBV2	353	297	0.02%	0.002%
39	7.182	1809	1817	1832	rVB5	2806	4971	0.28%	0.035%
40	7.452	1895	1901	1905	rBV2	361	348	0.02%	0.002%
41	7.565	1922	1936	1955	rBV	207916	367989	20.85%	2.576%
42	7.896	2025	2039	2054	rBV	716397	1222767	69.28%	8.559%
43	8.179	2113	2127	2144	rBV	148776	252403	14.30%	1.767%
44	8.443	2205	2209	2211	rBV3	409	341	0.02%	0.002%
45	8.472	2212	2218	2227	rVB5	939	1728	0.10%	0.012%
46	8.552	2234	2243	2255	rBV3	14865	24350	1.38%	0.170%
47	8.632	2255	2268	2302	rBV2	590930	1166687	66.11%	8.167%
48	8.861	2336	2339	2343	rBB4	577	336	0.02%	0.002%
49	9.118	2416	2419	2426	rVB3	439	374	0.02%	0.003%
50	9.227	2451	2453	2458	rBV2	398	278	0.02%	0.002%
51	9.317	2478	2481	2485	rBV2	255	271	0.02%	0.002%
52	9.417	2499	2512	2540	rBV	766405	1266088	71.74%	8.863%
53	9.575	2554	2561	2566	rBV6	695	1026	0.06%	0.007%
54	9.636	2577	2580	2583	rBV3	601	373	0.02%	0.003%
55	9.694	2593	2598	2599	rBV3	593	532	0.03%	0.004%
56	9.764	2617	2620	2625	rBV	473	378	0.02%	0.003%
57	9.980	2684	2687	2690	rBV2	328	298	0.02%	0.002%
58	10.102	2715	2725	2730	rBV4	740	1318	0.07%	0.009%
59	10.179	2746	2749	2754	rVV2	313	285	0.02%	0.002%
60	10.478	2838	2842	2843	rBV2	444	336	0.02%	0.002%
61	10.616	2882	2885	2891	rVB3	622	519	0.03%	0.004%
62	10.674	2895	2903	2914	rVB4	1532	2352	0.13%	0.016%
63	10.755	2914	2928	2950	rBV	651920	1050798	59.54%	7.356%
64	10.896	2968	2972	2974	rBV5	645	416	0.02%	0.003%
65	11.002	3003	3005	3011	rVB2	569	397	0.02%	0.003%
66	11.086	3026	3031	3033	rBV3	306	285	0.02%	0.002%
67	11.118	3035	3041	3045	rVB4	871	1040	0.06%	0.007%
68	11.176	3054	3059	3061	rBV3	404	346	0.02%	0.002%
69	11.224	3071	3074	3083	rVB2	271	285	0.02%	0.002%
70	11.285	3088	3093	3095	rBV4	1096	1009	0.06%	0.007%
71	11.311	3099	3101	3105	rVB2	684	407	0.02%	0.003%
72	11.414	3129	3133	3136	rBV2	545	473	0.03%	0.003%
73	11.468	3140	3150	3157	rBV4	2921	4802	0.27%	0.034%
74	11.565	3178	3180	3184	rVV2	382	314	0.02%	0.002%
75	11.693	3217	3220	3224	rBV4	684	553	0.03%	0.004%
76	11.809	3244	3256	3277	rBV	603774	966150	54.74%	6.763%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050899.D
 Acq On : 22 Sep 2022 15:40
 Operator : JC/MD
 Sample : N4650-05DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ01DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.095	3340	3345	3347	rBV2	933	822	0.05%	0.006%
78	12.192	3361	3375	3399	rBV	638937	1042451	59.07%	7.297%
79	12.459	3451	3458	3461	rBV2	861	783	0.04%	0.005%
80	12.636	3511	3513	3517	rBV2	352	292	0.02%	0.002%
81	12.681	3522	3527	3531	rBV5	781	738	0.04%	0.005%
82	12.809	3564	3567	3571	rBV2	410	357	0.02%	0.002%
83	12.867	3582	3585	3588	rVV4	430	293	0.02%	0.002%
84	12.925	3600	3603	3609	rVB2	526	491	0.03%	0.003%
85	12.973	3613	3618	3622	rBV	442	509	0.03%	0.004%
86	13.227	3694	3697	3700	rVB2	869	557	0.03%	0.004%
87	13.333	3727	3730	3733	rBV2	646	481	0.03%	0.003%
88	13.388	3744	3747	3752	rVB2	746	609	0.03%	0.004%
89	13.417	3752	3756	3762	rBV2	607	564	0.03%	0.004%
90	13.510	3783	3785	3788	rBV	731	455	0.03%	0.003%
91	13.581	3803	3807	3810	rBV2	1193	825	0.05%	0.006%
92	13.648	3825	3828	3835	rVB3	1133	876	0.05%	0.006%
93	13.680	3835	3838	3839	rBV	799	464	0.03%	0.003%
94	13.709	3844	3847	3852	rVB	1128	707	0.04%	0.005%
95	13.783	3867	3870	3873	rBV2	486	325	0.02%	0.002%
96	13.844	3885	3889	3891	rBV2	1429	939	0.05%	0.007%
97	13.880	3898	3900	3904	rVB	565	357	0.02%	0.002%
98	13.925	3912	3914	3919	rBV2	349	287	0.02%	0.002%
99	14.079	3959	3962	3964	rBV2	810	542	0.03%	0.004%
100	14.938	4223	4229	4234	rBV5	1016	1251	0.07%	0.009%



Sum of corrected areas: 14285719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050899.D
Acq On : 22 Sep 2022 15:40
Operator : JC/MD
Sample : N4650-05DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

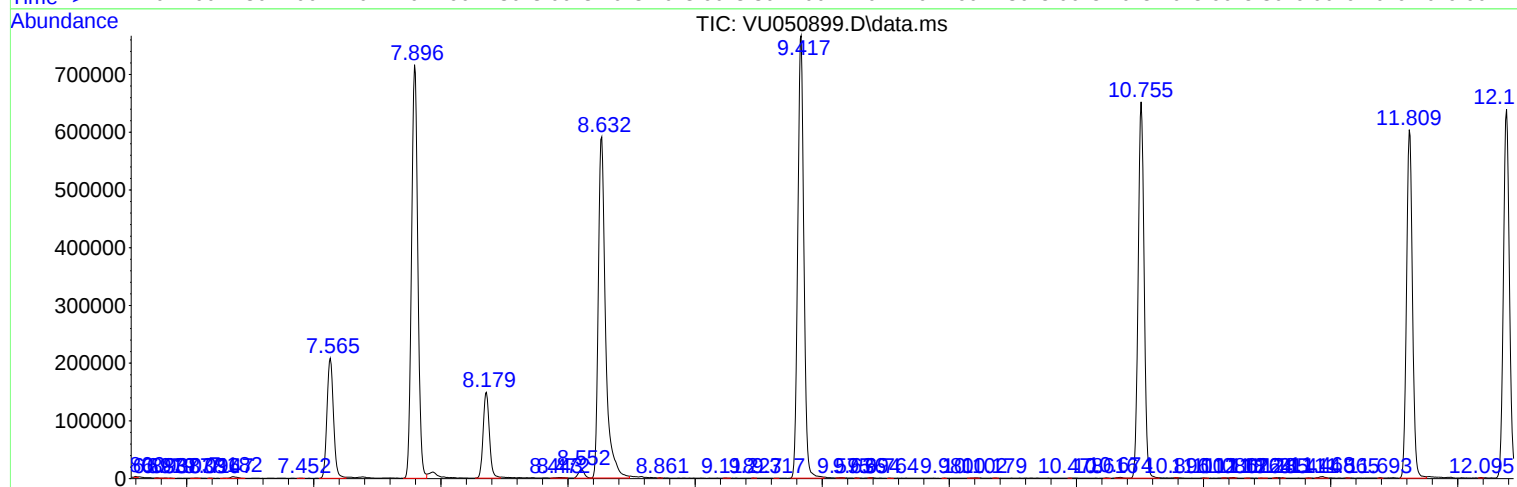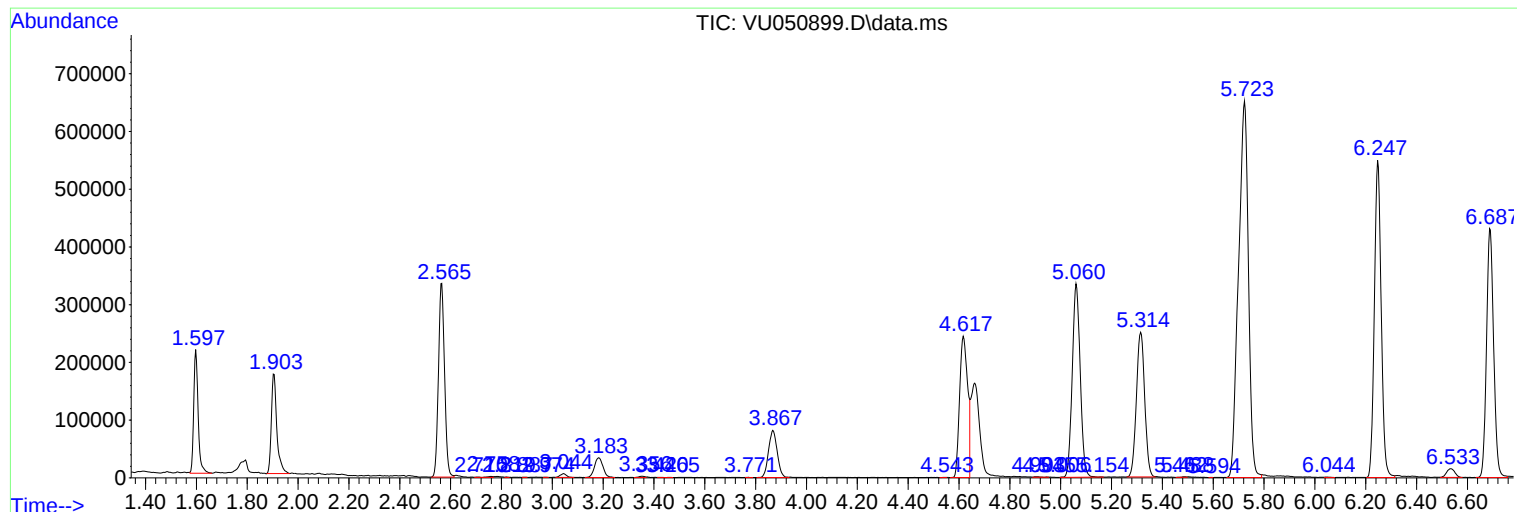

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050899.D
Acq On : 22 Sep 2022 15:40
Operator : JC/MD
Sample : N4650-05DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050899.D
Acq On : 22 Sep 2022 15:40
Operator : JC/MD
Sample : N4650-05DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------