

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050900.D
 Acq On : 22 Sep 2022 16:03
 Operator : JC/MD
 Sample : N4650-20DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ37DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	72	80	105	rVB	174160	248952	13.37%	1.597%
2	1.906	169	176	191	rBV	185275	260910	14.01%	1.674%
3	2.559	366	379	400	rBV2	388543	705945	37.92%	4.528%
4	2.752	434	439	442	rVB3	519	414	0.02%	0.003%
5	2.858	467	472	475	rBV2	453	408	0.02%	0.003%
6	3.038	518	528	539	rVB3	8665	14668	0.79%	0.094%
7	3.080	539	541	546	rVB3	492	406	0.02%	0.003%
8	3.179	556	572	590	rBV	44213	101952	5.48%	0.654%
9	3.350	618	625	639	rVB9	4326	8996	0.48%	0.058%
10	3.408	639	643	647	rBV	322	368	0.02%	0.002%
11	3.446	650	655	661	rVB3	410	440	0.02%	0.003%
12	3.485	661	667	670	rBV2	331	315	0.02%	0.002%
13	3.864	765	785	806	rVB2	86102	202479	10.87%	1.299%
14	3.951	806	812	817	rBV3	480	729	0.04%	0.005%
15	4.025	830	835	838	rBV2	709	717	0.04%	0.005%
16	4.408	950	954	957	rVB2	397	343	0.02%	0.002%
17	4.440	961	964	971	rBV	341	306	0.02%	0.002%
18	4.633	1008	1024	1074	rBV2	213812	784933	42.16%	5.035%
19	4.974	1128	1130	1133	rVB	624	322	0.02%	0.002%
20	5.060	1140	1157	1180	rBV	350617	764446	41.06%	4.903%
21	5.311	1216	1235	1254	rBV	253823	571149	30.68%	3.663%
22	5.578	1314	1318	1319	rBV2	577	318	0.02%	0.002%
23	5.723	1337	1363	1398	rBV2	683373	1861897	100.00%	11.942%
24	5.977	1432	1442	1457	rVB9	3592	7669	0.41%	0.049%
25	6.044	1459	1463	1475	rVB4	861	1296	0.07%	0.008%
26	6.247	1511	1526	1546	rBV	580020	1091255	58.61%	6.999%
27	6.420	1577	1580	1584	rVB3	484	315	0.02%	0.002%
28	6.469	1592	1595	1601	rBV4	749	565	0.03%	0.004%
29	6.539	1601	1617	1629	rBV5	60816	129845	6.97%	0.833%
30	6.687	1649	1663	1694	rBV	451098	887059	47.64%	5.690%
31	6.800	1695	1698	1701	rBV4	845	586	0.03%	0.004%
32	6.848	1711	1713	1720	rVB4	856	894	0.05%	0.006%
33	6.922	1733	1736	1738	rBV	425	315	0.02%	0.002%
34	7.057	1774	1778	1783	rVB3	464	540	0.03%	0.003%
35	7.192	1810	1820	1823	rBV4	3211	4883	0.26%	0.031%
36	7.404	1882	1886	1889	rBV2	339	282	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050900.D
 Acq On : 22 Sep 2022 16:03
 Operator : JC/MD
 Sample : N4650-20DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ37DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.443	1894	1898	1904	rBV3	255	278	0.01%	0.002%
38	7.565	1923	1936	1959	rBV	216656	389188	20.90%	2.496%
39	7.784	2000	2004	2006	rBV	517	351	0.02%	0.002%
40	7.800	2006	2009	2013	rBV2	396	347	0.02%	0.002%
41	7.896	2022	2039	2055	rBV	747155	1283936	68.96%	8.235%
42	8.179	2112	2127	2143	rBV	151618	266577	14.32%	1.710%
43	8.327	2167	2173	2176	rBV2	656	797	0.04%	0.005%
44	8.398	2189	2195	2203	rVB5	2892	4496	0.24%	0.029%
45	8.472	2211	2218	2229	rVB2	1984	3096	0.17%	0.020%
46	8.552	2231	2243	2257	rBV	76741	128619	6.91%	0.825%
47	8.642	2257	2271	2301	rBV2	602061	1281284	68.82%	8.218%
48	8.877	2342	2344	2351	rVB4	684	560	0.03%	0.004%
49	8.925	2353	2359	2361	rBV4	635	648	0.03%	0.004%
50	8.967	2366	2372	2375	rBV3	416	408	0.02%	0.003%
51	8.983	2375	2377	2379	rVV3	495	276	0.01%	0.002%
52	9.022	2383	2389	2393	rBV3	856	882	0.05%	0.006%
53	9.057	2396	2400	2403	rVB	492	357	0.02%	0.002%
54	9.089	2408	2410	2415	rVB3	574	368	0.02%	0.002%
55	9.285	2468	2471	2473	rVB2	531	294	0.02%	0.002%
56	9.337	2480	2487	2491	rBV2	306	352	0.02%	0.002%
57	9.417	2497	2512	2540	rBV	786773	1315269	70.64%	8.436%
58	9.591	2564	2566	2571	rVB3	763	446	0.02%	0.003%
59	9.645	2580	2583	2586	rBV2	540	372	0.02%	0.002%
60	9.694	2589	2598	2601	rBV4	1190	1678	0.09%	0.011%
61	9.755	2613	2617	2626	rVB3	350	523	0.03%	0.003%
62	9.919	2663	2668	2671	rVB2	447	345	0.02%	0.002%
63	9.951	2672	2678	2681	rBV2	422	415	0.02%	0.003%
64	10.009	2692	2696	2698	rVB	456	316	0.02%	0.002%
65	10.060	2709	2712	2718	rBV2	442	389	0.02%	0.002%
66	10.102	2720	2725	2730	rBV4	691	851	0.05%	0.005%
67	10.125	2730	2732	2736	rVB2	559	335	0.02%	0.002%
68	10.224	2757	2763	2766	rBV2	361	375	0.02%	0.002%
69	10.485	2842	2844	2849	rVV2	425	317	0.02%	0.002%
70	10.626	2883	2888	2891	rBV2	378	324	0.02%	0.002%
71	10.655	2891	2897	2898	rBV3	930	771	0.04%	0.005%
72	10.671	2898	2902	2910	rVB3	1652	1793	0.10%	0.012%
73	10.758	2916	2929	2946	rBV	686449	1115260	59.90%	7.153%
74	10.893	2964	2971	2981	rVB6	2006	2872	0.15%	0.018%
75	11.051	3016	3020	3023	rBV3	371	338	0.02%	0.002%
76	11.115	3032	3040	3050	rVB6	2114	2641	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050900.D
 Acq On : 22 Sep 2022 16:03
 Operator : JC/MD
 Sample : N4650-20DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ37DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.311	3097	3101	3106	rVB2	816	726	0.04%	0.005%
78	11.340	3106	3110	3112	rBV3	462	326	0.02%	0.002%
79	11.382	3121	3123	3129	rVB2	573	391	0.02%	0.003%
80	11.456	3139	3146	3149	rBV4	939	1284	0.07%	0.008%
81	11.748	3231	3237	3244	rBV4	795	1190	0.06%	0.008%
82	11.813	3244	3257	3275	rBV	636944	1019394	54.75%	6.539%
83	12.025	3321	3323	3330	rVB2	377	350	0.02%	0.002%
84	12.057	3330	3333	3337	rBV3	391	332	0.02%	0.002%
85	12.192	3363	3375	3393	rBV	668636	1094406	58.78%	7.020%
86	12.356	3424	3426	3431	rVB3	527	324	0.02%	0.002%
87	12.382	3431	3434	3437	rBV2	577	424	0.02%	0.003%
88	12.694	3527	3531	3534	rBV2	475	441	0.02%	0.003%
89	12.761	3548	3552	3557	rVV4	837	905	0.05%	0.006%
90	13.327	3726	3728	3734	rVB	763	387	0.02%	0.002%
91	13.356	3734	3737	3740	rBV	402	327	0.02%	0.002%
92	13.378	3742	3744	3750	rVB2	664	583	0.03%	0.004%
93	13.513	3783	3786	3788	rBV2	395	279	0.01%	0.002%
94	13.533	3788	3792	3797	rVB2	446	474	0.03%	0.003%
95	13.883	3898	3901	3902	rBV	515	285	0.02%	0.002%
96	14.012	3939	3941	3944	rVB	542	275	0.01%	0.002%
97	14.092	3963	3966	3967	rBV	687	407	0.02%	0.003%
98	14.173	3988	3991	3998	rVB4	612	638	0.03%	0.004%
99	14.443	4071	4075	4078	rBV2	539	442	0.02%	0.003%
100	15.494	4400	4402	4405	rBV3	796	352	0.02%	0.002%




Sum of corrected areas: 15590603

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050900.D
Acq On : 22 Sep 2022 16:03
Operator : JC/MD
Sample : N4650-20DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ37DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

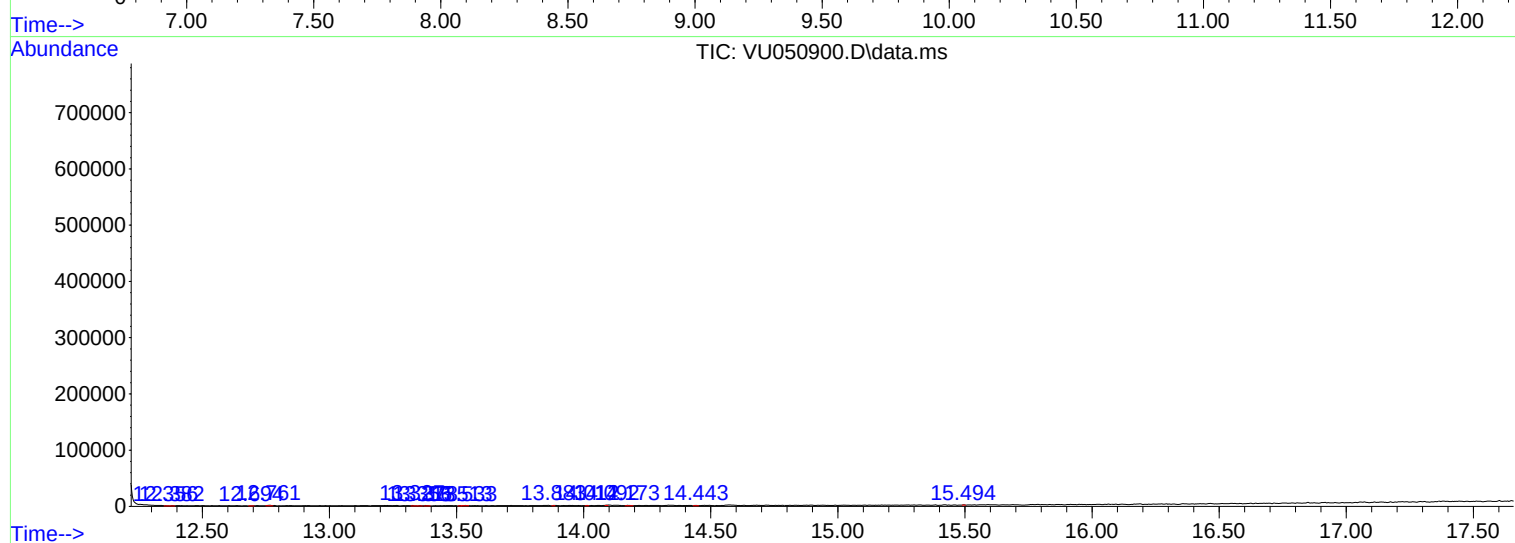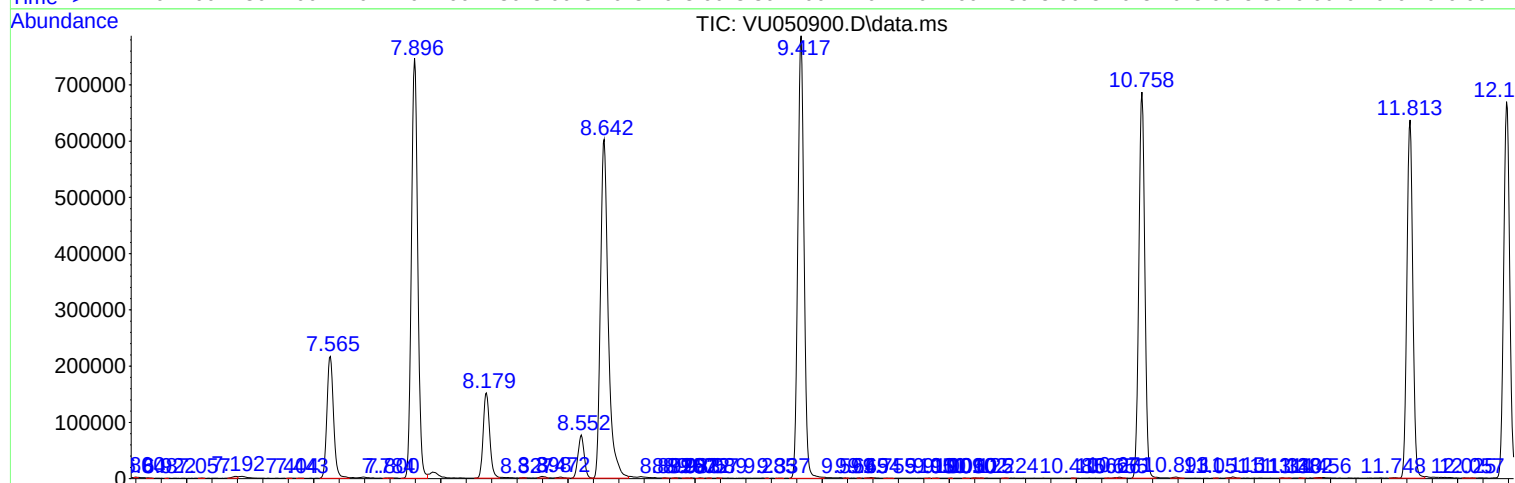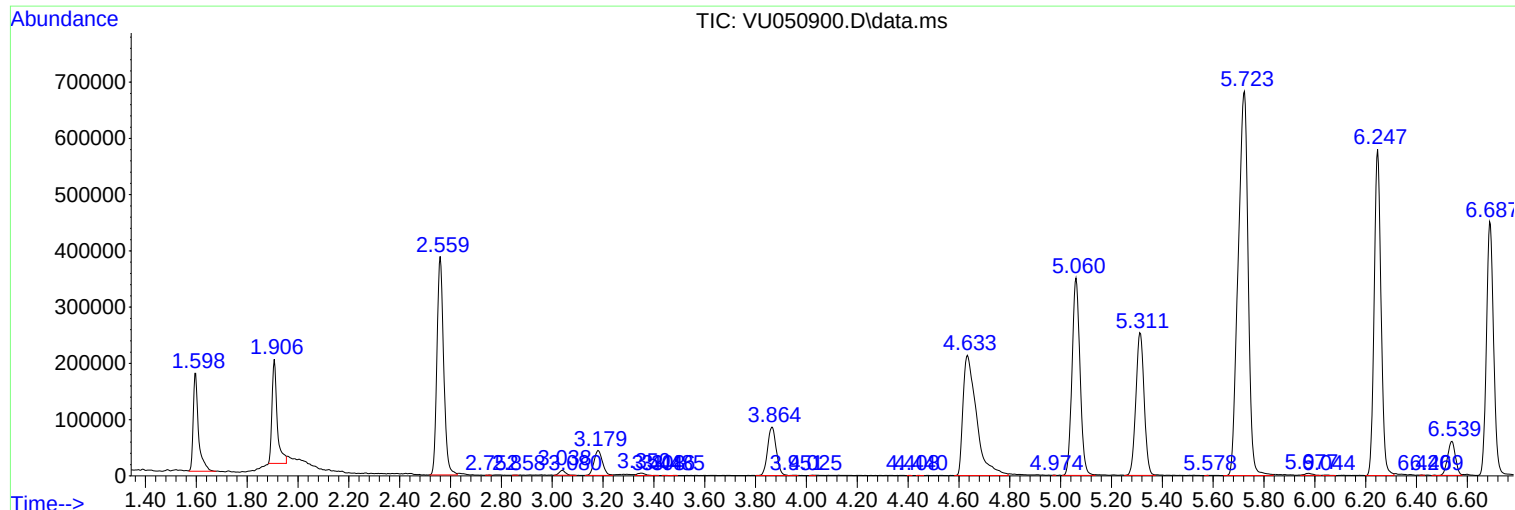

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050900.D
Acq On : 22 Sep 2022 16:03
Operator : JC/MD
Sample : N4650-20DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ37DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050900.D
Acq On : 22 Sep 2022 16:03
Operator : JC/MD
Sample : N4650-20DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ37DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc