

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050901.D
 Acq On : 22 Sep 2022 16:27
 Operator : JC/MD
 Sample : N4747-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	186101	214383	13.60%	1.772%
2	1.906	167	176	198	rVB	159561	218237	13.84%	1.804%
3	2.276	287	291	292	rBV3	3846	2772	0.18%	0.023%
4	2.488	355	357	362	rVB2	780	665	0.04%	0.005%
5	2.565	368	381	397	rBV	311083	509096	32.29%	4.208%
6	2.758	436	441	444	rBV3	531	418	0.03%	0.003%
7	2.781	444	448	449	rBV3	498	385	0.02%	0.003%
8	2.948	497	500	503	rBV3	508	349	0.02%	0.003%
9	3.041	520	529	539	rVB7	1606	2570	0.16%	0.021%
10	3.092	539	545	549	rBV2	306	282	0.02%	0.002%
11	3.118	550	553	560	rVB2	487	448	0.03%	0.004%
12	3.173	560	570	583	rBV5	1759	4156	0.26%	0.034%
13	3.353	621	626	636	rVB4	660	876	0.06%	0.007%
14	3.427	647	649	656	rVB2	339	305	0.02%	0.003%
15	3.578	694	696	706	rVB4	610	801	0.05%	0.007%
16	3.636	707	714	719	rBV2	242	331	0.02%	0.003%
17	3.871	776	787	790	rBV4	891	1599	0.10%	0.013%
18	4.006	823	829	834	rVB2	297	363	0.02%	0.003%
19	4.038	834	839	842	rBV2	341	312	0.02%	0.003%
20	4.617	1006	1019	1052	rBV	210893	528243	33.50%	4.366%
21	4.925	1112	1115	1119	rBV3	537	378	0.02%	0.003%
22	5.060	1141	1157	1186	rBV	295645	654846	41.53%	5.412%
23	5.289	1225	1228	1231	rBV4	680	435	0.03%	0.004%
24	5.565	1308	1314	1322	rVB2	226	387	0.02%	0.003%
25	5.723	1338	1363	1384	rBV2	570149	1576817	100.00%	13.032%
26	6.247	1512	1526	1555	rBV	478304	922638	58.51%	7.626%
27	6.539	1603	1617	1630	rBV6	40406	83634	5.30%	0.691%
28	6.690	1649	1664	1688	rBV	389041	760015	48.20%	6.281%
29	6.903	1728	1730	1733	rVB3	517	294	0.02%	0.002%
30	6.967	1745	1750	1756	rVB2	492	493	0.03%	0.004%
31	7.012	1761	1764	1768	rVB	460	289	0.02%	0.002%
32	7.044	1768	1774	1776	rBV2	496	577	0.04%	0.005%
33	7.182	1800	1817	1830	rBV6	2066	4529	0.29%	0.037%
34	7.565	1923	1936	1958	rBV2	185583	326776	20.72%	2.701%
35	7.671	1967	1969	1972	rBV2	591	456	0.03%	0.004%
36	7.790	2001	2006	2008	rBV3	903	656	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050901.D
 Acq On : 22 Sep 2022 16:27
 Operator : JC/MD
 Sample : N4747-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.832	2015	2019	2024	rBV3	355	390	0.02%	0.003%
38	7.896	2024	2039	2054	rBV	628071	1075613	68.21%	8.890%
39	8.034	2081	2082	2089	rVB3	805	485	0.03%	0.004%
40	8.073	2092	2094	2098	rVB4	587	404	0.03%	0.003%
41	8.092	2098	2100	2104	rVB3	464	279	0.02%	0.002%
42	8.179	2115	2127	2144	rBV	130235	223960	14.20%	1.851%
43	8.388	2187	2192	2197	rBV3	638	762	0.05%	0.006%
44	8.475	2210	2219	2224	rBV7	1775	2646	0.17%	0.022%
45	8.530	2233	2236	2239	rVB	457	313	0.02%	0.003%
46	8.549	2239	2242	2243	rBV2	604	350	0.02%	0.003%
47	8.581	2249	2252	2255	rBV2	416	397	0.03%	0.003%
48	8.632	2255	2268	2299	rBV2	558753	1088365	69.02%	8.995%
49	8.867	2339	2341	2344	rBV2	503	288	0.02%	0.002%
50	8.935	2358	2362	2365	rBV3	594	495	0.03%	0.004%
51	9.021	2386	2389	2395	rVB	409	358	0.02%	0.003%
52	9.131	2418	2423	2426	rBV2	315	316	0.02%	0.003%
53	9.295	2471	2474	2480	rBV2	438	365	0.02%	0.003%
54	9.417	2498	2512	2541	rBV	670826	1126489	71.44%	9.310%
55	9.613	2571	2573	2579	rVB3	449	321	0.02%	0.003%
56	9.645	2579	2583	2585	rBV2	597	444	0.03%	0.004%
57	10.298	2781	2786	2788	rBV	296	294	0.02%	0.002%
58	10.478	2839	2842	2848	rVB3	356	354	0.02%	0.003%
59	10.626	2884	2888	2890	rBV3	362	319	0.02%	0.003%
60	10.668	2895	2901	2911	rVB5	1574	2205	0.14%	0.018%
61	10.755	2913	2928	2950	rBV	582176	940001	59.61%	7.769%
62	10.893	2961	2971	2979	rVV6	1632	2527	0.16%	0.021%
63	11.095	3028	3034	3035	rBV2	422	356	0.02%	0.003%
64	11.140	3046	3048	3052	rBV	560	429	0.03%	0.004%
65	11.230	3072	3076	3079	rBV	402	342	0.02%	0.003%
66	11.375	3116	3121	3124	rBV3	456	374	0.02%	0.003%
67	11.465	3141	3149	3155	rBV6	1208	1983	0.13%	0.016%
68	11.571	3178	3182	3185	rBV	536	438	0.03%	0.004%
69	11.700	3219	3222	3226	rVB3	1042	773	0.05%	0.006%
70	11.748	3234	3237	3244	rVB3	526	578	0.04%	0.005%
71	11.809	3244	3256	3276	rBV	521467	838102	53.15%	6.927%
72	11.973	3303	3307	3315	rVB5	1498	1645	0.10%	0.014%
73	12.066	3326	3336	3349	rBV3	18266	35077	2.22%	0.290%
74	12.192	3362	3375	3396	rBV	572117	915351	58.05%	7.565%
75	12.343	3419	3422	3426	rVB3	1015	672	0.04%	0.006%
76	12.443	3449	3453	3454	rBV2	441	282	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050901.D
 Acq On : 22 Sep 2022 16:27
 Operator : JC/MD
 Sample : N4747-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.809	3561	3567	3570	rBV3	531	463	0.03%	0.004%
78	12.854	3579	3581	3585	rVB2	476	306	0.02%	0.003%
79	12.899	3590	3595	3600	rBV4	664	760	0.05%	0.006%
80	13.227	3691	3697	3701	rVV4	813	815	0.05%	0.007%
81	13.291	3713	3717	3724	rBV3	528	737	0.05%	0.006%
82	13.352	3733	3736	3739	rVB	621	376	0.02%	0.003%
83	13.452	3763	3767	3772	rBV3	328	327	0.02%	0.003%
84	13.539	3791	3794	3797	rBV4	562	401	0.03%	0.003%
85	13.565	3800	3802	3805	rVV2	497	349	0.02%	0.003%
86	13.587	3805	3809	3815	rVB3	455	560	0.04%	0.005%
87	13.738	3853	3856	3861	rBV2	453	371	0.02%	0.003%
88	13.793	3870	3873	3876	rBV2	495	356	0.02%	0.003%
89	13.812	3877	3879	3882	rVV3	647	409	0.03%	0.003%
90	13.848	3886	3890	3898	rVB4	744	899	0.06%	0.007%
91	13.896	3898	3905	3911	rBV3	503	915	0.06%	0.008%
92	14.028	3943	3946	3951	rBV2	455	379	0.02%	0.003%
93	14.095	3964	3967	3968	rBV2	649	361	0.02%	0.003%
94	14.561	4109	4112	4116	rBV3	650	480	0.03%	0.004%
95	14.864	4203	4206	4208	rBV2	538	284	0.02%	0.002%
96	14.996	4244	4247	4252	rBV4	1202	1303	0.08%	0.011%
97	15.430	4379	4382	4384	rBV2	888	499	0.03%	0.004%
98	15.462	4389	4392	4398	rVB5	869	1024	0.06%	0.008%
99	15.500	4398	4404	4410	rBV7	1195	1643	0.10%	0.014%
100	15.674	4456	4458	4459	rBV	703	327	0.02%	0.003%




Sum of corrected areas: 12099297

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050901.D
Acq On : 22 Sep 2022 16:27
Operator : JC/MD
Sample : N4747-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

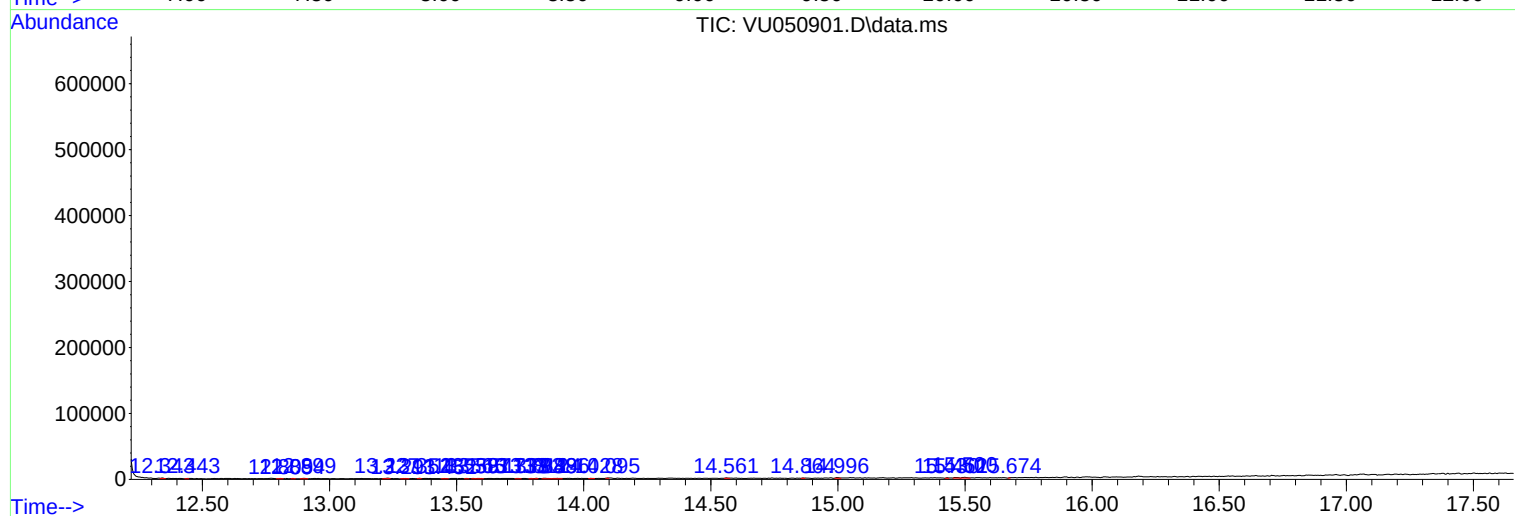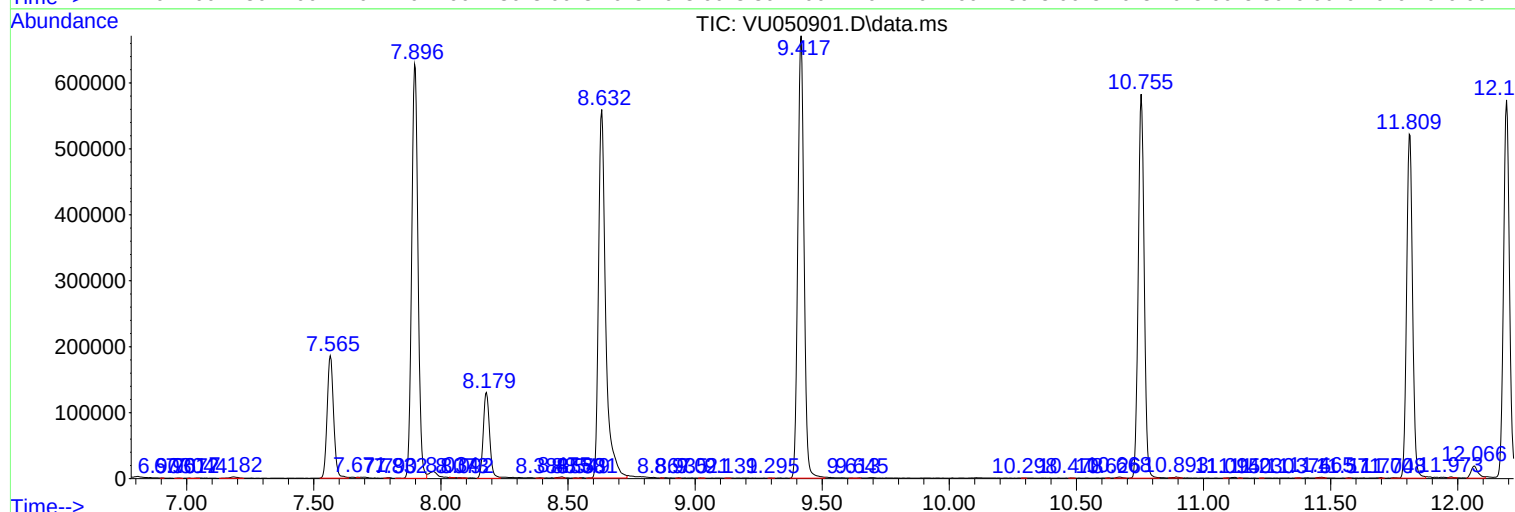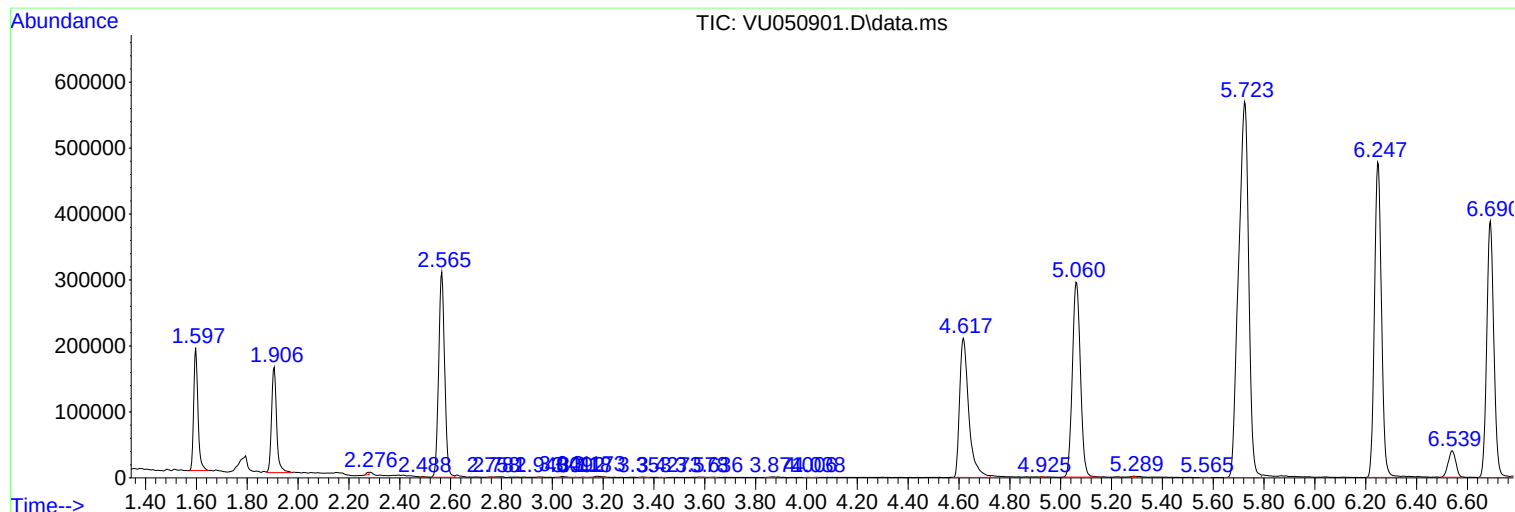

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050901.D
Acq On : 22 Sep 2022 16:27
Operator : JC/MD
Sample : N4747-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050901.D
Acq On : 22 Sep 2022 16:27
Operator : JC/MD
Sample : N4747-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------