

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050902.D
 Acq On : 22 Sep 2022 16:51
 Operator : JC/MD
 Sample : N4650-21DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	162450	216494	12.17%	1.501%
2	1.887	164	170	197	rVB	182509	269885	15.18%	1.872%
3	2.559	366	379	400	rBV2	341051	596505	33.54%	4.137%
4	2.960	495	504	511	rVB3	575	1238	0.07%	0.009%
5	3.041	517	529	541	rVV3	13901	25815	1.45%	0.179%
6	3.105	545	549	553	rBV2	401	381	0.02%	0.003%
7	3.179	558	572	587	rBV2	31040	73419	4.13%	0.509%
8	3.353	619	626	635	rBV5	1082	1728	0.10%	0.012%
9	3.391	636	638	644	rVB2	544	387	0.02%	0.003%
10	3.546	683	686	689	rVB	438	301	0.02%	0.002%
11	3.864	769	785	802	rVB2	27644	64644	3.64%	0.448%
12	4.028	831	836	839	rBV	276	303	0.02%	0.002%
13	4.102	855	859	863	rVB2	470	350	0.02%	0.002%
14	4.623	1007	1021	1066	rBV	209882	676952	38.07%	4.695%
15	4.848	1088	1091	1094	rBV4	638	486	0.03%	0.003%
16	5.060	1139	1157	1178	rBV	337624	740160	41.62%	5.133%
17	5.160	1184	1188	1199	rBV6	622	991	0.06%	0.007%
18	5.237	1208	1212	1215	rBV2	493	326	0.02%	0.002%
19	5.256	1215	1218	1220	rBV3	393	274	0.02%	0.002%
20	5.311	1220	1235	1253	rBV2	78951	181519	10.21%	1.259%
21	5.523	1296	1301	1305	rVB3	485	420	0.02%	0.003%
22	5.546	1305	1308	1314	rVB3	361	301	0.02%	0.002%
23	5.578	1314	1318	1319	rBV3	411	323	0.02%	0.002%
24	5.626	1330	1333	1338	rVB2	338	303	0.02%	0.002%
25	5.719	1341	1362	1383	rBV2	662895	1778326	100.00%	12.333%
26	5.964	1432	1438	1439	rBV3	2887	2280	0.13%	0.016%
27	6.086	1472	1476	1481	rBV3	466	453	0.03%	0.003%
28	6.247	1512	1526	1548	rBV	580506	1088868	61.23%	7.551%
29	6.401	1572	1574	1581	rVB4	740	683	0.04%	0.005%
30	6.433	1582	1584	1588	rVB2	591	304	0.02%	0.002%
31	6.536	1603	1616	1630	rBV4	43610	95116	5.35%	0.660%
32	6.687	1649	1663	1685	rBV	440823	850656	47.83%	5.899%
33	6.992	1756	1758	1764	rVB3	341	313	0.02%	0.002%
34	7.047	1765	1775	1776	rBV3	609	802	0.05%	0.006%
35	7.105	1786	1793	1794	rBV2	309	318	0.02%	0.002%
36	7.185	1808	1818	1837	rVV5	5308	11353	0.64%	0.079%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050902.D
 Acq On : 22 Sep 2022 16:51
 Operator : JC/MD
 Sample : N4650-21DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.256	1837	1840	1845	rVB	546	471	0.03%	0.003%
38	7.362	1869	1873	1879	rVB3	274	259	0.01%	0.002%
39	7.472	1904	1907	1910	rBV2	412	308	0.02%	0.002%
40	7.565	1922	1936	1957	rBV	210175	371091	20.87%	2.574%
41	7.793	2003	2007	2008	rVV4	427	310	0.02%	0.002%
42	7.828	2016	2018	2022	rVB3	430	314	0.02%	0.002%
43	7.896	2025	2039	2054	rBV	718428	1218844	68.54%	8.453%
44	7.967	2058	2061	2075	rVB6	9167	16042	0.90%	0.111%
45	8.179	2113	2127	2148	rBV	146744	252415	14.19%	1.751%
46	8.378	2185	2189	2191	rBV2	554	442	0.02%	0.003%
47	8.404	2191	2197	2204	rVB5	2282	2948	0.17%	0.020%
48	8.472	2206	2218	2227	rBV3	2657	4396	0.25%	0.030%
49	8.552	2234	2243	2253	rVB3	23826	39644	2.23%	0.275%
50	8.639	2256	2270	2313	rBV2	614390	1245869	70.06%	8.640%
51	8.783	2313	2315	2318	rBV3	913	686	0.04%	0.005%
52	8.880	2341	2345	2346	rBV2	479	313	0.02%	0.002%
53	8.918	2354	2357	2360	rVB2	633	364	0.02%	0.003%
54	8.957	2366	2369	2371	rVB3	588	314	0.02%	0.002%
55	9.050	2394	2398	2400	rBV3	400	288	0.02%	0.002%
56	9.330	2481	2485	2492	rBV2	348	482	0.03%	0.003%
57	9.417	2498	2512	2536	rBV	788842	1295162	72.83%	8.982%
58	9.571	2553	2560	2562	rBV4	854	895	0.05%	0.006%
59	9.639	2579	2581	2586	rVB2	488	321	0.02%	0.002%
60	9.700	2594	2600	2604	rVB5	846	949	0.05%	0.007%
61	9.844	2642	2645	2650	rVB3	376	362	0.02%	0.003%
62	9.873	2650	2654	2657	rBV	354	257	0.01%	0.002%
63	10.153	2737	2741	2745	rBV2	467	426	0.02%	0.003%
64	10.205	2754	2757	2759	rBV2	400	257	0.01%	0.002%
65	10.324	2788	2794	2797	rBV3	371	404	0.02%	0.003%
66	10.674	2896	2903	2908	rVB5	1499	2161	0.12%	0.015%
67	10.758	2916	2929	2959	rBV	680850	1105035	62.14%	7.664%
68	10.886	2963	2969	2971	rBV2	1372	1346	0.08%	0.009%
69	11.115	3034	3040	3041	rBV3	1353	1221	0.07%	0.008%
70	11.295	3089	3096	3097	rBV	339	311	0.02%	0.002%
71	11.314	3100	3102	3108	rVB4	473	486	0.03%	0.003%
72	11.381	3121	3123	3127	rBV2	568	327	0.02%	0.002%
73	11.436	3137	3140	3142	rBV2	493	319	0.02%	0.002%
74	11.459	3143	3147	3152	rVV4	1007	967	0.05%	0.007%
75	11.513	3161	3164	3167	rBV2	594	312	0.02%	0.002%
76	11.613	3191	3195	3197	rBV2	347	281	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050902.D
 Acq On : 22 Sep 2022 16:51
 Operator : JC/MD
 Sample : N4650-21DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

77	11.812	3243	3257	3275	rBV	657896	1046700	58.86%	7.259%
78	11.931	3291	3294	3298	rBV4	698	680	0.04%	0.005%
79	11.967	3303	3305	3307	rBV3	765	333	0.02%	0.002%
80	12.131	3352	3356	3360	rBV4	525	479	0.03%	0.003%
81	12.192	3362	3375	3397	rBV	695458	1110471	62.44%	7.701%
82	12.375	3430	3432	3434	rVB2	712	317	0.02%	0.002%
83	12.407	3438	3442	3444	rBV2	469	383	0.02%	0.003%
84	12.616	3503	3507	3511	rBV2	560	559	0.03%	0.004%
85	12.719	3536	3539	3544	rVB3	475	377	0.02%	0.003%
86	12.777	3551	3557	3562	rVB4	1092	1129	0.06%	0.008%
87	12.841	3574	3577	3581	rVB3	417	261	0.01%	0.002%
88	13.233	3695	3699	3703	rVB5	709	551	0.03%	0.004%
89	13.336	3729	3731	3735	rBV	404	276	0.02%	0.002%
90	13.391	3743	3748	3755	rVB2	484	733	0.04%	0.005%
91	13.423	3755	3758	3763	rBV3	390	358	0.02%	0.002%
92	13.458	3765	3769	3777	rVB4	791	1101	0.06%	0.008%
93	13.513	3784	3786	3790	rVB3	406	269	0.02%	0.002%
94	13.841	3885	3888	3889	rBV2	664	328	0.02%	0.002%
95	13.941	3917	3919	3922	rVB	578	266	0.01%	0.002%
96	14.201	3997	4000	4002	rBV2	752	460	0.03%	0.003%
97	14.571	4109	4115	4119	rBV4	1182	1418	0.08%	0.010%
98	15.134	4287	4290	4292	rBV2	708	463	0.03%	0.003%
99	15.188	4304	4307	4310	rBV2	608	361	0.02%	0.003%
100	15.307	4341	4344	4345	rBV	818	434	0.02%	0.003%




Sum of corrected areas: 14419283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050902.D
Acq On : 22 Sep 2022 16:51
Operator : JC/MD
Sample : N4650-21DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

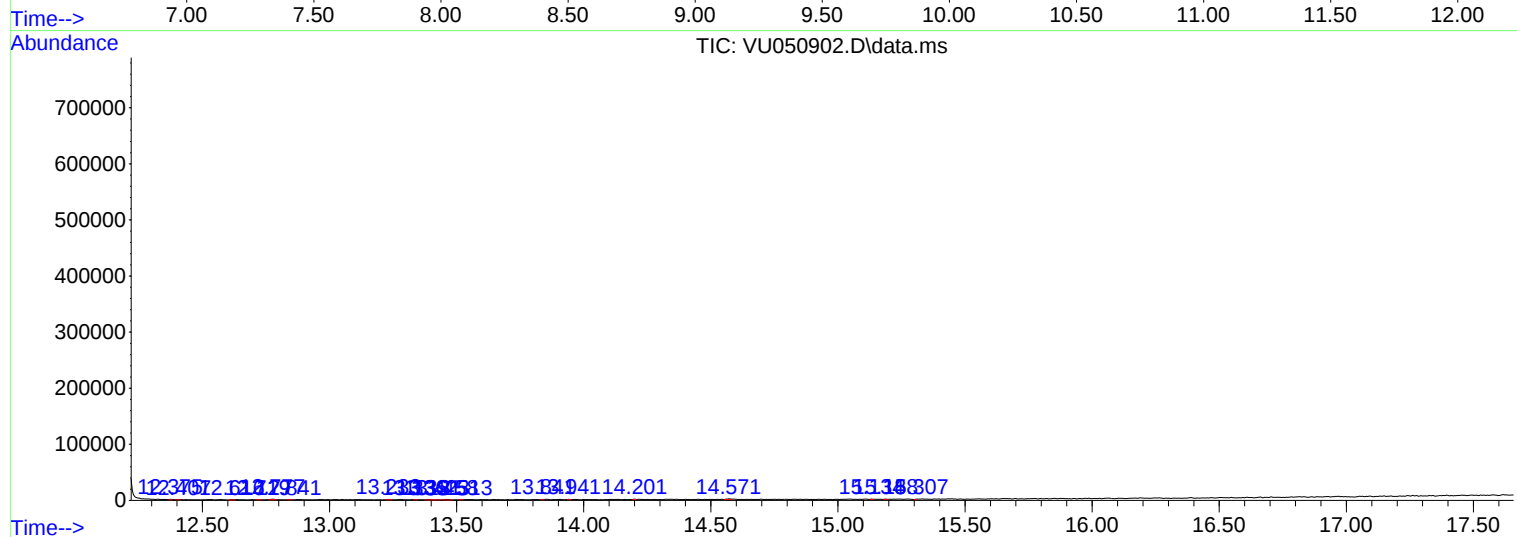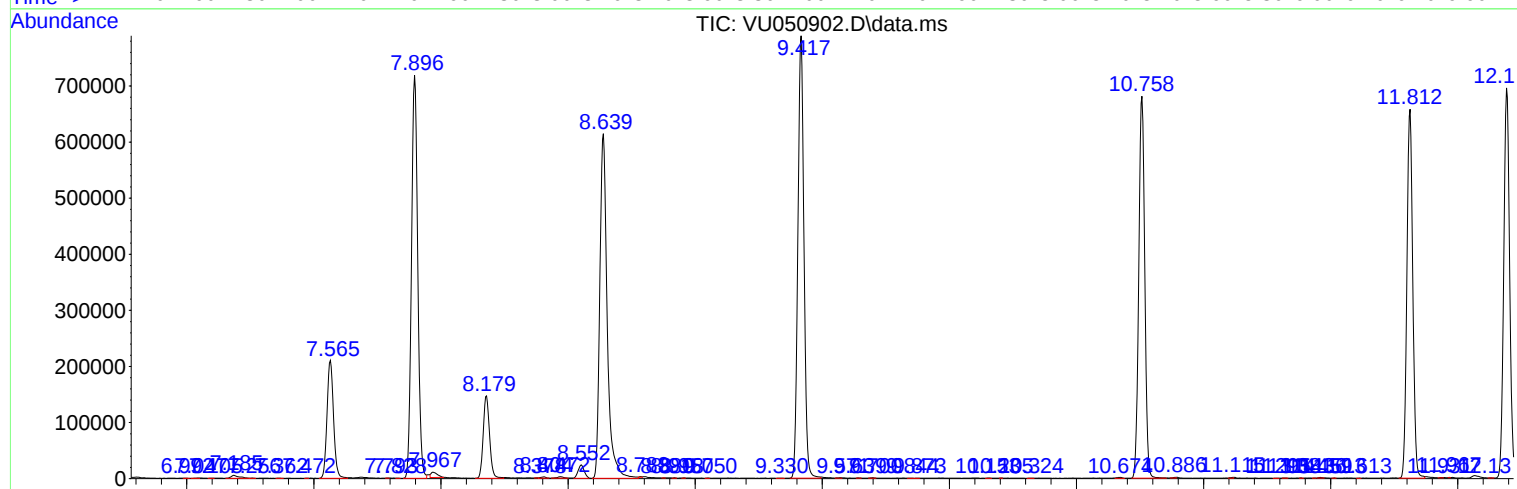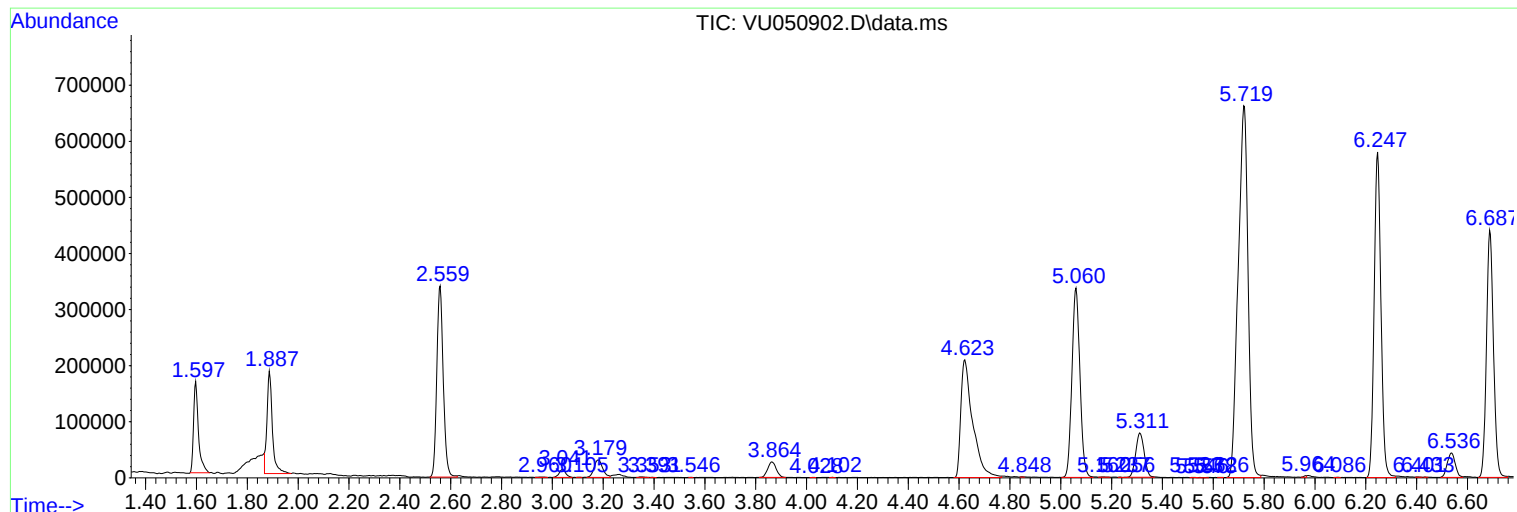

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050902.D
Acq On : 22 Sep 2022 16:51
Operator : JC/MD
Sample : N4650-21DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050902.D
Acq On : 22 Sep 2022 16:51
Operator : JC/MD
Sample : N4650-21DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc