

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050903.D
 Acq On : 22 Sep 2022 17:14
 Operator : JC/MD
 Sample : N4650-17DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ12DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	198852	240523	13.94%	1.741%
2	1.903	167	175	201	rVB2	173891	271663	15.74%	1.966%
3	2.562	368	380	396	rBV	317874	532280	30.84%	3.852%
4	2.765	440	443	444	rBV2	702	393	0.02%	0.003%
5	2.861	469	473	476	rBV3	519	471	0.03%	0.003%
6	2.945	495	499	500	rBV	504	350	0.02%	0.003%
7	3.044	519	530	542	rVB3	6270	10404	0.60%	0.075%
8	3.183	556	573	596	rBV2	31538	77515	4.49%	0.561%
9	3.353	616	626	638	rVB6	2658	4984	0.29%	0.036%
10	3.517	672	677	680	rBV2	426	418	0.02%	0.003%
11	3.732	739	744	749	rBV2	265	368	0.02%	0.003%
12	3.793	759	763	765	rBV3	370	290	0.02%	0.002%
13	3.867	770	786	806	rBV	83921	195123	11.30%	1.412%
14	4.038	837	839	845	rVB2	508	472	0.03%	0.003%
15	4.073	845	850	854	rBV	514	594	0.03%	0.004%
16	4.231	894	899	903	rVB3	350	331	0.02%	0.002%
17	4.256	903	907	912	rBV	311	333	0.02%	0.002%
18	4.356	931	938	943	rVB2	297	388	0.02%	0.003%
19	4.391	943	949	957	rBV2	267	436	0.03%	0.003%
20	4.623	1004	1021	1026	rBV	234159	488491	28.30%	3.535%
21	5.060	1140	1157	1181	rBV	325107	717774	41.59%	5.195%
22	5.195	1196	1199	1202	rBV3	674	471	0.03%	0.003%
23	5.314	1220	1236	1255	rVB3	122817	276845	16.04%	2.004%
24	5.610	1323	1328	1333	rBV3	424	589	0.03%	0.004%
25	5.723	1340	1363	1385	rBV2	635470	1726004	100.00%	12.491%
26	6.031	1453	1459	1460	rBV2	294	280	0.02%	0.002%
27	6.041	1460	1462	1467	rVB2	821	623	0.04%	0.005%
28	6.108	1481	1483	1487	rBV2	346	354	0.02%	0.003%
29	6.247	1511	1526	1547	rBV	550142	1037775	60.13%	7.510%
30	6.369	1562	1564	1568	rVB3	995	522	0.03%	0.004%
31	6.530	1603	1614	1628	rVB5	17703	36481	2.11%	0.264%
32	6.591	1630	1633	1637	rBV2	585	528	0.03%	0.004%
33	6.690	1645	1664	1686	rBV	421621	828418	48.00%	5.995%
34	6.896	1723	1728	1731	rBV3	549	574	0.03%	0.004%
35	6.938	1739	1741	1746	rVB3	479	314	0.02%	0.002%
36	6.964	1746	1749	1754	rBV2	363	447	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050903.D
 Acq On : 22 Sep 2022 17:14
 Operator : JC/MD
 Sample : N4650-17DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ12DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.054	1772	1777	1779	rBV2	421	379	0.02%	0.003%
38	7.186	1811	1818	1829	rVV6	3021	5217	0.30%	0.038%
39	7.565	1923	1936	1954	rBV	204304	359167	20.81%	2.599%
40	7.790	2001	2006	2008	rBV2	631	606	0.04%	0.004%
41	7.896	2025	2039	2054	rBV	677426	1169373	67.75%	8.463%
42	7.967	2055	2061	2077	rVB	18433	36277	2.10%	0.263%
43	8.063	2089	2091	2099	rVB2	764	853	0.05%	0.006%
44	8.179	2115	2127	2149	rBV	142875	245658	14.23%	1.778%
45	8.395	2191	2194	2195	rBV	584	287	0.02%	0.002%
46	8.475	2210	2219	2223	rBV3	689	979	0.06%	0.007%
47	8.520	2230	2233	2235	rVB2	466	306	0.02%	0.002%
48	8.552	2235	2243	2252	rBV4	8595	13646	0.79%	0.099%
49	8.632	2256	2268	2294	rBV2	588097	1139138	66.00%	8.244%
50	8.899	2348	2351	2355	rBV4	297	309	0.02%	0.002%
51	8.980	2372	2376	2377	rBV2	427	282	0.02%	0.002%
52	8.989	2377	2379	2382	rVV	628	345	0.02%	0.002%
53	9.018	2384	2388	2390	rVV2	565	402	0.02%	0.003%
54	9.054	2398	2399	2404	rVB3	366	288	0.02%	0.002%
55	9.144	2422	2427	2431	rBV	482	557	0.03%	0.004%
56	9.195	2436	2443	2445	rBV2	564	416	0.02%	0.003%
57	9.272	2461	2467	2472	rBV	398	480	0.03%	0.003%
58	9.349	2487	2491	2494	rBV2	355	346	0.02%	0.003%
59	9.417	2498	2512	2539	rBV	776422	1268205	73.48%	9.178%
60	9.571	2552	2560	2569	rVB3	4863	7585	0.44%	0.055%
61	9.694	2588	2598	2612	rVV2	9606	16123	0.93%	0.117%
62	9.745	2612	2614	2623	rVB2	538	515	0.03%	0.004%
63	9.964	2679	2682	2687	rBV3	373	309	0.02%	0.002%
64	10.099	2714	2724	2734	rBV3	9103	14895	0.86%	0.108%
65	10.198	2753	2755	2759	rVB	416	314	0.02%	0.002%
66	10.343	2795	2800	2805	rBV2	364	379	0.02%	0.003%
67	10.478	2837	2842	2847	rBV2	482	644	0.04%	0.005%
68	10.661	2894	2899	2901	rBV3	1065	956	0.06%	0.007%
69	10.755	2915	2928	2948	rBV	641789	1018142	58.99%	7.368%
70	10.890	2966	2970	2973	rBV4	962	889	0.05%	0.006%
71	10.957	2987	2991	2995	rBV3	482	423	0.02%	0.003%
72	10.996	2995	3003	3010	rBV3	4191	7384	0.43%	0.053%
73	11.086	3024	3031	3038	rBV3	5143	7889	0.46%	0.057%
74	11.292	3087	3095	3108	rBV3	6249	9205	0.53%	0.067%
75	11.372	3117	3120	3123	rVB2	547	332	0.02%	0.002%
76	11.414	3130	3133	3137	rVB2	619	445	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050903.D
 Acq On : 22 Sep 2022 17:14
 Operator : JC/MD
 Sample : N4650-17DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ12DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

77	11.468	3140	3150	3159	rVV	13443	20354	1.18%	0.147%
78	11.578	3182	3184	3191	rVB3	435	385	0.02%	0.003%
79	11.742	3231	3235	3243	rVB4	925	928	0.05%	0.007%
80	11.809	3243	3256	3272	rBV	591941	951684	55.14%	6.887%
81	11.893	3276	3282	3292	rVB2	10682	16843	0.98%	0.122%
82	11.970	3303	3306	3310	rVB3	1056	887	0.05%	0.006%
83	12.073	3331	3338	3339	rBV3	1713	1341	0.08%	0.010%
84	12.095	3340	3345	3351	rVB4	3377	4026	0.23%	0.029%
85	12.192	3362	3375	3396	rBV	617847	1003120	58.12%	7.260%
86	12.478	3455	3464	3476	rBV2	14820	24887	1.44%	0.180%
87	12.639	3510	3514	3516	rBV3	593	486	0.03%	0.004%
88	12.758	3549	3551	3554	rBV	497	320	0.02%	0.002%
89	12.812	3564	3568	3573	rBV3	528	586	0.03%	0.004%
90	12.922	3599	3602	3607	rBV2	338	339	0.02%	0.002%
91	13.025	3629	3634	3636	rBV	822	764	0.04%	0.006%
92	13.082	3646	3652	3656	rBV3	760	973	0.06%	0.007%
93	13.105	3656	3659	3666	rVV3	644	837	0.05%	0.006%
94	13.266	3705	3709	3712	rBV	441	450	0.03%	0.003%
95	13.301	3717	3720	3722	rBV	431	298	0.02%	0.002%
96	13.346	3730	3734	3737	rBV	776	686	0.04%	0.005%
97	13.452	3763	3767	3775	rVB3	1118	1090	0.06%	0.008%
98	14.095	3962	3967	3976	rBV4	1085	1724	0.10%	0.012%
99	15.272	4330	4333	4335	rBV2	694	540	0.03%	0.004%
100	15.423	4378	4380	4385	rBV4	575	603	0.03%	0.004%




Sum of corrected areas: 13817922

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050903.D
Acq On : 22 Sep 2022 17:14
Operator : JC/MD
Sample : N4650-17DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ12DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

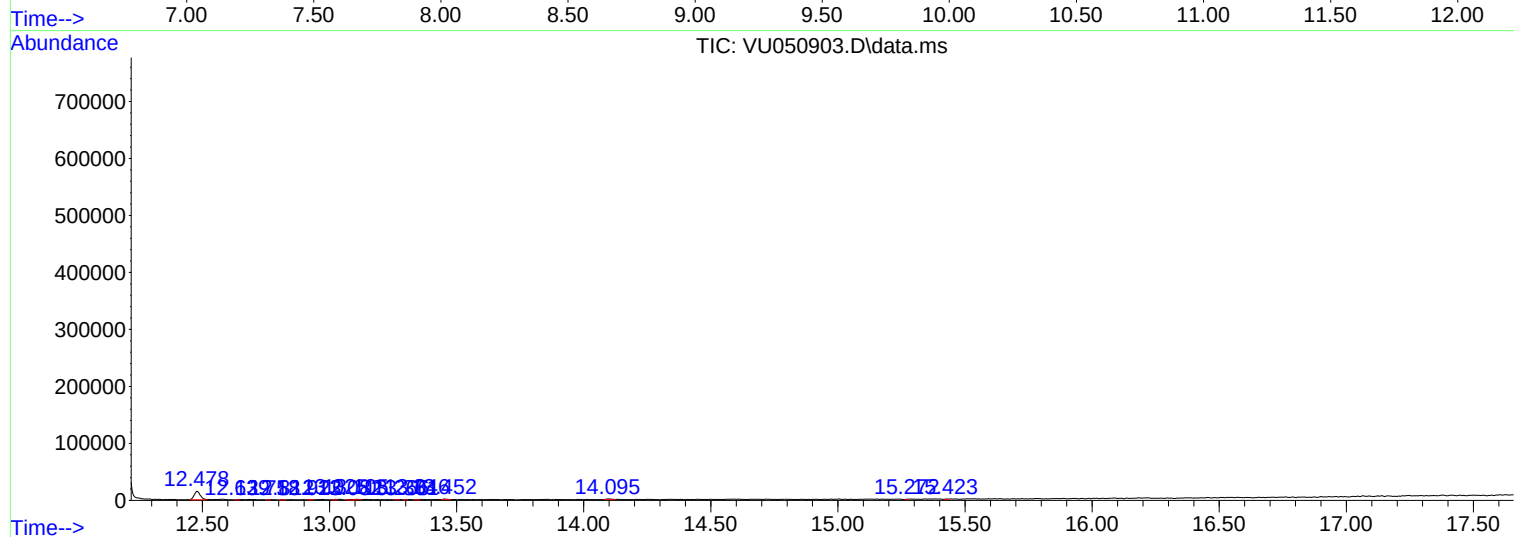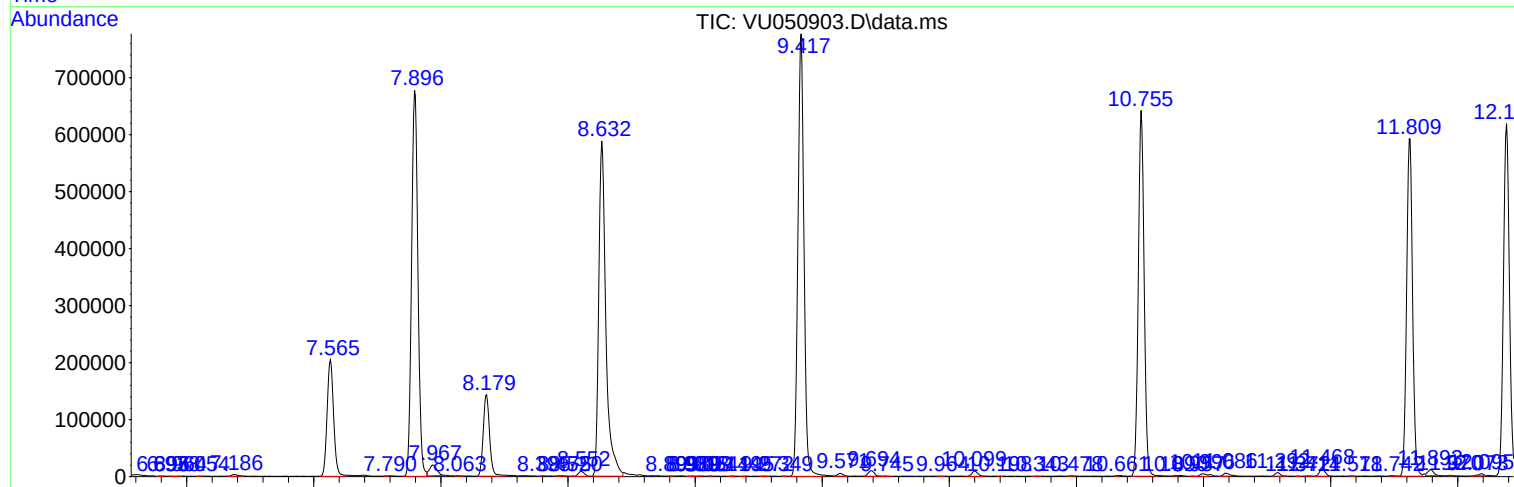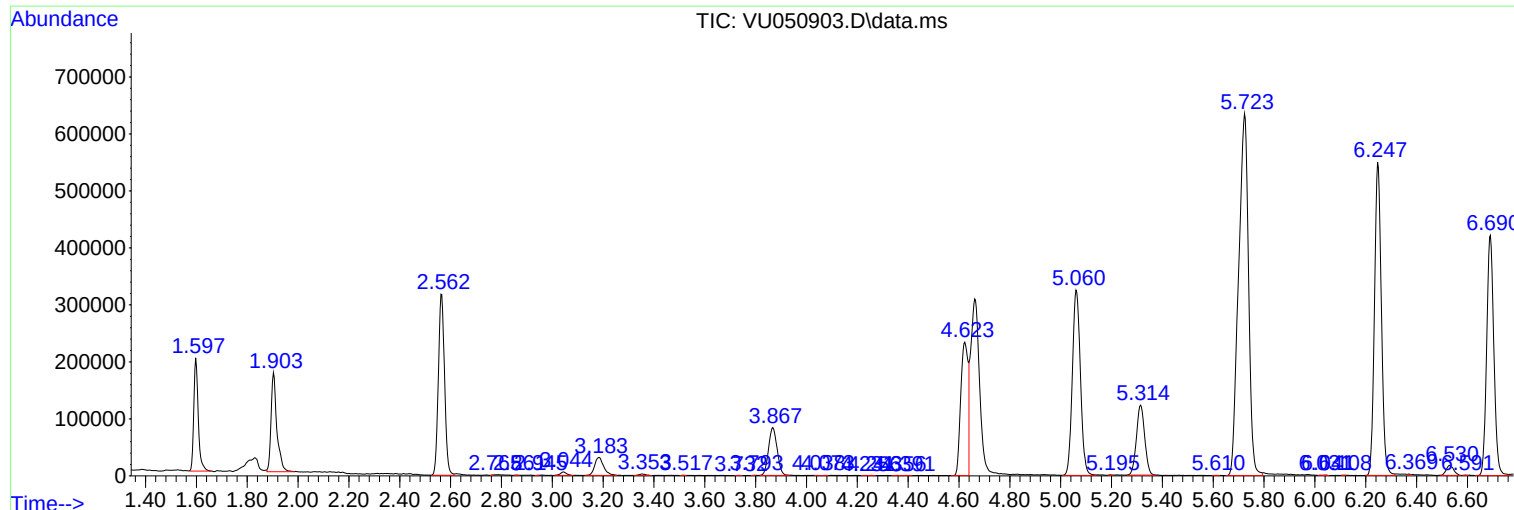

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050903.D
Acq On : 22 Sep 2022 17:14
Operator : JC/MD
Sample : N4650-17DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ12DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050903.D
Acq On : 22 Sep 2022 17:14
Operator : JC/MD
Sample : N4650-17DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ12DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------