

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050904.D
 Acq On : 22 Sep 2022 17:38
 Operator : JC/MD
 Sample : N4747-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	182012	218490	13.74%	1.805%
2	1.906	169	176	194	rVB	177720	237350	14.93%	1.961%
3	2.565	368	381	398	rBV	299427	497067	31.27%	4.108%
4	2.748	432	438	440	rBV4	366	428	0.03%	0.004%
5	2.822	458	461	463	rBV4	634	321	0.02%	0.003%
6	2.838	463	466	468	rVB2	413	270	0.02%	0.002%
7	2.883	477	480	484	rVB4	700	549	0.03%	0.005%
8	3.044	522	530	539	rVB4	1944	3303	0.21%	0.027%
9	3.182	564	573	576	rBV2	1229	1499	0.09%	0.012%
10	3.411	641	644	650	rVB3	307	254	0.02%	0.002%
11	3.597	696	702	707	rBV2	442	515	0.03%	0.004%
12	3.649	712	718	726	rBV2	403	571	0.04%	0.005%
13	3.867	783	786	793	rVV3	557	504	0.03%	0.004%
14	3.951	806	812	818	rBV2	359	461	0.03%	0.004%
15	4.002	823	828	832	rVB2	281	299	0.02%	0.002%
16	4.028	832	836	839	rBV	392	359	0.02%	0.003%
17	4.259	905	908	913	rBV2	339	320	0.02%	0.003%
18	4.414	951	956	959	rVB2	350	369	0.02%	0.003%
19	4.623	1009	1021	1062	rBV	208444	544645	34.26%	4.501%
20	4.880	1098	1101	1103	rBV2	462	316	0.02%	0.003%
21	5.063	1140	1158	1181	rBV	303568	666475	41.93%	5.507%
22	5.295	1228	1230	1236	rVB4	990	800	0.05%	0.007%
23	5.369	1247	1253	1258	rBV5	835	870	0.05%	0.007%
24	5.446	1274	1277	1279	rBV	379	270	0.02%	0.002%
25	5.533	1301	1304	1310	rVB3	407	427	0.03%	0.004%
26	5.722	1341	1363	1384	rBV2	578464	1589661	100.00%	13.136%
27	5.976	1438	1442	1451	rVB6	1069	1351	0.08%	0.011%
28	6.246	1512	1526	1546	rBV	498146	949922	59.76%	7.850%
29	6.529	1603	1614	1630	rVB3	12697	24862	1.56%	0.205%
30	6.591	1630	1633	1635	rBV	545	351	0.02%	0.003%
31	6.690	1649	1664	1689	rVV	394482	766461	48.22%	6.334%
32	6.909	1729	1732	1735	rVV2	360	270	0.02%	0.002%
33	7.005	1757	1762	1769	rBV2	359	493	0.03%	0.004%
34	7.041	1769	1773	1777	rVV2	395	417	0.03%	0.003%
35	7.063	1777	1780	1784	rVV2	616	594	0.04%	0.005%
36	7.189	1811	1819	1830	rVV5	2487	4714	0.30%	0.039%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050904.D
 Acq On : 22 Sep 2022 17:38
 Operator : JC/MD
 Sample : N4747-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.404	1883	1886	1888	rBV	376	307	0.02%	0.003%
38	7.565	1923	1936	1955	rBV	183799	327301	20.59%	2.705%
39	7.690	1970	1975	1993	rVB6	2154	4512	0.28%	0.037%
40	7.896	2025	2039	2055	rBV	615578	1061040	66.75%	8.768%
41	8.050	2085	2087	2091	rVB4	533	352	0.02%	0.003%
42	8.124	2108	2110	2115	rVB3	750	510	0.03%	0.004%
43	8.179	2115	2127	2151	rBV	132580	228686	14.39%	1.890%
44	8.388	2189	2192	2195	rBV3	401	258	0.02%	0.002%
45	8.426	2202	2204	2209	rVB4	332	277	0.02%	0.002%
46	8.468	2209	2217	2232	rVB2	1878	3589	0.23%	0.030%
47	8.526	2232	2235	2238	rBV3	369	241	0.02%	0.002%
48	8.549	2240	2242	2246	rBV3	404	316	0.02%	0.003%
49	8.632	2256	2268	2308	rBV2	559393	1132044	71.21%	9.355%
50	8.848	2332	2335	2340	rBV4	822	719	0.05%	0.006%
51	8.896	2348	2350	2353	rVB	553	321	0.02%	0.003%
52	8.986	2376	2378	2381	rBV2	411	251	0.02%	0.002%
53	9.060	2398	2401	2405	rBV2	512	397	0.02%	0.003%
54	9.153	2427	2430	2434	rVB	381	319	0.02%	0.003%
55	9.198	2440	2444	2449	rBV2	495	395	0.02%	0.003%
56	9.224	2449	2452	2456	rBV2	485	356	0.02%	0.003%
57	9.298	2469	2475	2479	rBV2	426	469	0.03%	0.004%
58	9.417	2498	2512	2540	rBV	688285	1144158	71.97%	9.455%
59	9.542	2547	2551	2554	rVB2	626	474	0.03%	0.004%
60	9.571	2554	2560	2565	rVB4	848	799	0.05%	0.007%
61	9.693	2593	2598	2600	rBV3	623	490	0.03%	0.004%
62	9.825	2635	2639	2643	rVV3	413	367	0.02%	0.003%
63	9.860	2648	2650	2654	rVB	300	243	0.02%	0.002%
64	10.092	2720	2722	2724	rBV	507	255	0.02%	0.002%
65	10.176	2745	2748	2753	rVB2	306	297	0.02%	0.002%
66	10.385	2810	2813	2816	rBV2	369	242	0.02%	0.002%
67	10.668	2897	2901	2909	rVB4	1034	1266	0.08%	0.010%
68	10.754	2909	2928	2950	rBV	588513	956425	60.17%	7.903%
69	10.851	2955	2958	2961	rVV2	537	365	0.02%	0.003%
70	10.867	2961	2963	2965	rVV2	517	310	0.02%	0.003%
71	10.889	2966	2970	2977	rVB5	1431	1871	0.12%	0.015%
72	11.040	3014	3017	3025	rVB3	379	277	0.02%	0.002%
73	11.089	3028	3032	3035	rBV3	540	397	0.02%	0.003%
74	11.311	3099	3101	3105	rBV	608	382	0.02%	0.003%
75	11.696	3218	3221	3226	rVB3	569	549	0.03%	0.005%
76	11.751	3231	3238	3241	rVB3	446	472	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050904.D
 Acq On : 22 Sep 2022 17:38
 Operator : JC/MD
 Sample : N4747-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.809	3244	3256	3283	rBV	499943	797367	50.16%	6.589%
78	12.063	3325	3335	3353	rBV3	18476	36912	2.32%	0.305%
79	12.192	3362	3375	3394	rBV	534233	869011	54.67%	7.181%
80	12.391	3434	3437	3440	rBV2	399	245	0.02%	0.002%
81	12.471	3456	3462	3465	rBV4	736	809	0.05%	0.007%
82	12.552	3484	3487	3491	rVB2	613	441	0.03%	0.004%
83	12.584	3492	3497	3499	rBV	450	395	0.02%	0.003%
84	12.671	3520	3524	3529	rVB3	501	493	0.03%	0.004%
85	12.764	3550	3553	3554	rBV	646	380	0.02%	0.003%
86	12.886	3588	3591	3592	rBV	1206	608	0.04%	0.005%
87	13.056	3642	3644	3647	rVB	556	275	0.02%	0.002%
88	13.150	3668	3673	3676	rBV2	340	357	0.02%	0.003%
89	13.166	3676	3678	3681	rBV2	444	250	0.02%	0.002%
90	13.220	3693	3695	3701	rVB4	666	523	0.03%	0.004%
91	13.394	3746	3749	3753	rBV3	412	315	0.02%	0.003%
92	13.468	3768	3772	3777	rBV2	538	654	0.04%	0.005%
93	13.671	3832	3835	3837	rBV	363	249	0.02%	0.002%
94	13.844	3887	3889	3891	rBV2	538	299	0.02%	0.002%
95	14.024	3943	3945	3953	rVB4	545	503	0.03%	0.004%
96	14.812	4186	4190	4193	rBV2	518	494	0.03%	0.004%
97	15.224	4311	4318	4321	rBV3	999	1275	0.08%	0.011%
98	15.417	4376	4378	4382	rBV2	830	417	0.03%	0.003%
99	15.664	4453	4455	4457	rBV3	855	422	0.03%	0.003%
100	15.873	4518	4520	4523	rBV3	939	596	0.04%	0.005%




Sum of corrected areas: 12101417

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050904.D
Acq On : 22 Sep 2022 17:38
Operator : JC/MD
Sample : N4747-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

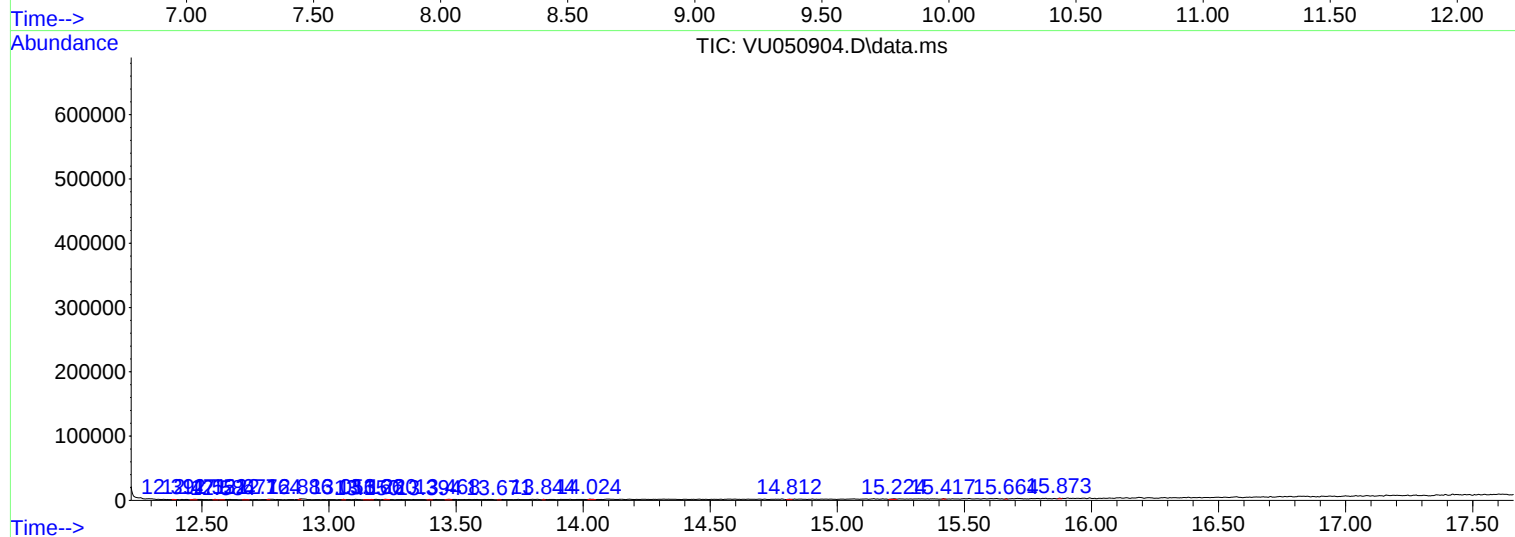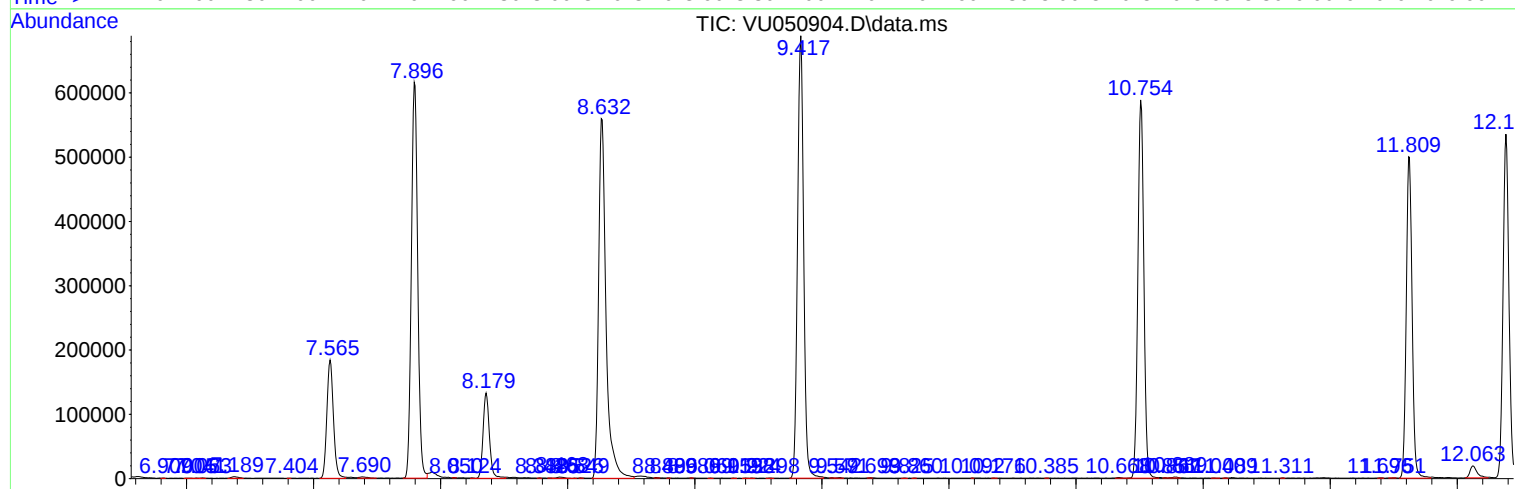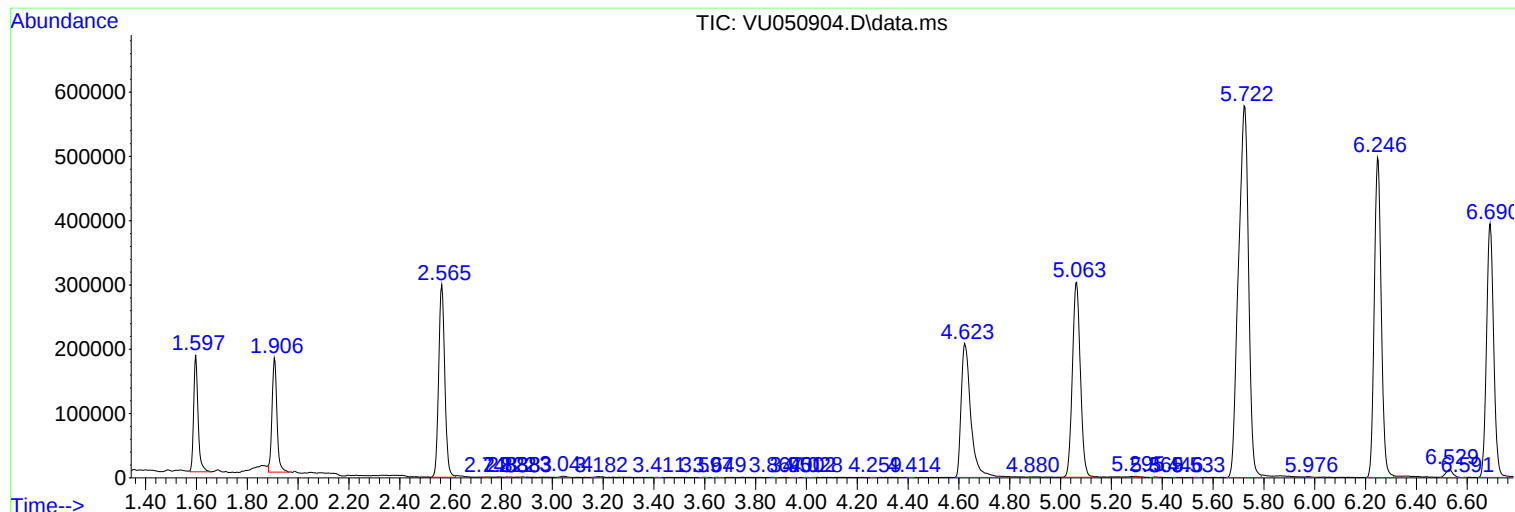

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050904.D
Acq On : 22 Sep 2022 17:38
Operator : JC/MD
Sample : N4747-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050904.D
Acq On : 22 Sep 2022 17:38
Operator : JC/MD
Sample : N4747-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc