

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050908.D
 Acq On : 22 Sep 2022 19:12
 Operator : JC/MD
 Sample : N4747-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	235115	276648	15.94%	1.985%
2	1.906	169	176	193	rVB	185089	243466	14.03%	1.747%
3	2.565	368	381	396	rBV	350832	575222	33.14%	4.127%
4	3.041	523	529	531	rBV3	1558	1673	0.10%	0.012%
5	3.150	560	563	564	rBV2	283	142	0.01%	0.001%
6	3.269	597	600	603	rBV2	327	243	0.01%	0.002%
7	3.356	617	627	639	rVB4	3206	6688	0.39%	0.048%
8	3.408	641	643	645	rVV	185	93	0.01%	0.001%
9	3.427	646	649	654	rVB3	282	244	0.01%	0.002%
10	3.478	663	665	667	rBV	161	65	0.00%	0.000%
11	3.517	671	677	683	rBV3	478	653	0.04%	0.005%
12	3.578	693	696	697	rBV	215	104	0.01%	0.001%
13	3.591	697	700	701	rBV	256	150	0.01%	0.001%
14	3.652	716	719	720	rBV2	288	173	0.01%	0.001%
15	3.681	726	728	729	rBV	306	136	0.01%	0.001%
16	3.768	752	755	758	rBV	219	159	0.01%	0.001%
17	3.806	765	767	772	rVB2	349	187	0.01%	0.001%
18	3.854	780	782	784	rBV3	243	137	0.01%	0.001%
19	3.970	815	818	821	rBV2	217	137	0.01%	0.001%
20	4.170	878	880	883	rBV	159	86	0.00%	0.001%
21	4.231	896	899	901	rBV2	167	104	0.01%	0.001%
22	4.282	912	915	918	rBV	333	195	0.01%	0.001%
23	4.327	927	929	930	rBV	200	94	0.01%	0.001%
24	4.395	947	950	951	rBV	216	122	0.01%	0.001%
25	4.427	957	960	962	rBV2	264	175	0.01%	0.001%
26	4.469	968	973	976	rBV2	218	232	0.01%	0.002%
27	4.530	988	992	995	rBV	356	284	0.02%	0.002%
28	4.620	1007	1020	1029	rBV	200663	468877	27.01%	3.364%
29	5.060	1140	1157	1177	rBV	311895	685212	39.48%	4.916%
30	5.456	1276	1280	1283	rBV2	244	187	0.01%	0.001%
31	5.475	1283	1286	1291	rVB2	219	199	0.01%	0.001%
32	5.497	1291	1293	1294	rBV	61	33	0.00%	0.000%
33	5.514	1294	1298	1301	rBV2	393	306	0.02%	0.002%
34	5.559	1310	1312	1317	rVB	326	165	0.01%	0.001%
35	5.581	1317	1319	1326	rVB	265	256	0.01%	0.002%
36	5.610	1326	1328	1329	rBV	110	49	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050908.D
 Acq On : 22 Sep 2022 19:12
 Operator : JC/MD
 Sample : N4747-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	5.639	1334	1337	1341	rBV2	195	156	0.01%	0.001%
38	5.723	1341	1363	1390	rBV2	645886	1735780	100.00%	12.454%
39	6.128	1487	1489	1494	rVB3	504	278	0.02%	0.002%
40	6.173	1499	1503	1508	rBV3	547	455	0.03%	0.003%
41	6.198	1508	1511	1512	rBV	354	159	0.01%	0.001%
42	6.247	1512	1526	1548	rBV	537723	1005511	57.93%	7.214%
43	6.539	1602	1617	1639	rBV	553203	1050774	60.54%	7.539%
44	6.690	1651	1664	1682	rVB	415863	799684	46.07%	5.738%
45	7.044	1770	1774	1780	rBV3	575	562	0.03%	0.004%
46	7.108	1792	1794	1798	rVB	174	50	0.00%	0.000%
47	7.179	1812	1816	1817	rBV2	1298	960	0.06%	0.007%
48	7.250	1835	1838	1840	rBV2	311	228	0.01%	0.002%
49	7.359	1870	1872	1875	rBV	188	121	0.01%	0.001%
50	7.414	1885	1889	1891	rBV	305	215	0.01%	0.002%
51	7.430	1891	1894	1895	rBV	137	59	0.00%	0.000%
52	7.497	1912	1915	1918	rBV2	170	143	0.01%	0.001%
53	7.565	1923	1936	1954	rBV	204888	360022	20.74%	2.583%
54	7.777	1997	2002	2004	rBV3	595	497	0.03%	0.004%
55	7.896	2025	2039	2054	rBV	728819	1252355	72.15%	8.986%
56	8.131	2110	2112	2113	rBV	320	153	0.01%	0.001%
57	8.176	2114	2126	2142	rVV	145411	249791	14.39%	1.792%
58	8.552	2239	2243	2247	rBV3	828	628	0.04%	0.005%
59	8.632	2256	2268	2307	rBV2	539179	1050782	60.54%	7.539%
60	8.867	2339	2341	2345	rVB4	521	350	0.02%	0.003%
61	8.931	2359	2361	2364	rVB	388	142	0.01%	0.001%
62	8.951	2364	2367	2369	rBV2	445	254	0.01%	0.002%
63	8.967	2369	2372	2374	rBV2	300	177	0.01%	0.001%
64	9.057	2398	2400	2402	rBV2	387	204	0.01%	0.001%
65	9.092	2410	2411	2413	rBV2	204	75	0.00%	0.001%
66	9.111	2413	2417	2420	rBV2	599	399	0.02%	0.003%
67	9.160	2424	2432	2434	rBV3	444	436	0.03%	0.003%
68	9.192	2440	2442	2445	rBV2	295	148	0.01%	0.001%
69	9.214	2445	2449	2452	rBV	348	225	0.01%	0.002%
70	9.256	2458	2462	2465	rBV	246	197	0.01%	0.001%
71	9.275	2466	2468	2470	rBV2	215	86	0.00%	0.001%
72	9.314	2477	2480	2482	rBV	358	205	0.01%	0.001%
73	9.417	2497	2512	2548	rBV	733795	1211237	69.78%	8.691%
74	9.693	2588	2598	2606	rBV6	1476	2422	0.14%	0.017%
75	9.841	2641	2644	2648	rBV3	554	429	0.02%	0.003%
76	9.964	2678	2682	2683	rBV	367	234	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050908.D
 Acq On : 22 Sep 2022 19:12
 Operator : JC/MD
 Sample : N4747-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	10.005	2692	2695	2698	rBV	413	269	0.02%	0.002%
78	10.063	2709	2713	2717	rBV2	387	365	0.02%	0.003%
79	10.279	2777	2780	2782	rBV2	371	221	0.01%	0.002%
80	10.304	2785	2788	2791	rBV2	294	201	0.01%	0.001%
81	10.472	2838	2840	2842	rBV	345	214	0.01%	0.002%
82	10.636	2888	2891	2894	rBV2	406	308	0.02%	0.002%
83	10.664	2895	2900	2912	rVB7	1964	3084	0.18%	0.022%
84	10.754	2915	2928	2948	rBV	597292	940620	54.19%	6.749%
85	11.025	3005	3012	3013	rBV2	814	942	0.05%	0.007%
86	11.227	3072	3075	3081	rBV2	333	322	0.02%	0.002%
87	11.256	3081	3084	3087	rBV2	363	274	0.02%	0.002%
88	11.295	3090	3096	3098	rBV3	774	909	0.05%	0.007%
89	11.465	3141	3149	3166	rVB4	9054	14992	0.86%	0.108%
90	11.648	3203	3206	3212	rBV3	563	514	0.03%	0.004%
91	11.809	3244	3256	3277	rBV	573357	921157	53.07%	6.609%
92	12.015	3317	3320	3321	rBV2	481	289	0.02%	0.002%
93	12.063	3327	3335	3352	rBV2	19745	37608	2.17%	0.270%
94	12.192	3363	3375	3396	rVB	631300	1024736	59.04%	7.352%
95	12.555	3484	3488	3490	rBV4	803	607	0.03%	0.004%
96	13.253	3703	3705	3707	rBV2	605	326	0.02%	0.002%




Sum of corrected areas: 13937437

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050908.D
Acq On : 22 Sep 2022 19:12
Operator : JC/MD
Sample : N4747-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

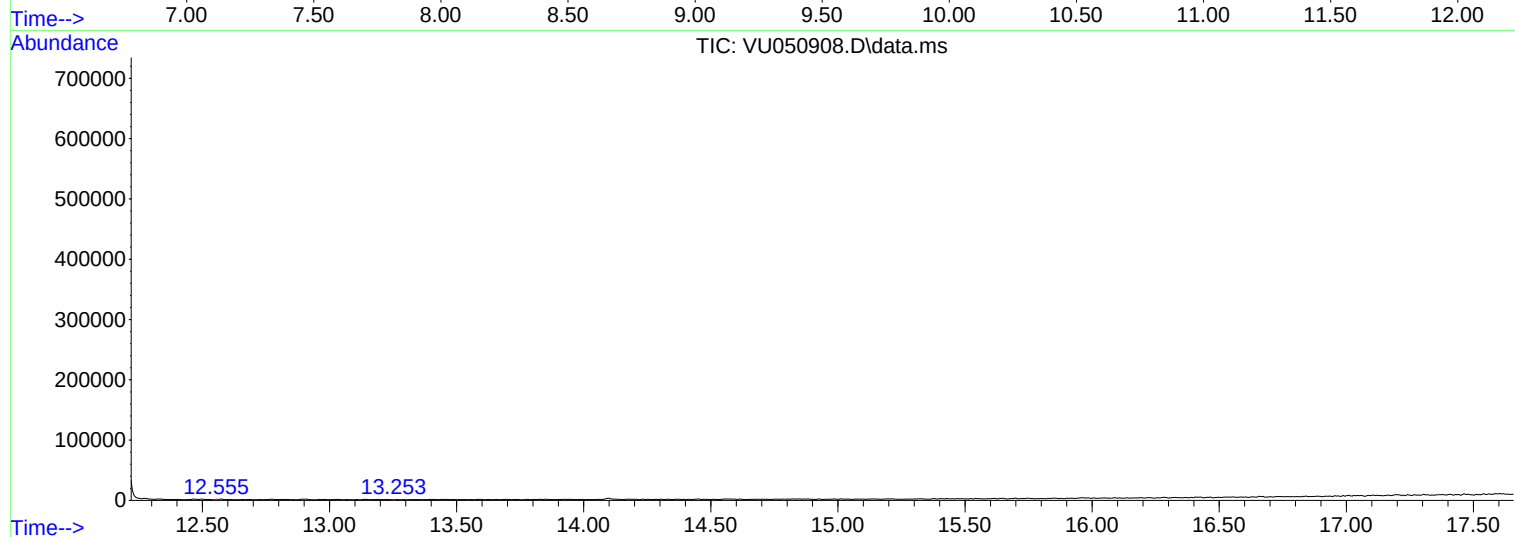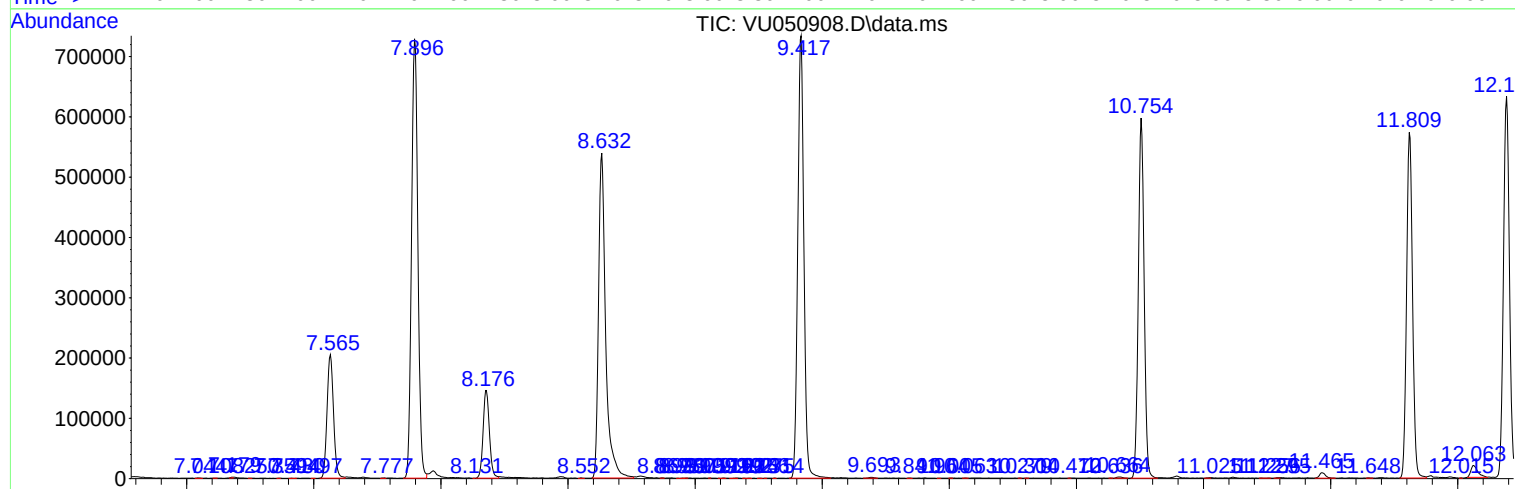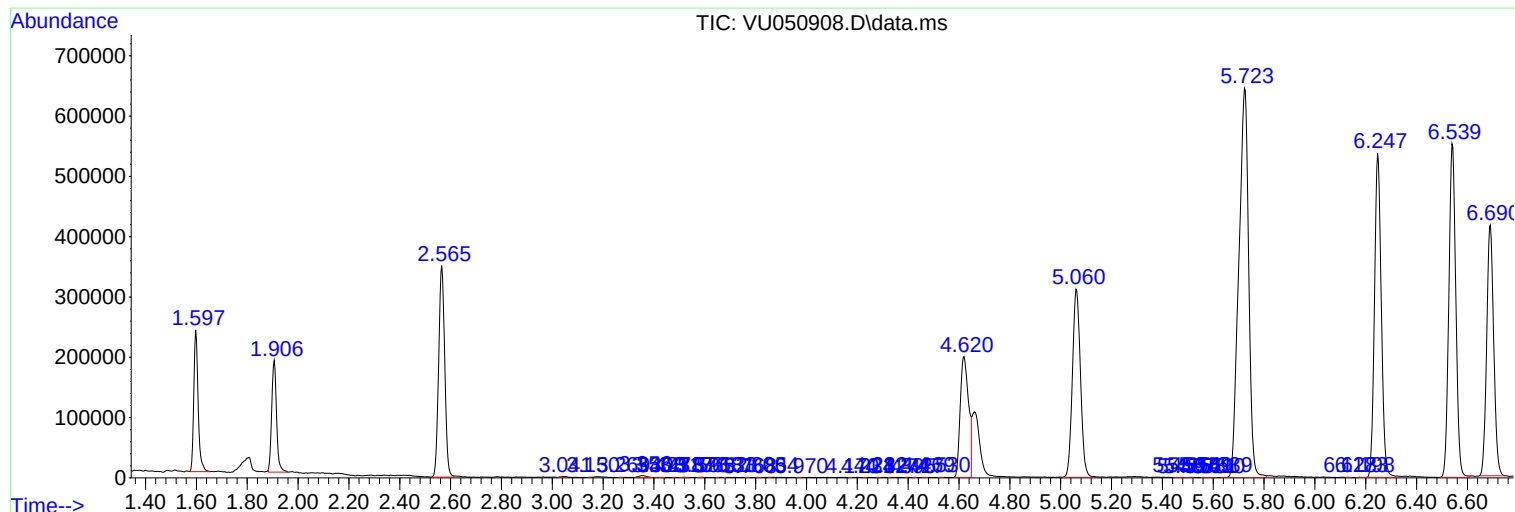

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050908.D
Acq On : 22 Sep 2022 19:12
Operator : JC/MD
Sample : N4747-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
Data File : VU050908.D
Acq On : 22 Sep 2022 19:12
Operator : JC/MD
Sample : N4747-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45A5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc