


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092222\
 Data File : VU050888.D
 Acq On : 22 Sep 2022 09:24
 Operator : JC/MD
 Sample : BFB129
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB129

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis
 Last Update : Mon Sep 26 20:52:47 2022

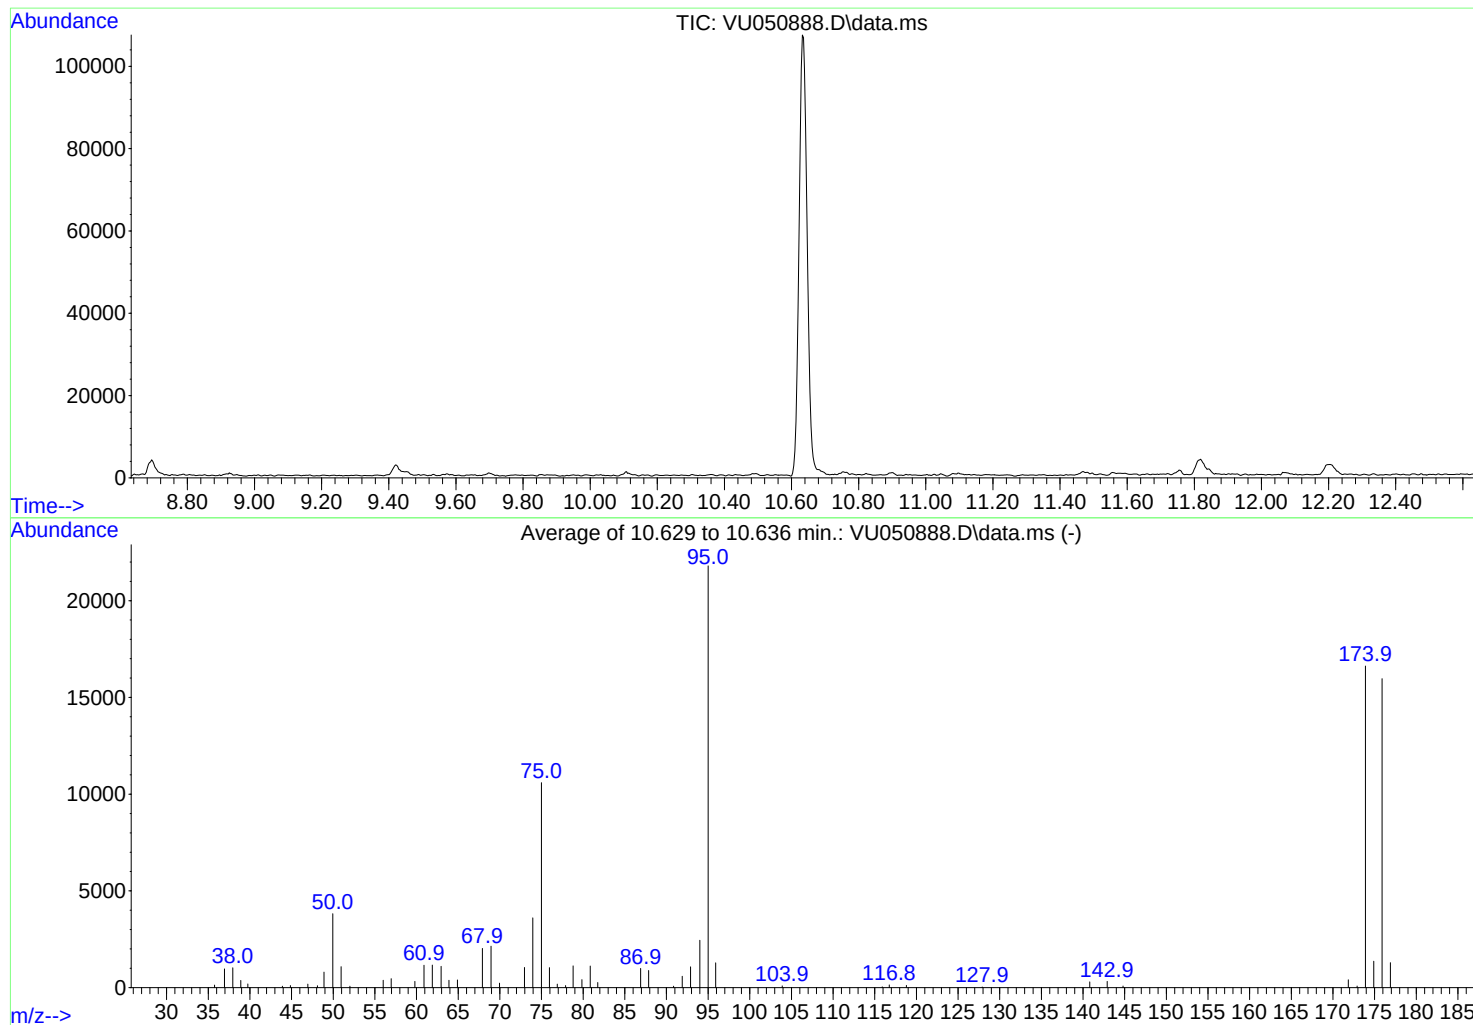

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	3819	PASS
75	95	30	80	48.6	10590	PASS
95	95	100	100	100.0	21800	PASS
96	95	5	9	5.9	1280	PASS
173	174	0.00	2	0.5	83	PASS
174	95	50	120	76.3	16625	PASS
175	174	5	9	8.2	1364	PASS
176	174	95	101	96.0	15968	PASS
177	176	5	9	8.1	1287	PASS

m/z	Abundance
44.00	448.0

Instrument :
MSVOA_U
ClientSampleId :
BFB129

m/z	Abundance
35.70	114.0
37.00	954.0
37.90	930.0
38.90	318.0
39.70	225.0
43.90	627.0
44.80	169.0
46.90	146.0
48.90	754.0
49.90	3860.0
50.90	1061.0
52.00	109.0
56.00	355.0
56.90	475.0
59.80	262.0
60.90	1022.0
61.90	1184.0
63.00	1182.0
63.90	356.0
64.90	367.0
67.90	1947.0
69.00	2137.0
69.90	221.0
72.90	1093.0
73.90	3479.0
75.00	10171.0
75.90	1054.0
76.90	168.0
78.80	1036.0
79.90	339.0
80.90	971.0
81.70	280.0
86.90	898.0
87.90	787.0
90.80	115.0
91.90	604.0
92.90	1131.0
94.00	2368.0
95.00	20528.0
95.90	1200.0
115.90	130.0
116.80	180.0
127.90	101.0
140.80	347.0
142.90	346.0
171.90	395.0
173.90	15491.0
174.90	1376.0
175.90	14825.0
176.90	1194.0

Instrument :
MSVOA_U
ClientSampleId :
BFB129

m/z	Abundance
35.80	133.0
37.00	990.0
37.90	1064.0
38.90	384.0
39.70	181.0
43.90	497.0
44.90	147.0
47.00	188.0
48.10	127.0
48.90	806.0
50.00	3937.0
51.00	1120.0
52.00	112.0
56.00	396.0
56.90	443.0
59.80	351.0
60.90	1169.0
61.90	1219.0
63.00	1106.0
63.90	395.0
64.90	392.0
67.90	2047.0
68.90	2207.0
70.00	248.0
72.90	1091.0
74.00	3682.0
75.00	10929.0
75.90	1040.0
76.90	190.0
77.90	145.0
78.80	1181.0
79.90	418.0
80.90	1147.0
81.70	262.0
86.90	1083.0
87.80	924.0
90.90	111.0
91.90	602.0
92.90	1089.0
94.00	2515.0
95.00	22440.0
95.90	1298.0
103.90	133.0
116.70	141.0
118.80	144.0
140.80	303.0
142.90	322.0
144.80	123.0
171.80	422.0
173.90	17088.0
174.90	1397.0
175.90	16358.0
176.90	1349.0

Instrument :
MSVOA_U
ClientSampleId :
BFB129

m/z	Abundance
35.80	159.0
36.90	966.0
38.00	1073.0
38.90	427.0
39.80	165.0
43.90	452.0
47.00	225.0
48.10	166.0
48.90	853.0
50.00	3661.0
51.00	1073.0
56.00	391.0
57.00	461.0
59.80	358.0
60.90	1281.0
61.90	1095.0
62.90	1003.0
63.90	384.0
64.90	444.0
67.90	2097.0
68.90	2071.0
70.00	226.0
73.00	947.0
74.00	3651.0
75.00	10670.0
76.00	998.0
76.90	187.0
77.90	171.0
78.80	1147.0
79.80	472.0
80.80	1229.0
81.80	254.0
86.90	986.0
87.80	937.0
91.90	557.0
92.90	1014.0
94.00	2461.0
95.00	22432.0
95.90	1342.0
103.90	140.0
116.70	111.0
118.80	201.0
140.80	237.0
142.90	299.0
144.80	131.0
171.80	403.0
172.90	250.0
173.90	17296.0
174.90	1319.0
175.90	16720.0
176.90	1318.0

Instrument :
MSVOA_U
ClientSampleId :
BFB129