


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092223\
Data File : VU055452.D
Acq On : 22 Sep 2023 11:56
Operator : MD/SY
Sample : BFB050
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB050

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Sep 25 01:08:17 2023

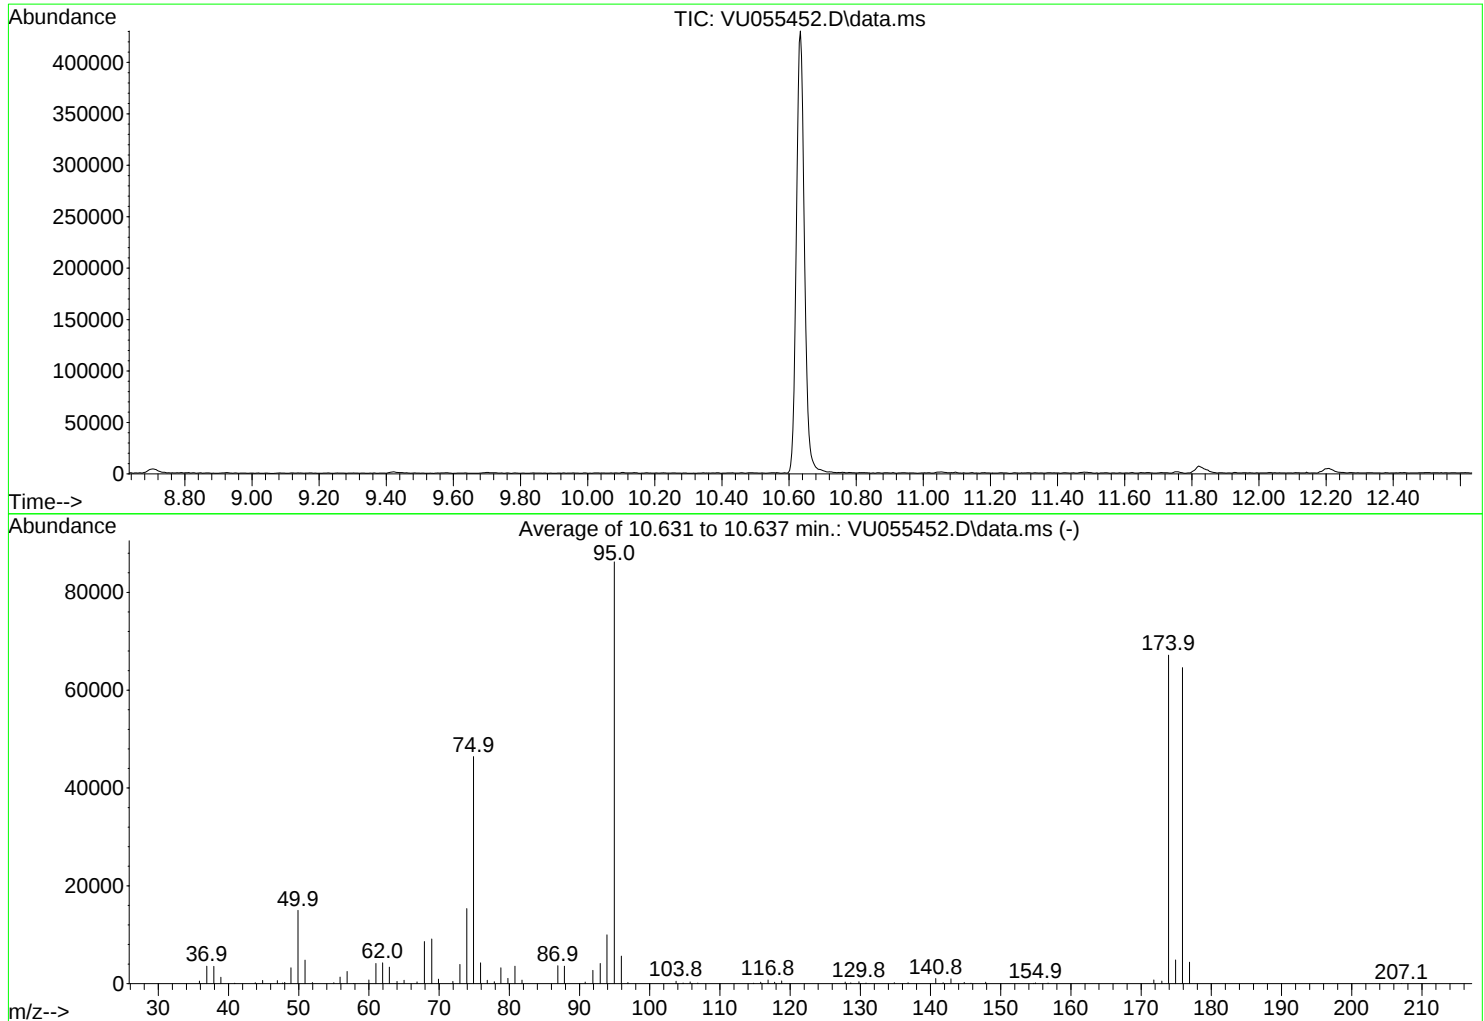

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	14973	PASS
75	95	30	80	53.8	46435	PASS
95	95	100	100	100.0	86245	PASS
96	95	5	9	6.5	5622	PASS
173	174	0.00	2	0.8	525	PASS
174	95	50	120	77.9	67157	PASS
175	174	5	9	7.2	4849	PASS
176	174	95	101	96.2	64600	PASS
177	176	5	9	6.8	4392	PASS

m/z	Abundance
39.80	242.0
43.90	733.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050

m/z	Abundance
35.90	587.0
36.90	3653.0
37.90	3508.0
38.90	1433.0
40.00	255.0
43.80	917.0
44.80	731.0
47.00	616.0
48.00	433.0
48.90	3294.0
49.90	15109.0
50.90	4945.0
52.00	269.0
55.00	218.0
55.90	1314.0
56.90	2531.0
57.80	105.0
60.00	772.0
61.00	4294.0
61.90	4296.0
62.90	3320.0
64.00	493.0
65.00	570.0
66.90	341.0
67.90	8816.0
68.90	9179.0
69.90	778.0
71.90	473.0
73.00	3702.0
74.00	15681.0
74.90	46944.0
75.90	4287.0
76.80	670.0
77.90	370.0
78.80	3267.0
79.80	989.0
80.80	3588.0
81.80	600.0
86.90	3755.0
87.80	3772.0
90.80	318.0
91.90	2676.0
93.00	4080.0
93.90	10180.0
95.00	87008.0
95.90	5572.0
96.90	167.0
103.80	532.0
104.80	116.0
105.80	406.0
106.90	148.0
115.80	276.0
116.90	852.0
117.80	316.0
118.80	589.0
127.80	309.0
128.70	184.0
129.80	424.0
130.90	133.0
134.90	147.0
136.80	187.0
140.80	1007.0
141.80	167.0
142.90	1084.0
144.80	265.0
145.80	102.0
147.80	322.0
155.00	230.0
156.80	141.0
171.80	749.0
172.90	500.0
173.90	66848.0
174.90	4848.0
175.90	62872.0
176.90	4578.0
207.10	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050

m/z	Abundance
35.80	535.0
36.90	3682.0
37.90	3623.0
38.90	1298.0
40.00	217.0
40.90	109.0
43.80	935.0
44.80	674.0
47.00	618.0
48.00	405.0
48.90	3403.0
49.90	15306.0
50.90	4883.0
52.00	249.0
55.00	182.0
55.90	1413.0
56.90	2592.0
60.00	781.0
61.00	4182.0
61.90	4352.0
62.90	3433.0
64.00	466.0
65.00	726.0
66.90	387.0
67.90	8855.0
69.00	9505.0
69.90	950.0
71.90	491.0
73.00	4091.0
74.00	15761.0
74.90	48112.0
75.90	4472.0
76.80	689.0
77.80	397.0
78.80	3277.0
79.80	1131.0
80.80	3645.0
81.80	746.0
86.90	3802.0
87.80	3723.0
90.80	308.0
91.90	2855.0
92.90	4233.0
93.90	10200.0
95.00	88048.0
96.00	5858.0
96.90	256.0
103.80	492.0
104.80	160.0
105.70	386.0
106.90	148.0
114.80	126.0
115.80	287.0
116.90	764.0
117.80	280.0
118.80	584.0
127.80	330.0
128.60	155.0
129.80	435.0
130.80	121.0
134.90	200.0
136.80	209.0
140.70	1095.0
141.80	200.0
142.90	1025.0
144.80	248.0
145.70	118.0
147.80	279.0
154.90	225.0
156.70	150.0
171.80	794.0
173.00	537.0
173.90	69000.0
174.90	4982.0
175.90	66760.0
176.90	4536.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050

m/z	Abundance
35.90	454.0
36.90	3402.0
37.90	3465.0
38.90	1159.0
39.80	181.0
40.90	144.0
43.80	944.0
44.90	566.0
46.90	629.0
47.70	382.0
48.90	3059.0
49.90	14504.0
50.90	4585.0
51.90	176.0
55.00	210.0
55.90	1299.0
56.90	2369.0
60.00	758.0
61.00	3887.0
62.00	4102.0
62.90	3370.0
64.00	381.0
65.00	793.0
66.80	337.0
67.90	8114.0
69.00	8680.0
69.90	994.0
72.00	460.0
72.90	3965.0
73.90	14595.0
74.90	44248.0
75.90	4040.0
76.90	677.0
77.80	420.0
78.80	3141.0
79.80	1111.0
80.80	3430.0
81.80	825.0
86.90	3469.0
87.90	3213.0
90.80	315.0
91.90	2634.0
92.90	4055.0
93.90	9576.0
94.90	83680.0
96.00	5435.0
96.90	267.0
103.70	462.0
104.70	176.0
105.80	335.0
106.80	123.0
114.80	135.0
115.80	307.0
116.80	688.0
117.80	288.0
118.80	527.0
127.90	337.0
128.60	126.0
129.80	334.0
130.70	121.0
134.80	234.0
136.80	194.0
140.70	1010.0
141.80	213.0
142.90	878.0
144.80	252.0
145.70	120.0
147.90	261.0
154.70	228.0
156.70	152.0
171.80	753.0
173.00	539.0
173.90	65624.0
174.90	4717.0
175.90	64168.0
176.90	4063.0

Instrument :
MSVOA_U
ClientSampleId :
BFB050